
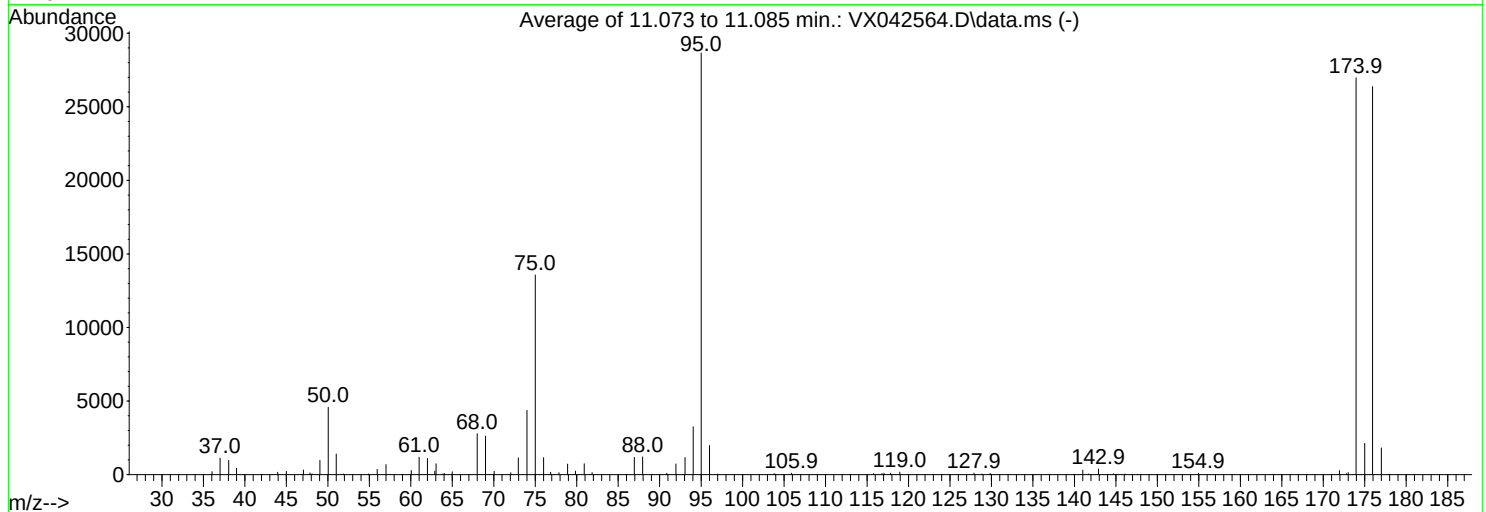


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072724\
Data File : VX042564.D
Acq On : 25 Jul 2024 13:30
Operator : JC/MD
Sample : BFB685
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB685

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Fri Jul 26 15:07:25 2024

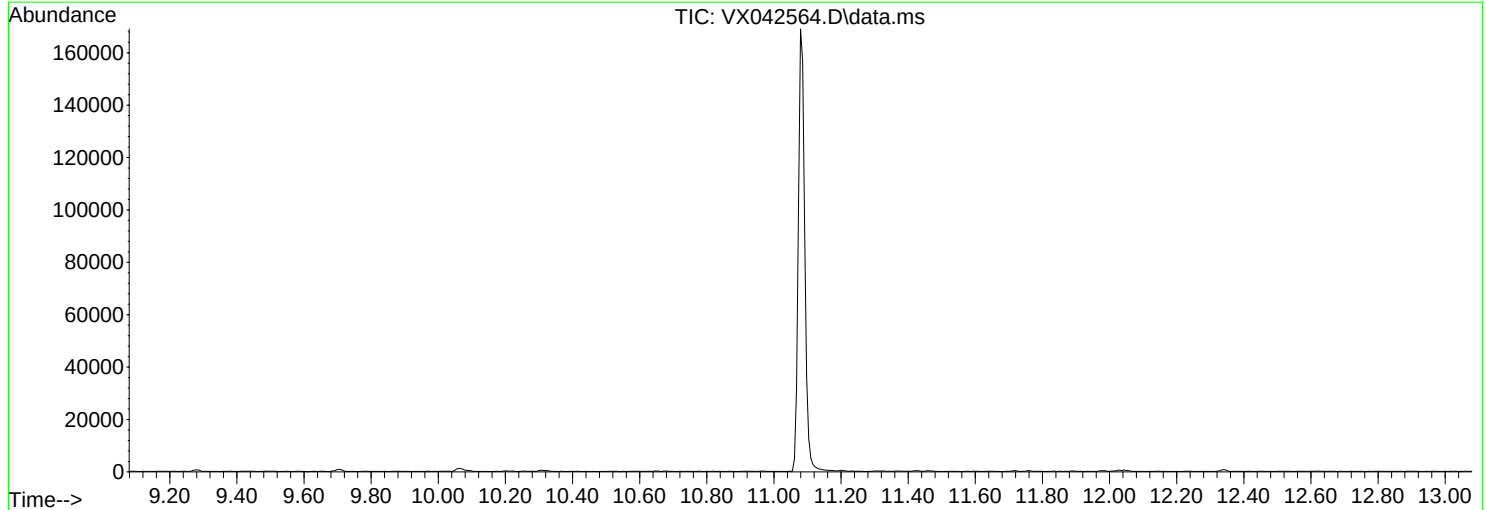

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	4578	PASS
75	95	30	80	47.3	13574	PASS
95	95	100	100	100.0	28669	PASS
96	95	5	9	6.9	1981	PASS
173	174	0.00	2	0.5	146	PASS
174	95	50	120	94.1	26972	PASS
175	174	5	9	7.9	2119	PASS
176	174	95	101	97.8	26377	PASS
177	176	5	9	6.9	1815	PASS

m/z	Abundance
39.90	100.0
43.80	60.0

Instrument :
MSVOA_X
ClientSampleId :
BFB685

m/z	Abundance
36.10	147.0
37.00	933.0
38.00	781.0
39.00	307.0
40.00	110.0
44.00	175.0
45.00	227.0
47.10	273.0
47.80	159.0
49.00	827.0
50.00	3904.0
51.00	1244.0
51.90	66.0
55.90	340.0
57.00	560.0
60.10	212.0
61.00	1112.0
62.00	999.0
62.90	711.0
63.90	149.0
65.00	144.0
68.00	2398.0
69.00	2080.0
70.00	140.0
72.10	99.0
72.90	896.0
74.00	3516.0
75.00	10548.0
76.00	988.0
76.80	147.0
77.90	106.0
78.90	594.0
79.90	188.0
80.90	607.0
81.90	101.0
87.00	1038.0
88.00	821.0
90.90	85.0
91.90	599.0
93.10	824.0
94.00	2466.0
95.00	21192.0
96.00	1458.0
103.80	68.0
105.90	62.0
116.00	59.0
117.10	108.0
117.90	58.0
119.00	165.0
128.00	102.0
129.90	69.0
141.10	231.0
142.90	318.0
148.00	60.0
155.00	67.0
172.00	180.0
172.80	190.0
174.00	16244.0
175.00	1335.0
176.00	15322.0
177.00	1186.0

Instrument :
MSVOA_X
ClientSampleId :
BFB685

m/z	Abundance
36.10	265.0
37.00	1319.0
38.10	1233.0
39.00	595.0
39.90	146.0
44.00	246.0
45.10	260.0
47.00	413.0
47.90	203.0
49.10	1129.0
50.10	5552.0
51.00	1617.0
51.90	62.0
54.90	69.0
56.00	391.0
57.00	818.0
60.00	352.0
61.00	1294.0
62.00	1260.0
63.10	1200.0
64.10	124.0
65.00	247.0
68.00	3035.0
69.00	2998.0
70.10	294.0
72.10	153.0
73.00	1362.0
74.00	5315.0
75.00	16008.0
76.00	1353.0
76.90	174.0
77.80	183.0
78.90	801.0
79.90	296.0
80.90	822.0
81.80	222.0
86.90	1389.0
88.00	1591.0
90.90	91.0
92.00	889.0
93.00	1365.0
94.00	3853.0
95.00	34392.0
96.00	2316.0
97.00	67.0
104.00	106.0
105.90	91.0
115.80	102.0
117.00	172.0
117.80	152.0
119.00	239.0
127.90	114.0
128.90	66.0
129.90	133.0
140.90	332.0
141.70	64.0
142.90	443.0
144.70	112.0
146.10	56.0
147.60	55.0
154.90	106.0
171.90	330.0
173.00	437.0
173.90	31968.0
175.00	2419.0
175.90	31616.0
177.00	2123.0
177.90	66.0

Instrument :
MSVOA_X
ClientSampleId :
BFB685

m/z	Abundance
35.90	211.0
37.00	1118.0
38.10	891.0
39.00	390.0
40.00	137.0
44.00	251.0
44.90	209.0
47.00	270.0
48.10	166.0
49.00	939.0
50.00	4277.0
51.00	1361.0
54.90	56.0
56.00	352.0
57.00	681.0
60.00	290.0
61.00	1150.0
62.00	1045.0
63.00	1017.0
64.00	97.0
65.00	185.0
68.00	2916.0
69.00	2790.0
70.00	248.0
72.00	157.0
73.00	1172.0
74.00	4298.0
75.00	14167.0
76.00	1118.0
76.80	165.0
77.80	108.0
78.90	765.0
79.80	227.0
80.90	791.0
81.90	112.0
86.90	1108.0
87.90	1207.0
90.80	118.0
92.00	704.0
93.00	1295.0
94.10	3443.0
95.00	30424.0
96.00	2168.0
97.00	60.0
103.80	116.0
105.90	128.0
115.70	79.0
116.80	222.0
117.90	100.0
118.80	129.0
127.80	97.0
128.80	60.0
129.70	72.0
130.90	71.0
141.00	350.0
141.70	65.0
142.90	370.0
144.70	79.0
146.10	67.0
154.90	107.0
161.00	54.0
172.00	295.0
173.90	32704.0
175.00	2602.0
176.00	32192.0
177.00	2136.0

Instrument :
MSVOA_X
ClientSampleId :
BFB685