


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072820\
Data File : VX017643.D
Acq On : 28 Jul 2020 09:55
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Title : SW846 8260
Last Update : Fri Jul 24 05:48:09 2020

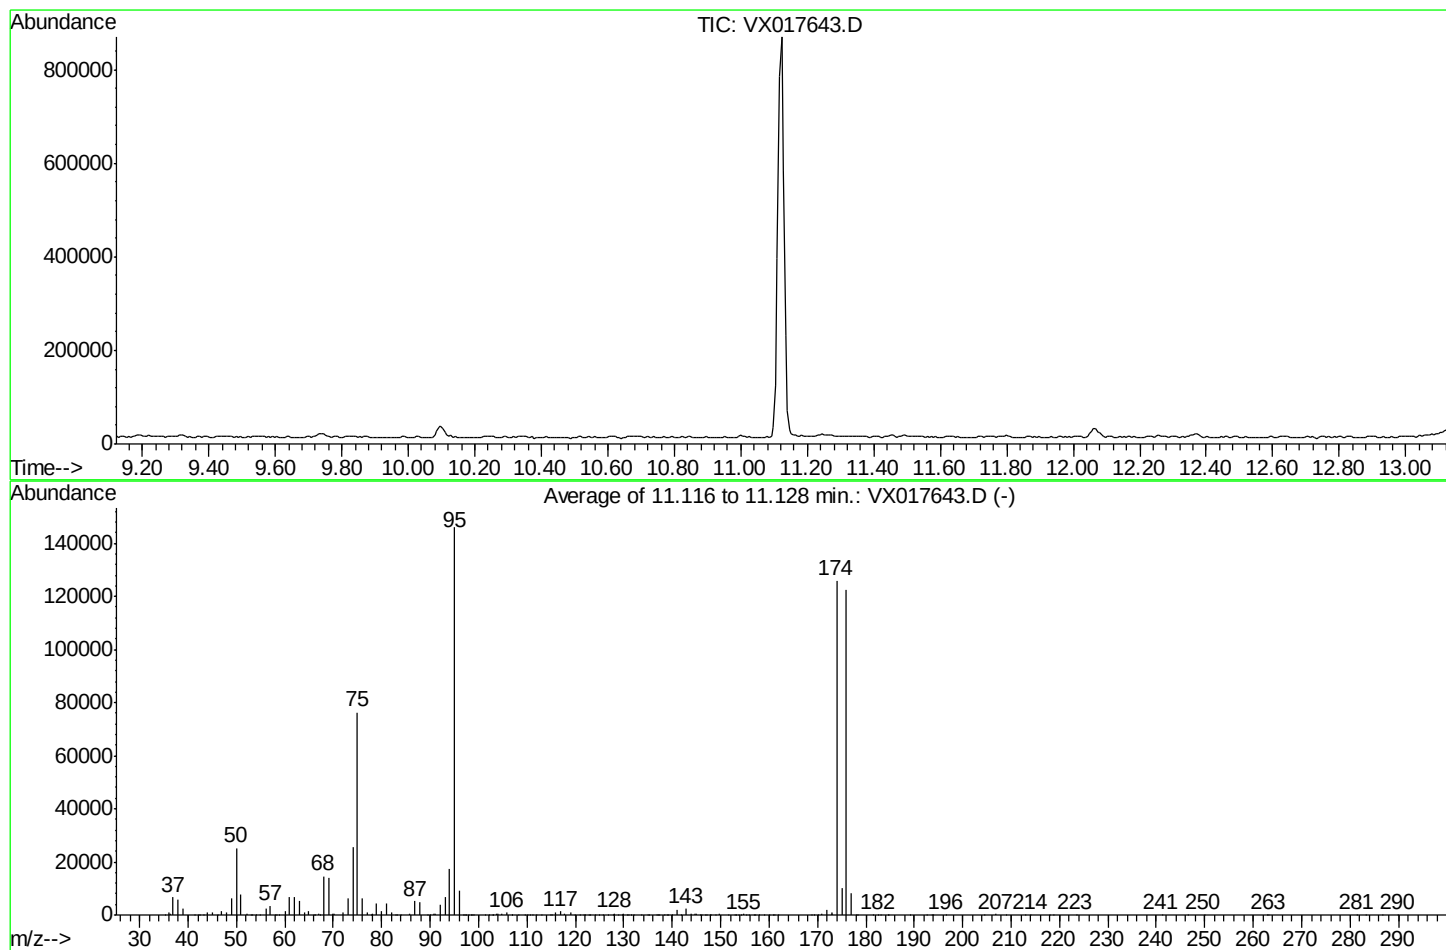

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	25124	PASS
75	95	30	60	52.3	76314	PASS
95	95	100	100	100.0	146024	PASS
96	95	5	9	6.4	9364	PASS
173	174	0.00	2	0.8	1035	PASS
174	95	50	100	86.3	126016	PASS
175	174	5	9	8.0	10080	PASS
176	174	95	101	97.3	122613	PASS
177	176	5	9	6.6	8142	PASS