

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
 Data File : VX030278.D
 Acq On : 28 Jul 2022 18:32
 Operator : JC/MD
 Sample : N3773-16MEDL 10X
 Misc : 5.73g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DL-3(5-5.5)ME

Quant Time: Jul 29 05:59:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 25 16:49:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	147213	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	257433	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	262024	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	155970	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	158809	53.672	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 107.340%			
35) Dibromofluoromethane	5.391	113	127165	51.674	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.340%			
50) Toluene-d8	8.653	98	487344	51.136	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.280%			
62) 4-Bromofluorobenzene	11.085	95	180656	51.077	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 102.160%			
Target Compounds						Qvalue
5) Bromomethane	1.593	94	630	Below Cal	#	69
10) Methyl Iodide	2.447	142	373	1.683	ug/l #	63
11) Tert butyl alcohol	2.947	59	23879	33.084	ug/l #	80
13) Acrolein	2.233	56	58	0.327	ug/l #	14
16) Acetone	2.392	43	2242	1.480	ug/l #	85
18) Methyl Acetate	2.782	43	6142	1.371	ug/l #	51
20) Methylene Chloride	2.788	84	2537	Below Cal		94
25) 2-Butanone	4.574	43	4233	1.663	ug/l	93
31) Cyclohexane	5.501	56	8665	2.017	ug/l #	57
36) 1,1-Dichloropropene	5.556	75	12846	3.627	ug/l #	48
38) Carbon Tetrachloride	5.550	117	14978	4.530	ug/l #	17
39) Methylcyclohexane	7.391	83	10118	2.213	ug/l	95
51) 4-Methyl-2-Pentanone	8.623	43	3126	0.626	ug/l #	36
55) 1,1,2-Trichloroethane	9.110	97	2501	0.864	ug/l #	21
67) Ethyl Benzene	10.201	91	17043	Below Cal		100
68) m/p-Xylenes	10.305	106	8535	1.770	ug/l	92
73) Isopropylbenzene	10.964	105	4341	0.357	ug/l	95
74) N-amyl acetate	10.860	43	1277	0.216	ug/l #	36
76) 1,2,3-Trichloropropane	11.085	75	89644	21.804	ug/l #	38
78) n-propylbenzene	11.311	91	20233	1.392	ug/l	99
79) 2-Chlorotoluene	11.403	91	3224	0.351	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.457	105	24337	2.387	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	89644	65.412	ug/l #	13
82) 4-Chlorotoluene	11.457	91	2962	0.295	ug/l #	48
83) tert-Butylbenzene	11.976	119	2697	0.285	ug/l	71
84) 1,2,4-Trimethylbenzene	11.756	105	45038	4.428	ug/l	99
85) sec-Butylbenzene	11.896	105	2912	0.225	ug/l #	56
86) p-Isopropyltoluene	11.976	119	2697	0.261	ug/l	91
89) n-Butylbenzene	12.329	91	10002	1.038	ug/l #	33
90) Hexachloroethane	12.530	117	967	0.543	ug/l #	16
95) Naphthalene	13.780	128	16233	1.314	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
Data File : VX030278.D
Acq On : 28 Jul 2022 18:32
Operator : JC/MD
Sample : N3773-16MEDL 10X
Misc : 5.73g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME

Quant Time: Jul 29 05:59:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 25 16:49:17 2022
Response via : Initial Calibration




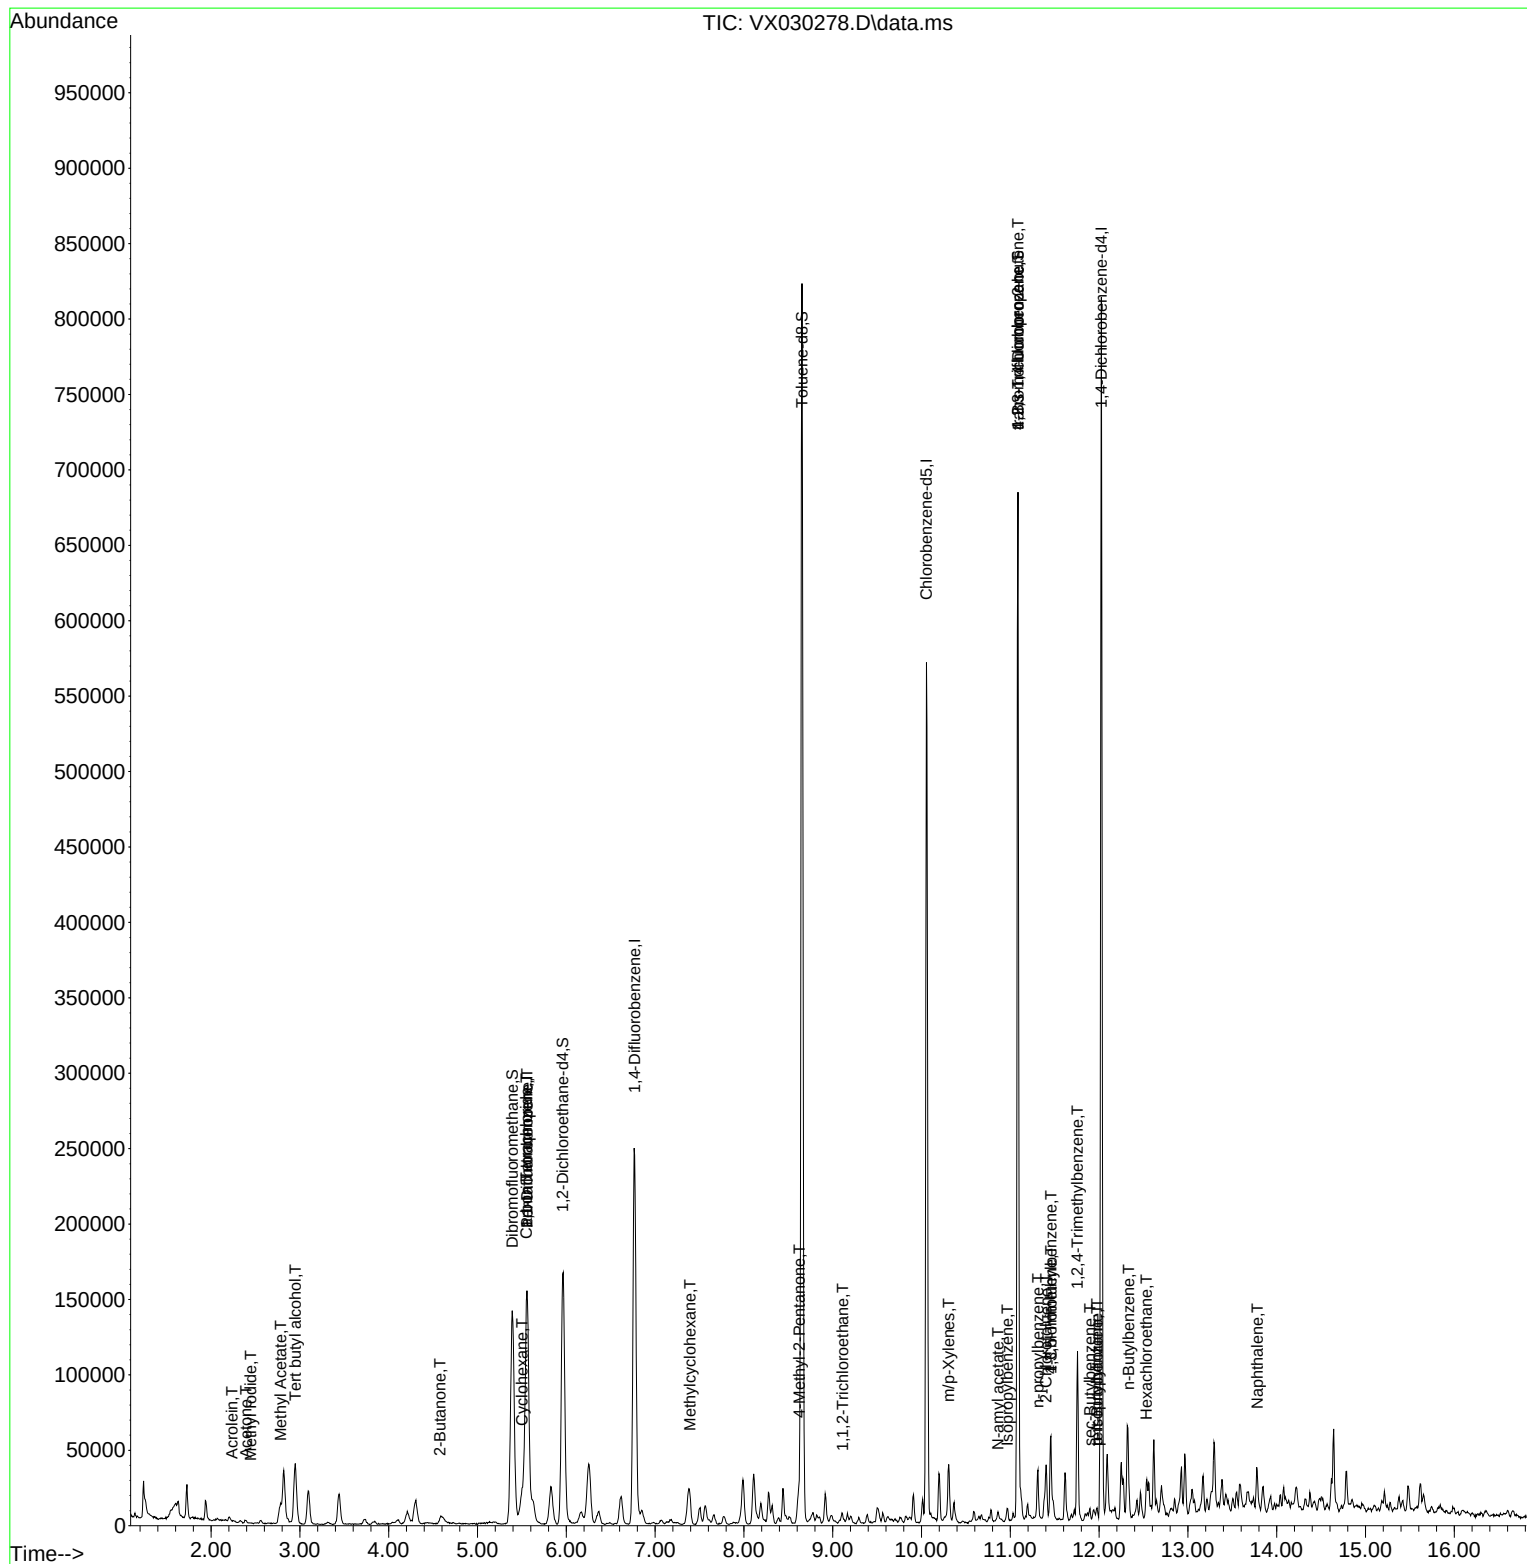




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:168 Resp: 147213
Ion Ratio Lower Upper
168 100
99 59.3 44.0 66.0



#5
Bromomethane
Concen: Below Cal
RT: 1.593 min Scan# 83
Delta R.T. -0.006 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 94 Resp: 630
Ion Ratio Lower Upper
94 100
96 66.1 76.9 115.3#




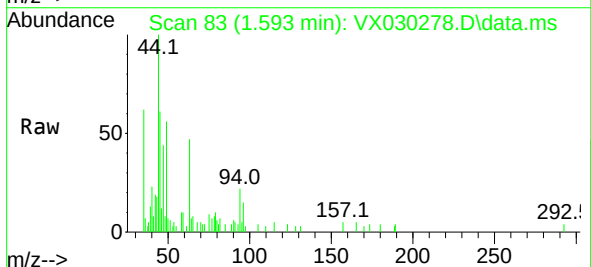




#10
Methyl Iodide
Concen: 1.683 ug/l
RT: 2.447 min Scan# 21
Delta R.T. 0.001 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:142 Resp: 373
Ion Ratio Lower Upper
142 100
127 15.3 30.2 45.2#
141 0.0 11.3 16.9#

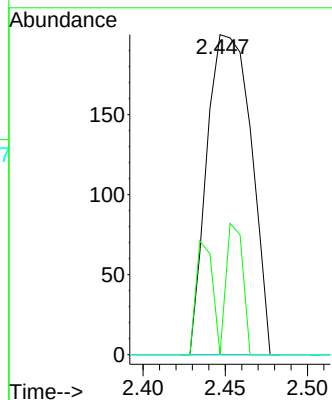

#11
Tert butyl alcohol
Concen: 33.084 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.030 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32


Tgt Ion: 59 Resp: 23879
Ion Ratio Lower Upper
59 100
57 1.9 7.4 11.2#

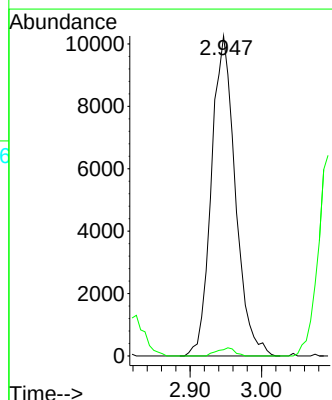






#13
Acrolein
Concen: 0.327 ug/l
RT: 2.233 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME







Tgt Ion: 56 Resp: 58
Ion Ratio Lower Upper
56 100
55 0.0 56.6 84.8#

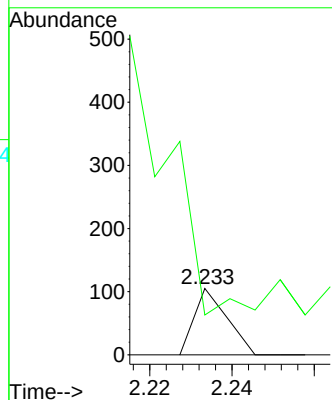

#16
Acetone
Concen: 1.480 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.007 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 43 Resp: 2242
Ion Ratio Lower Upper
43 100
58 26.0 27.7 41.5#


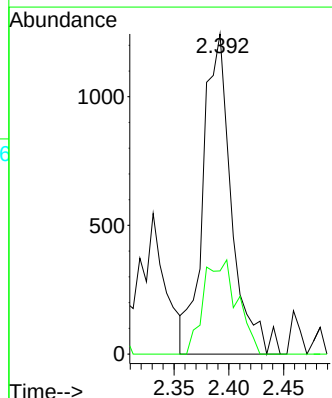

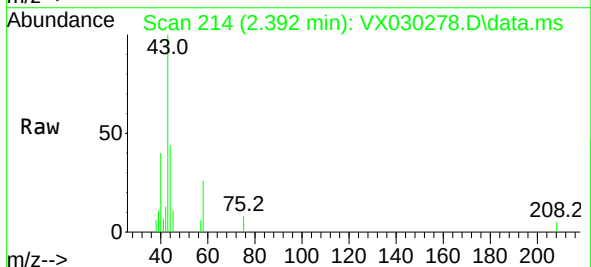




#18
Methyl Acetate
Concen: 1.371 ug/l
RT: 2.782 min Scan# 219
Delta R.T. 0.074 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion: 43 Resp: 6142
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.2#

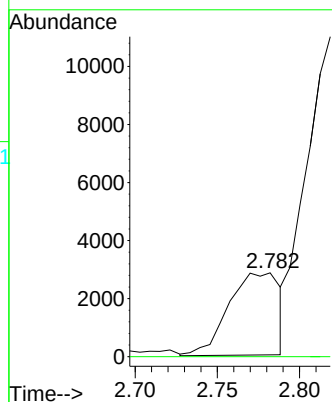

#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 84 Resp: 2537
Ion Ratio Lower Upper
84 100
49 123.7 93.8 140.6
51 39.9 29.4 44.0
86 57.8 51.0 76.4

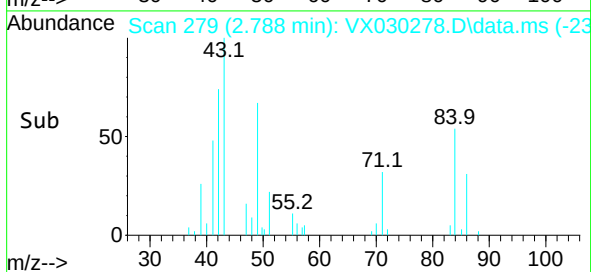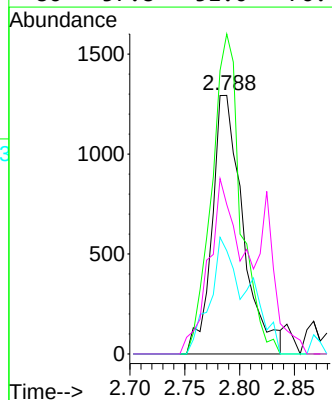

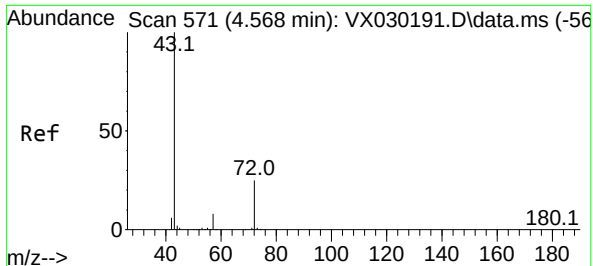

#25

2-Butanone

Concen: 1.663 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX030278.D


Acq: 28 Jul 2022 18:32

Instrument :

MSVOA_X

ClientSampleId :

DL-3(5-5.5)ME



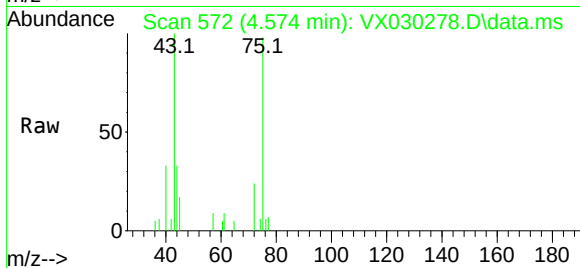


Tgt Ion: 43 Resp: 4233

Ion Ratio Lower Upper

43 100

72 23.5 21.7 32.5

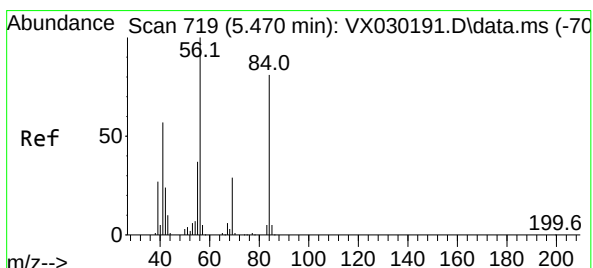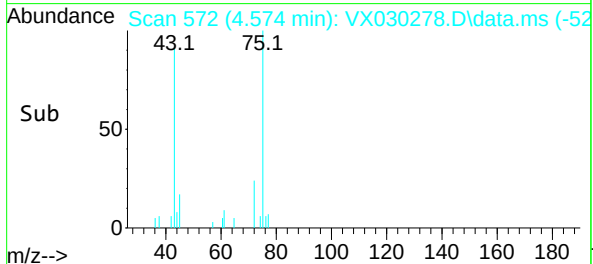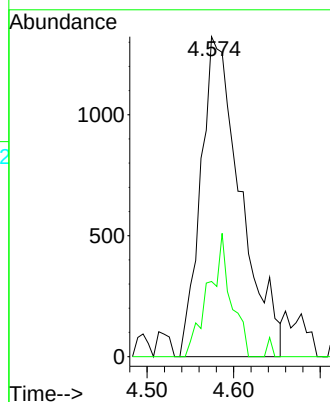

#31

Cyclohexane

Concen: 2.017 ug/l

RT: 5.501 min Scan# 724

Delta R.T. 0.031 min

Lab File: VX030278.D

Acq: 28 Jul 2022 18:32




Tgt Ion: 56 Resp: 8665


Ion Ratio Lower Upper

56 100

69 20.3 25.4 38.0#

84 39.2 68.9 103.3#

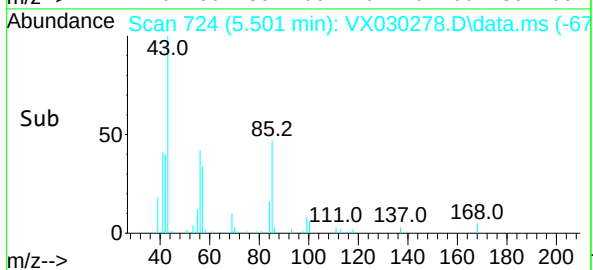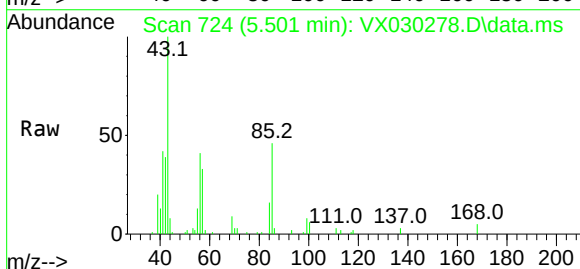



#33

1,2-Dichloroethane-d4

Concen: 53.672 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX030278.D

Acq: 28 Jul 2022 18:32

Instrument :

MSVOA_X

ClientSampleId :





DL-3(5-5.5)ME

Tgt Ion: 65 Resp: 158809

Ion Ratio Lower Upper

65 100

67 55.0 0.0 109.6

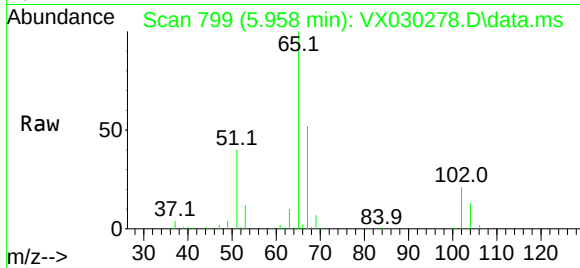

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX030278.D

Acq: 28 Jul 2022 18:32




Tgt Ion: 114 Resp: 257433


Ion Ratio Lower Upper

114 100

63 21.0 0.0 38.4


88 16.1 0.0 31.8

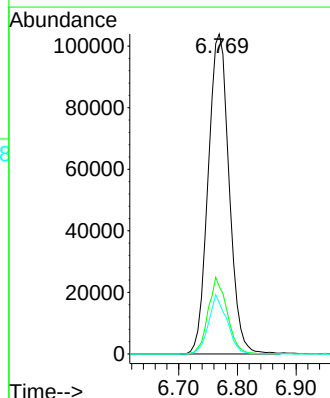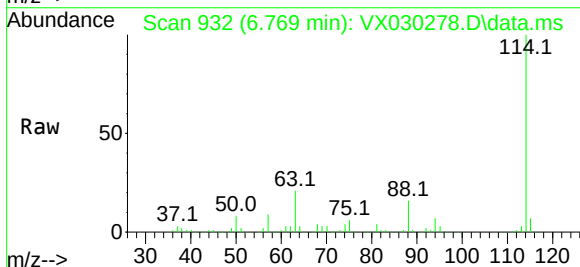






#35
Dibromofluoromethane
Concen: 51.674 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32


Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME

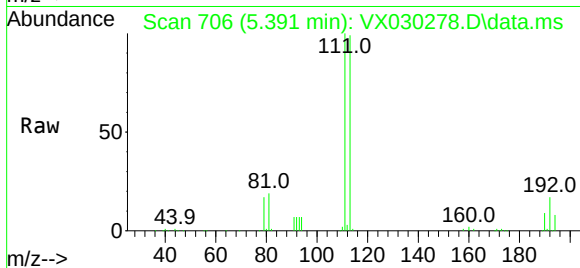



Tgt Ion:113 Resp: 127165
Ion Ratio Lower Upper
113 100
111 101.5 83.2 124.8
192 17.8 14.8 22.2




#36
1,1-Dichloropropene
Concen: 3.627 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

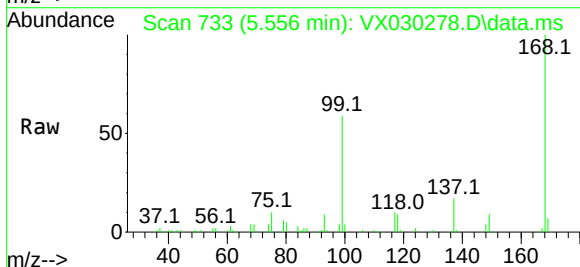

Tgt Ion: 75 Resp: 12846
Ion Ratio Lower Upper
75 100
110 8.5 19.3 57.9#
77 0.0 24.4 36.6#



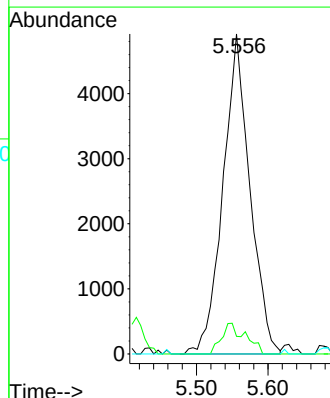





#38
Carbon Tetrachloride
Concen: 4.530 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.133 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:117 Resp: 14978
Ion Ratio Lower Upper
117 100
119 5.1 74.1 111.1#
121 0.0 25.8 38.8#

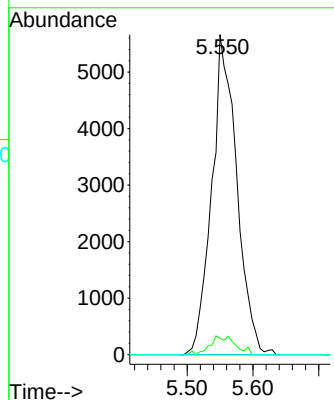

#39
Methylcyclohexane
Concen: 2.213 ug/l
RT: 7.391 min Scan# 1034
Delta R.T. 0.007 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 83 Resp: 10118
Ion Ratio Lower Upper
83 100
55 73.3 57.7 86.5
98 38.3 36.5 54.7

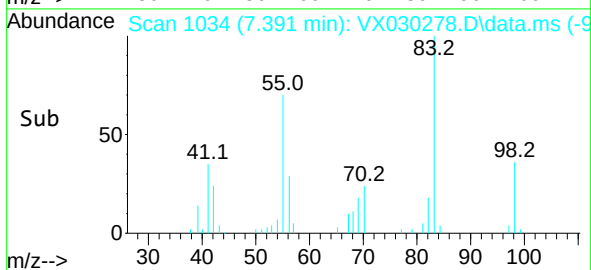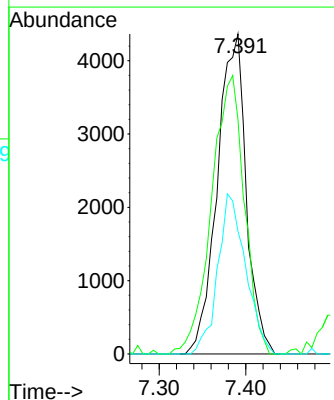



#50

Toluene-d8

Concen: 51.136 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.001 min

Lab File: VX030278.D

Acq: 28 Jul 2022 18:32

Instrument :

MSVOA_X

ClientSampleId :





DL-3(5-5.5)ME

Tgt Ion: 98 Resp: 487344

Ion Ratio Lower Upper

98 100

100 64.8 52.3 78.5



#51

4-Methyl-2-Pentanone

Concen: 0.626 ug/l

RT: 8.623 min Scan# 1236

Delta R.T. 0.043 min

Lab File: VX030278.D




Acq: 28 Jul 2022 18:32


Tgt Ion: 43 Resp: 3126

Ion Ratio Lower Upper

43 100

58 0.0 31.4 47.2#


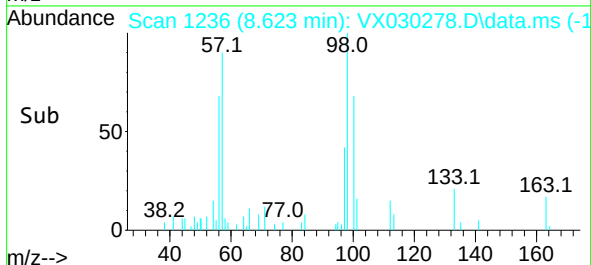

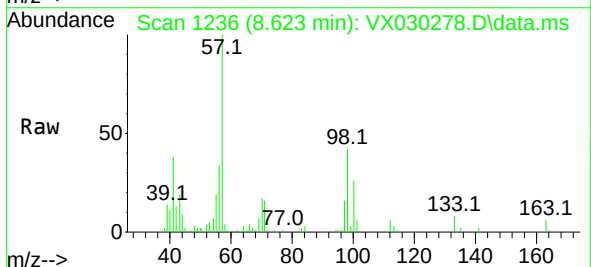




#55
1,1,2-Trichloroethane
Concen: 0.864 ug/l
RT: 9.110 min Scan# 11
Delta R.T. -0.048 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion: 97	Resp: 2501
Ion Ratio	Lower Upper
97 100	
83 8.3	68.9 103.3#
85 3.5	44.0 66.0#
99 0.0	48.3 72.5#



#62
4-Bromofluorobenzene
Concen: 51.077 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 95	Resp: 180656
Ion Ratio	Lower Upper
95 100	
174 71.6	0.0 149.0
176 68.5	0.0 146.0


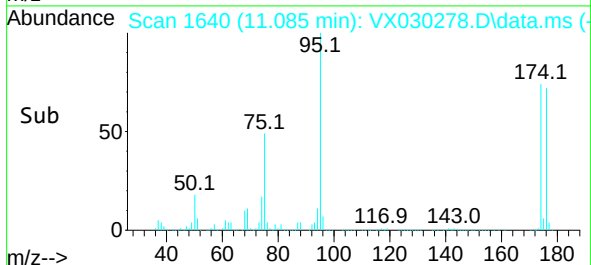

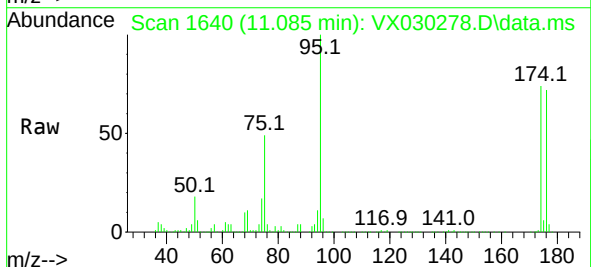




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:117 Resp: 262024
Ion Ratio Lower Upper
117 100
82 57.5 42.7 64.1
119 31.7 25.4 38.2

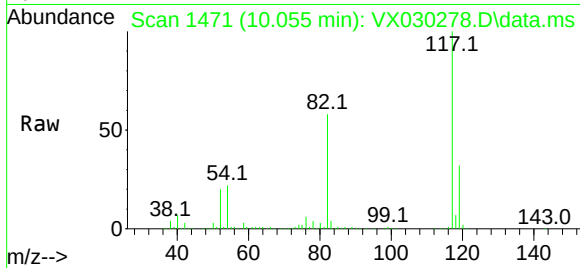

#67
Ethyl Benzene
Concen: Below Cal
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 91 Resp: 17043
Ion Ratio Lower Upper
91 100
106 32.1 25.5 38.3




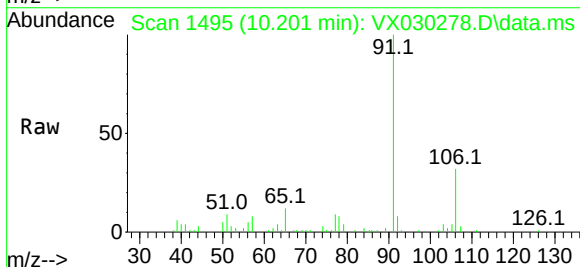


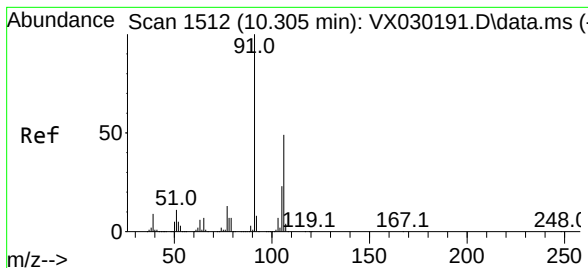

#68
m/p-Xylenes
Concen: 1.770 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:106 Resp: 8535
Ion Ratio Lower Upper
106 100
91 209.8 158.2 237.4

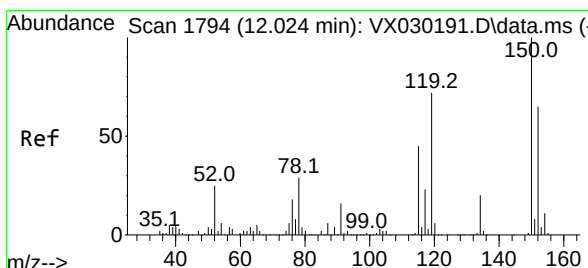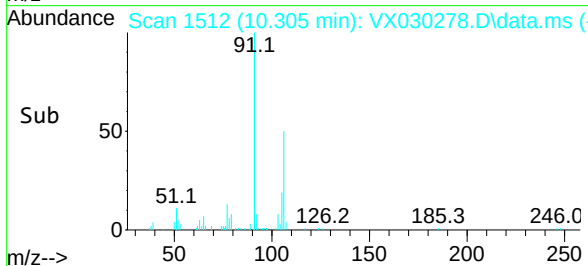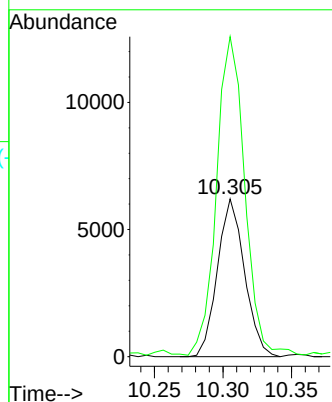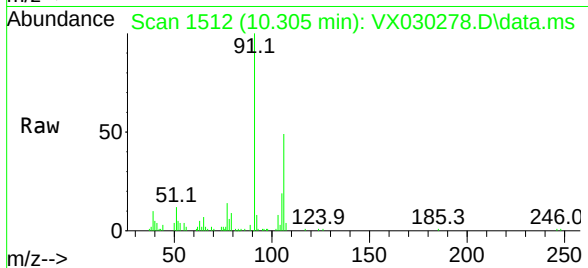

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion:152 Resp: 155970
Ion Ratio Lower Upper
152 100
115 61.7 40.5 121.5
150 158.4 0.0 347.0


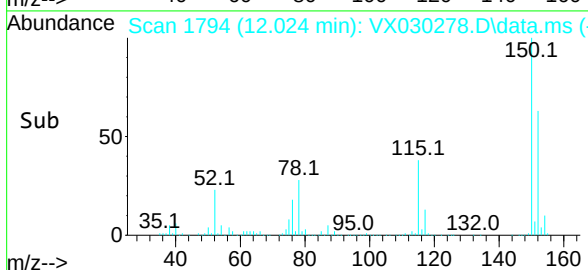
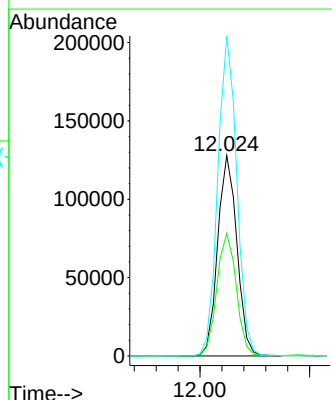
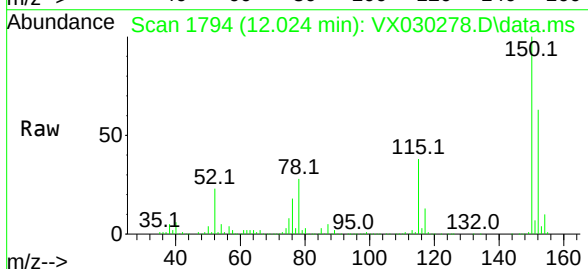




#73
Isopropylbenzene
Concen: 0.357 ug/l
RT: 10.964 min Scan# 1603
Delta R.T. 0.001 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:105 Resp: 4341
Ion Ratio Lower Upper
105 100
120 29.5 13.5 40.4

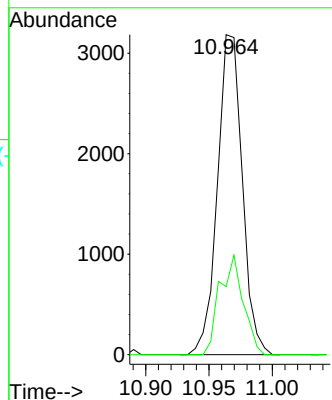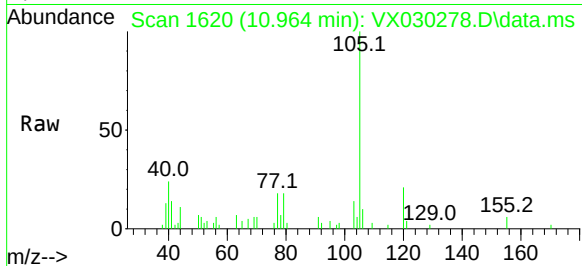

#74
N-ethyl acetate
Concen: 0.216 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.013 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 43 Resp: 1277
Ion Ratio Lower Upper
43 100
70 51.4 32.3 48.5#
55 101.3 18.4 27.6#
61 0.0 19.2 28.8#

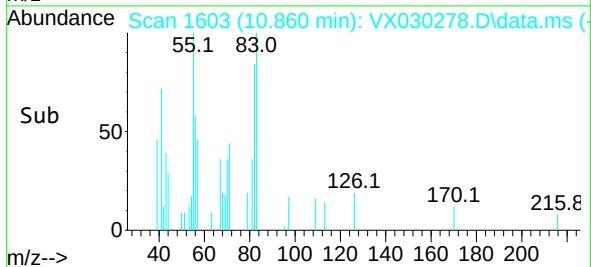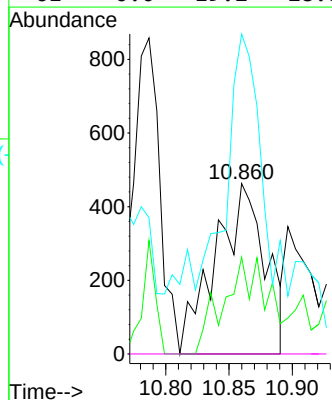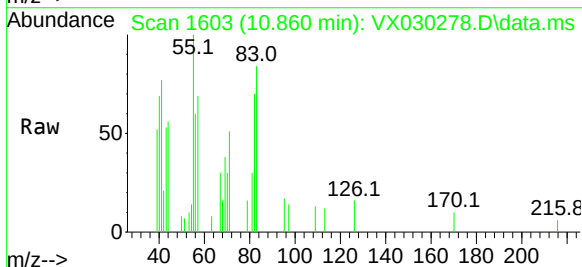



#76

1,2,3-Trichloropropane

Concen: 21.804 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.158 min

Lab File: VX030278.D

Acq: 28 Jul 2022 18:32

Instrument :

MSVOA_X

ClientSampleId :





DL-3(5-5.5)ME

Tgt Ion: 75 Resp: 89644

Ion Ratio Lower Upper

75 100

77 1.6 19.8 59.3#

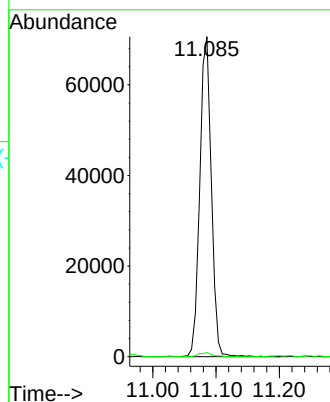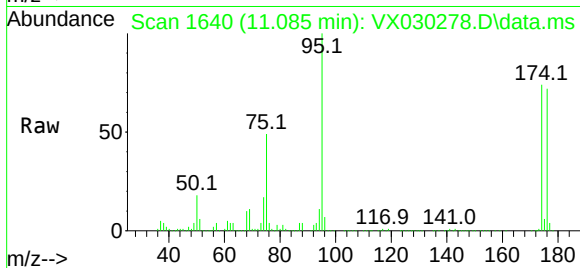

#78

n-propylbenzene

Concen: 1.392 ug/l

RT: 11.311 min Scan# 1677

Delta R.T. 0.001 min

Lab File: VX030278.D




Acq: 28 Jul 2022 18:32


Tgt Ion: 91 Resp: 20233

Ion Ratio Lower Upper

91 100

120 23.5 11.6 34.8

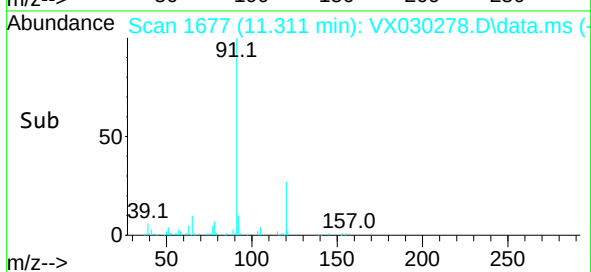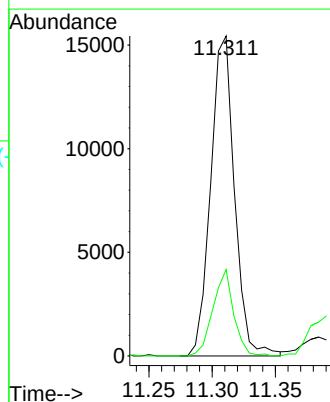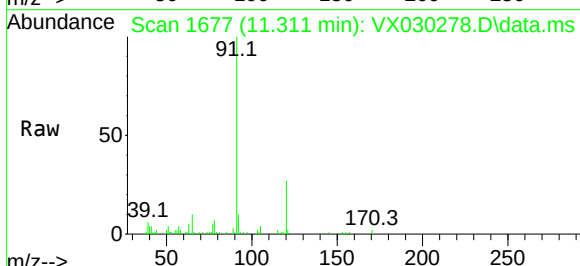



#79

2-Chlorotoluene

Concen: 0.351 ug/l

RT: 11.403 min Scan# 1

Delta R.T. 0.037 min

Lab File: VX030278.D

Acq: 28 Jul 2022 18:32

Instrument :

MSVOA_X

ClientSampleId :





DL-3(5-5.5)ME

Tgt Ion: 91 Resp: 3224

Ion Ratio Lower Upper

91 100

126 0.0 17.4 52.3#

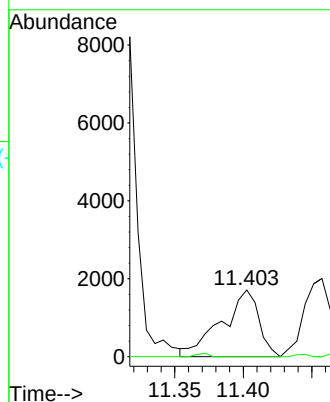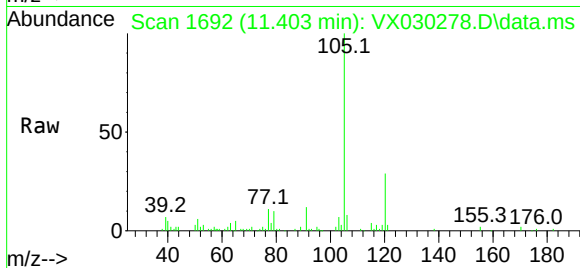

#80

1,3,5-Trimethylbenzene

Concen: 2.387 ug/l

RT: 11.457 min Scan# 1701

Delta R.T. 0.000 min

Lab File: VX030278.D




Acq: 28 Jul 2022 18:32


Tgt Ion: 105 Resp: 24337

Ion Ratio Lower Upper

105 100

120 48.4 24.4 73.2


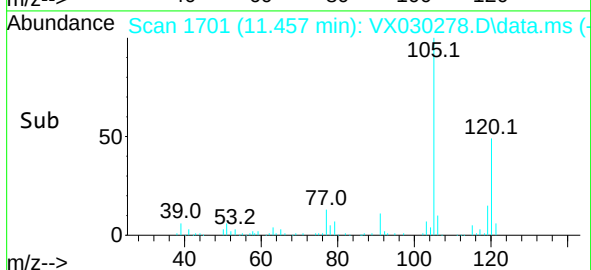

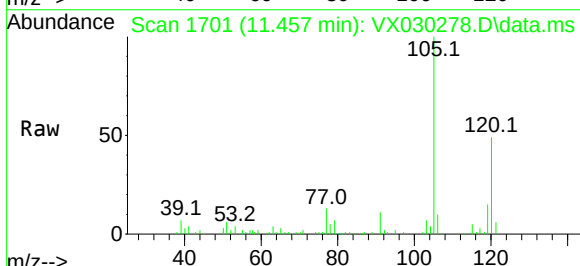




#81
trans-1,4-Dichloro-2-butene
Concen: 65.412 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion: 75 Resp: 89644
Ion Ratio Lower Upper
75 100
53 0.2 74.2 111.4#
89 0.0 34.8 52.2#

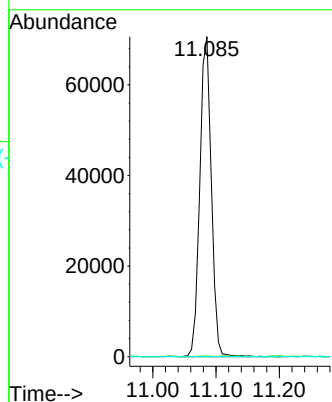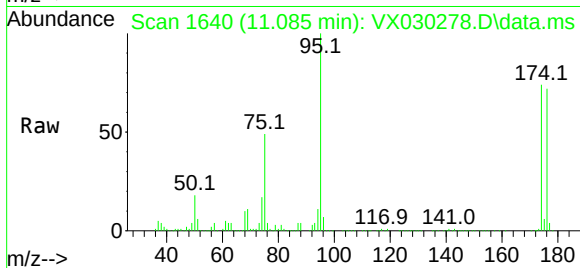

#82
4-Chlorotoluene
Concen: 0.295 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 91 Resp: 2962
Ion Ratio Lower Upper
91 100
126 1.9 15.3 45.9#


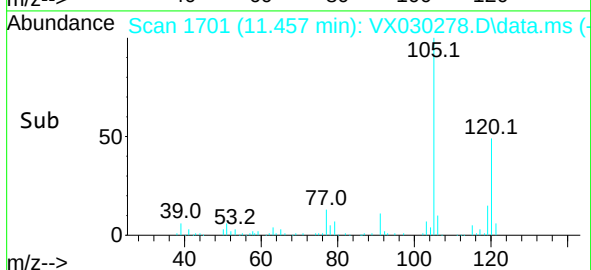
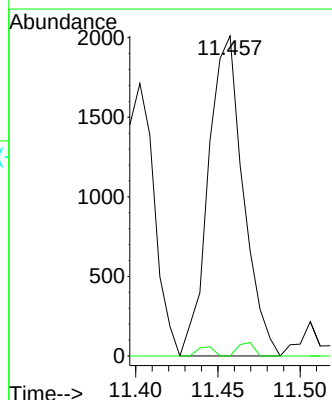
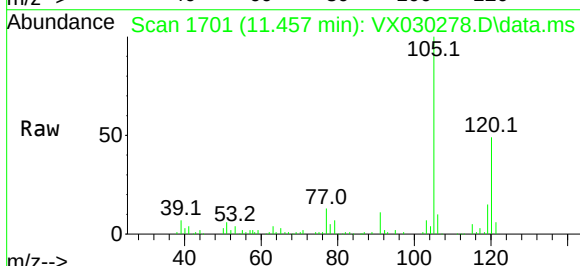




#83
tert-Butylbenzene
Concen: 0.285 ug/l
RT: 11.976 min Scan# 119
Delta R.T. 0.257 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion:119 Resp: 2697
Ion Ratio Lower Upper
119 100
91 31.0 28.3 84.9
134 29.8 11.2 33.5

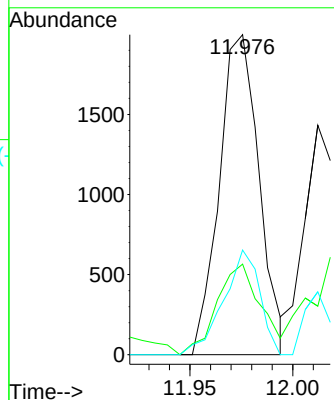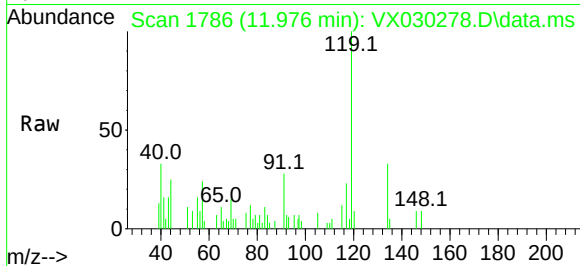

#84
1,2,4-Trimethylbenzene
Concen: 4.428 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion:105 Resp: 45038
Ion Ratio Lower Upper
105 100
120 46.7 22.9 68.8


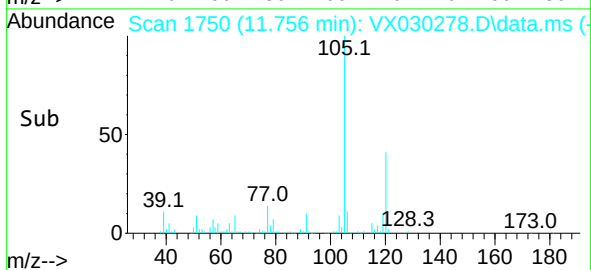
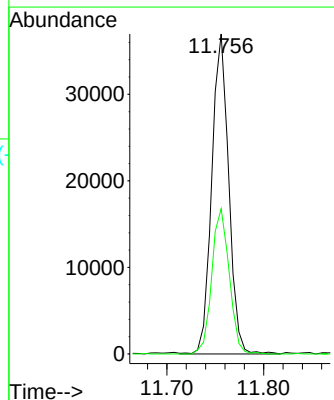
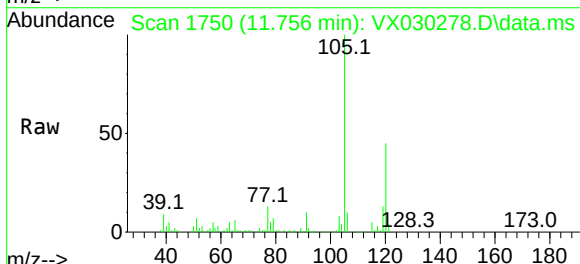




#85
 sec-Butylbenzene
 Concen: 0.225 ug/l
 RT: 11.896 min Scan# 1773
 Delta R.T. 0.000 min
 Lab File: VX030278.D
 Acq: 28 Jul 2022 18:32




Instrument :
 MSVOA_X
 ClientSampleId :
 DL-3(5-5.5)ME


Tgt Ion:105 Resp: 2912
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#

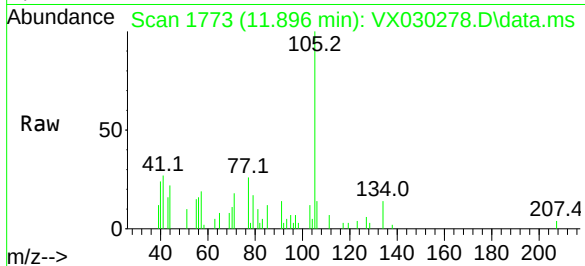

#86
 p-Isopropyltoluene
 Concen: 0.261 ug/l
 RT: 11.976 min Scan# 1786
 Delta R.T. -0.036 min
 Lab File: VX030278.D
 Acq: 28 Jul 2022 18:32

Tgt Ion:119 Resp: 2697
 Ion Ratio Lower Upper
 119 100
 134 29.8 13.9 41.6
 91 31.0 11.8 35.3


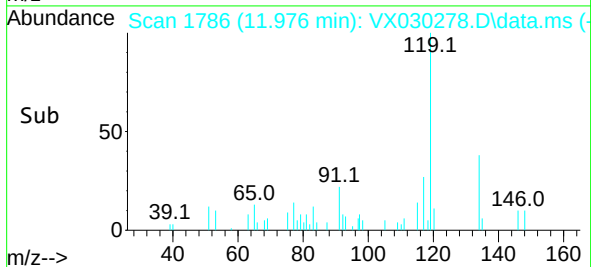

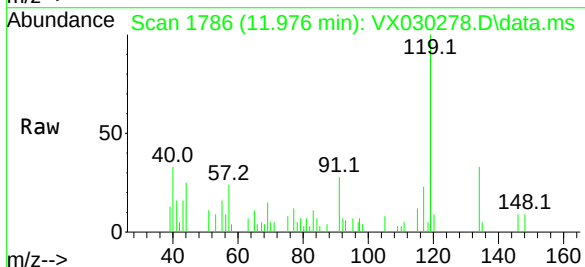




#89
n-Butylbenzene
Concen: 1.038 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32




Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME


Tgt Ion: 91 Resp: 10002
Ion Ratio Lower Upper
91 100
92 33.5 26.2 78.5
134 100.6 12.6 37.8#

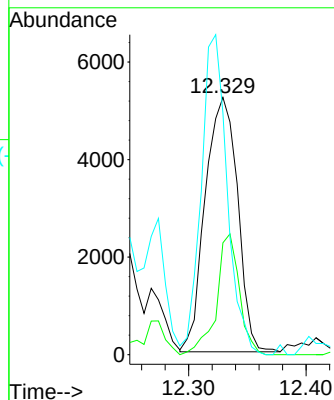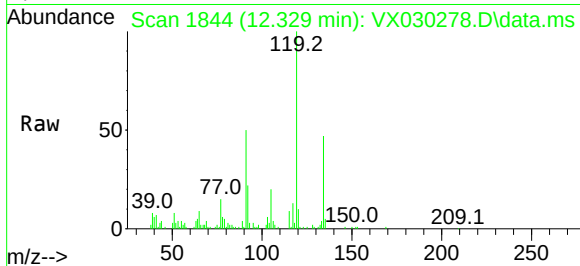

#90
Hexachloroethane
Concen: 0.543 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Tgt Ion: 117 Resp: 967
Ion Ratio Lower Upper
117 100
201 0.0 34.2 102.5#

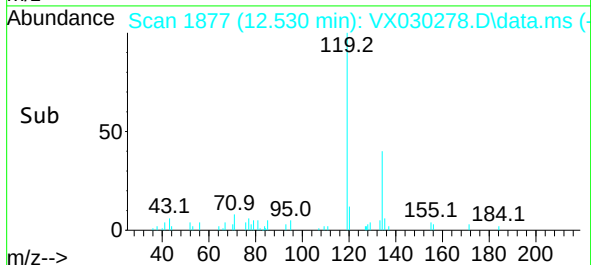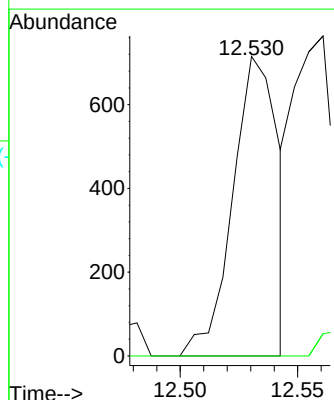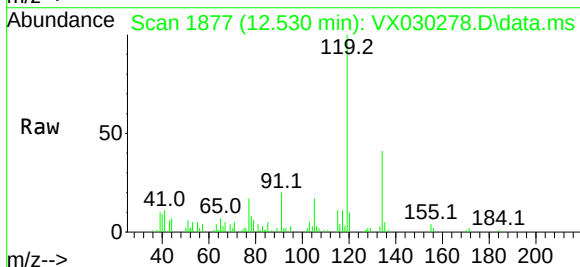



#95
Naphthalene
Concen: 1.314 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX030278.D
Acq: 28 Jul 2022 18:32

Instrument :
MSVOA_X
ClientSampleId :
DL-3(5-5.5)ME

Tgt Ion:128 Resp: 16233
Ion Ratio Lower Upper
128 100
127 12.6 10.2 15.2
129 14.2 8.6 13.0#

