

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
 Data File : VX030280.D
 Acq On : 28 Jul 2022 19:19
 Operator : JC/MD
 Sample : N3914-01MEDL 10X
 Misc : 7.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 METRO-DISPME

Quant Time: Jul 29 05:59:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 25 16:49:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	145032	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	256564	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	263564	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	172169	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	152707	52.386	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 104.780%			
35) Dibromofluoromethane	5.391	113	121714	49.626	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.260%			
50) Toluene-d8	8.653	98	475085	50.019	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 100.040%			
62) 4-Bromofluorobenzene	11.085	95	188349	53.432	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 106.860%			
Target Compounds					Qvalue	
5) Bromomethane	1.611	94	471	Below Cal	#	56
10) Methyl Iodide	2.459	142	202	1.612	ug/l #	45
11) Tert butyl alcohol	2.941	59	30202	42.474	ug/l #	79
13) Acrolein	2.245	56	58	0.332	ug/l #	1
16) Acetone	2.386	43	2642	1.770	ug/l	92
17) Carbon Disulfide	2.502	76	1437	0.235	ug/l #	74
18) Methyl Acetate	2.715	43	1325	0.300	ug/l	92
20) Methylene Chloride	2.788	84	2715	Below Cal		97
25) 2-Butanone	4.593	43	1942	0.774	ug/l #	71
31) Cyclohexane	5.556	56	3406	0.805	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	12303	3.486	ug/l #	48
38) Carbon Tetrachloride	5.562	117	14848	4.506	ug/l #	18
40) Benzene	6.044	78	14758	1.329	ug/l	99
49) 1,4-Dioxane	7.470	88	20	0.240	ug/l #	1
52) Toluene	8.726	92	3666	0.541	ug/l	97
67) Ethyl Benzene	10.195	91	378623	32.347	ug/l	98
68) m/p-Xylenes	10.305	106	40879	8.429	ug/l	95
69) o-Xylene	10.646	106	89661	18.757	ug/l	93
70) Styrene	10.646	104	5696	0.725	ug/l #	1
73) Isopropylbenzene	10.963	105	90624	6.743	ug/l	97
76) 1,2,3-Trichloropropane	11.085	75	90742	19.995	ug/l #	38
78) n-propylbenzene	11.305	91	36218	2.258	ug/l	97
79) 2-Chlorotoluene	11.402	91	39415	3.891	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.457	105	151779	13.486	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.085	75	90742	59.983	ug/l #	13
82) 4-Chlorotoluene	11.451	91	16275	1.470	ug/l #	46
83) tert-Butylbenzene	11.756	119	36673	3.516	ug/l #	47
84) 1,2,4-Trimethylbenzene	11.756	105	318633	28.378	ug/l	99
85) sec-Butylbenzene	11.756	105	318633	22.317	ug/l #	56
86) p-Isopropyltoluene	12.012	119	75835	6.639	ug/l	96
89) n-Butylbenzene	12.323	91	68717	6.462	ug/l #	1
90) Hexachloroethane	12.701	117	103697	52.725	ug/l #	16
92) 1,2-Dibromo-3-Chloropr...	12.920	75	525	0.445	ug/l #	1
95) Naphthalene	13.786	128	13014688	954.085	ug/l #	90

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
Data File : VX030280.D
Acq On : 28 Jul 2022 19:19
Operator : JC/MD
Sample : N3914-01MEDL 10X
Misc : 7.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME

Quant Time: Jul 29 05:59:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 25 16:49:17 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
Data File : VX030280.D
Acq On : 28 Jul 2022 19:19
Operator : JC/MD
Sample : N3914-01MEDL 10X
Misc : 7.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME

Quant Time: Jul 29 05:59:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 25 16:49:17 2022
Response via : Initial Calibration




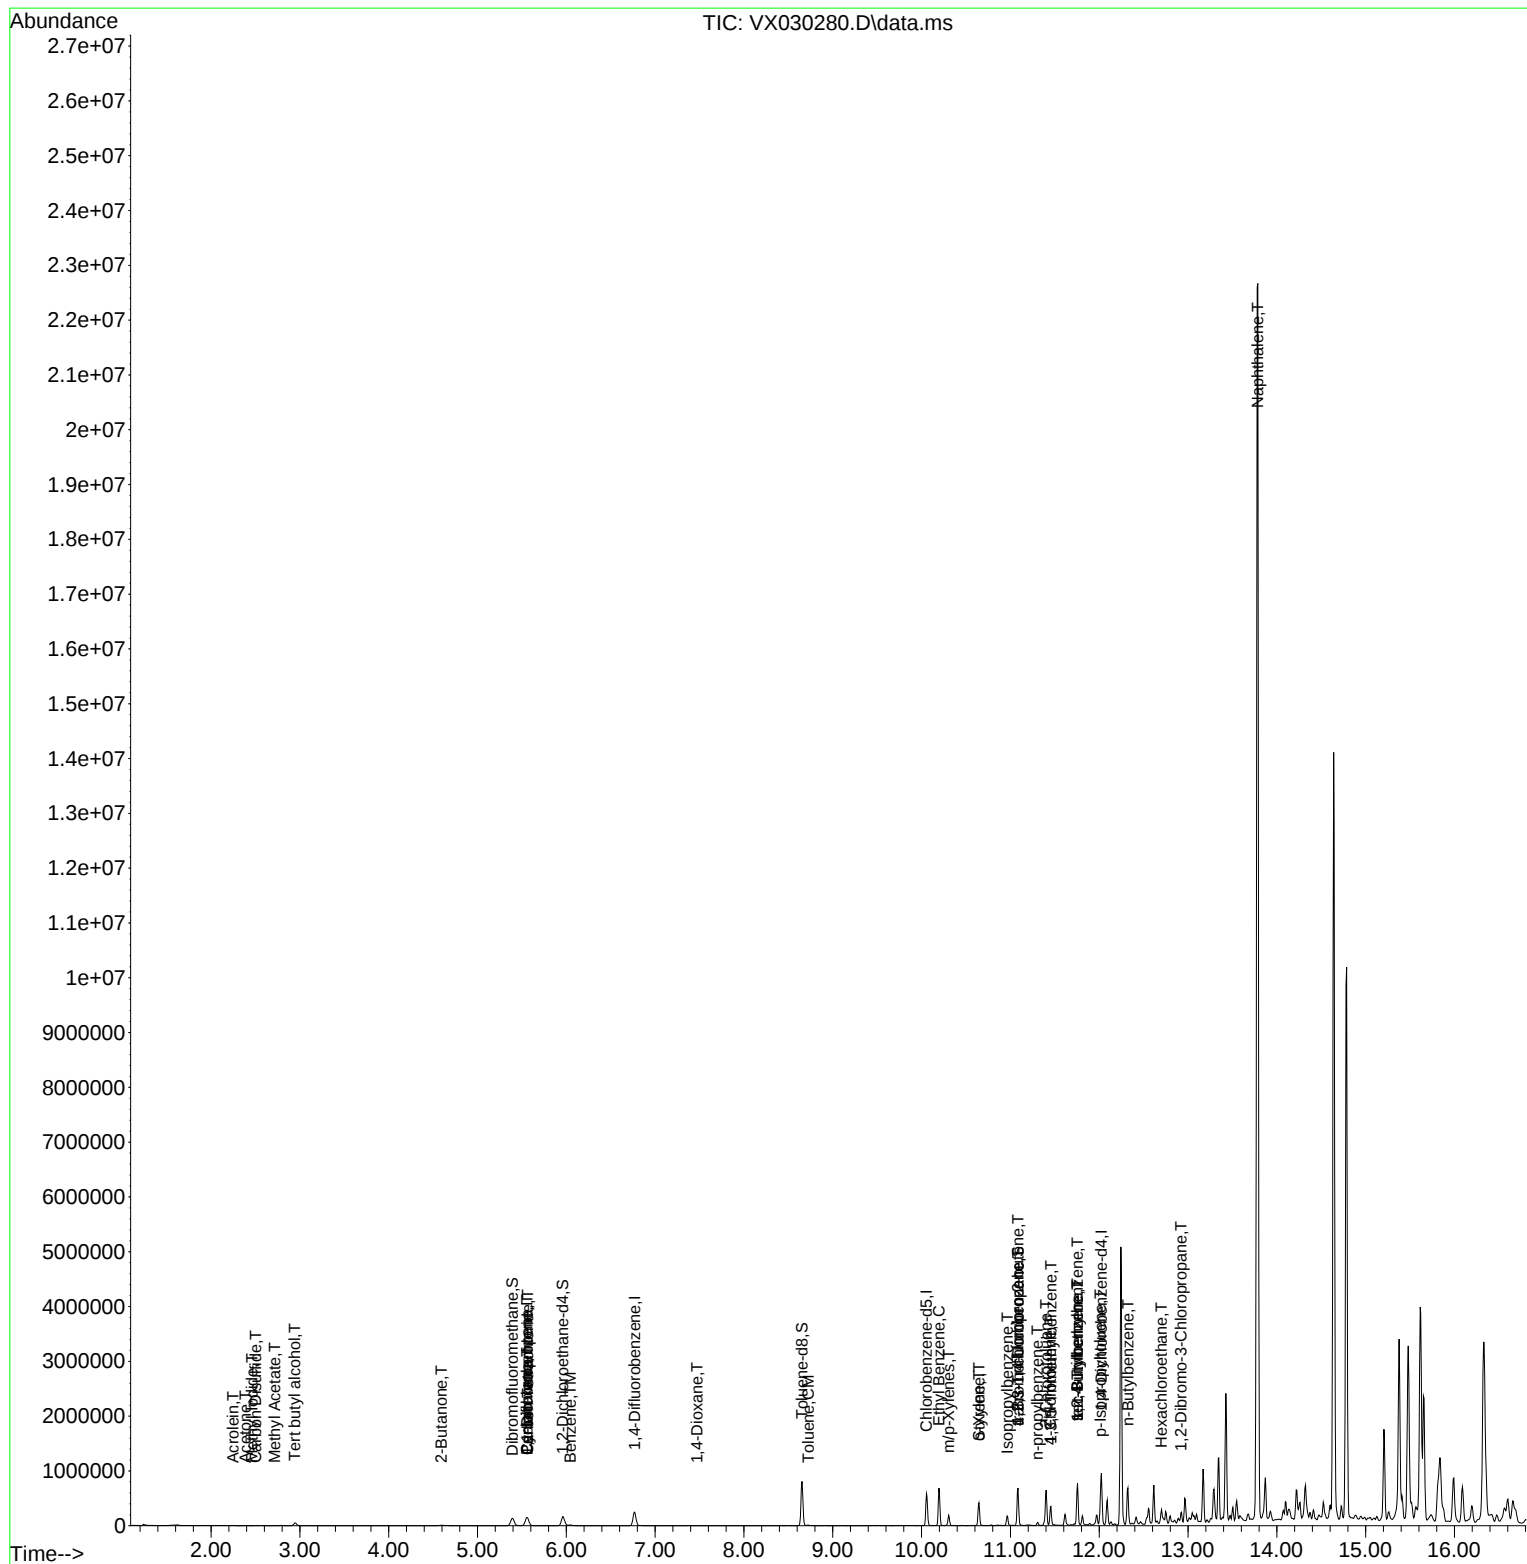




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion:168 Resp: 145032
Ion Ratio Lower Upper
168 100
99 58.7 44.0 66.0

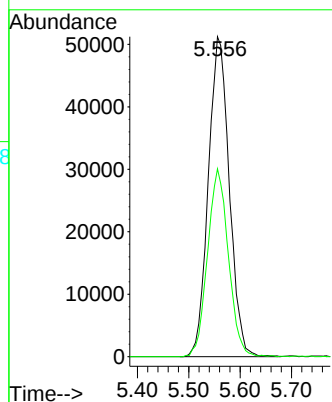

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 94 Resp: 471
Ion Ratio Lower Upper
94 100
96 52.7 76.9 115.3#


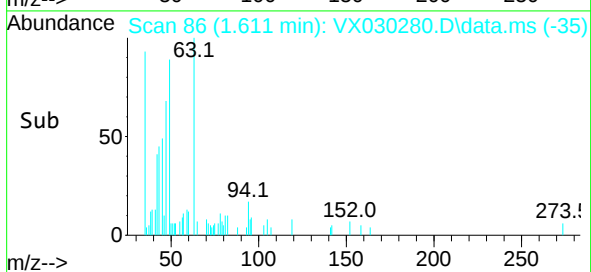
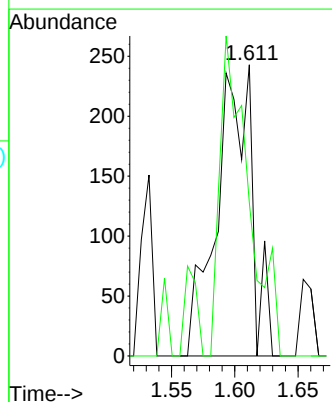
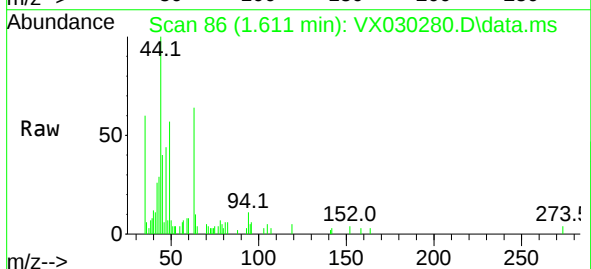




#10
Methyl Iodide
Concen: 1.612 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.013 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion:142 Resp: 202
Ion Ratio Lower Upper
142 100
127 0.0 30.2 45.2#
141 0.0 11.3 16.9#



#11
Tert butyl alcohol
Concen: 42.474 ug/l
RT: 2.941 min Scan# 304
Delta R.T. -0.036 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 59 Resp: 30202
Ion Ratio Lower Upper
59 100
57 1.7 7.4 11.2#


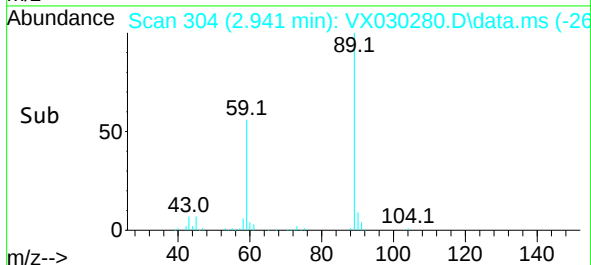
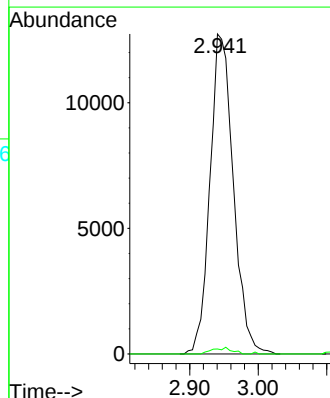





#13
Acrolein
Concen: 0.332 ug/l
RT: 2.245 min Scan# 189
Delta R.T. 0.006 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 56 Resp: 58
Ion Ratio Lower Upper
56 100
55 319.0 56.6 84.8#

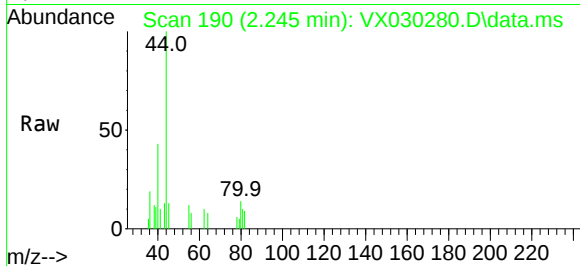

#16
Acetone
Concen: 1.770 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.001 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 43 Resp: 2642
Ion Ratio Lower Upper
43 100
58 30.0 27.7 41.5




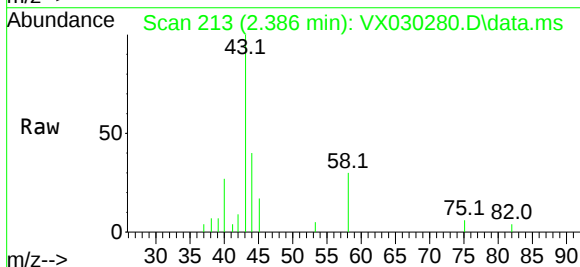




#17
Carbon Disulfide
Concen: 0.235 ug/l
RT: 2.502 min Scan# 21
Delta R.T. -0.005 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 76 Resp: 1437
Ion Ratio Lower Upper
76 100
78 0.0 7.8 11.6#

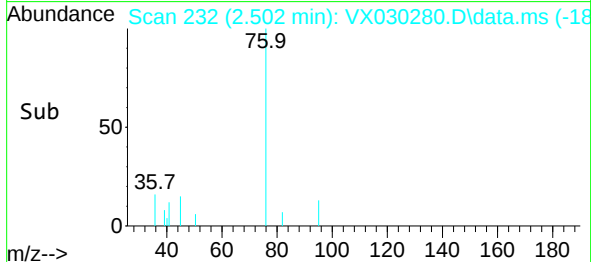

#18
Methyl Acetate
Concen: 0.300 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.007 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19


Tgt Ion: 43 Resp: 1325
Ion Ratio Lower Upper
43 100
74 20.5 19.4 29.2

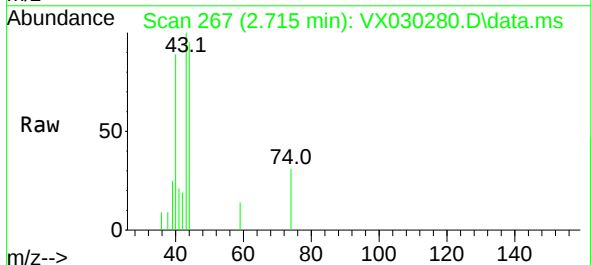






#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME







Tgt Ion:	84	Resp:	2715
Ion	Ratio	Lower	Upper
84	100		
49	115.8	93.8	140.6
51	40.3	29.4	44.0
86	66.6	51.0	76.4

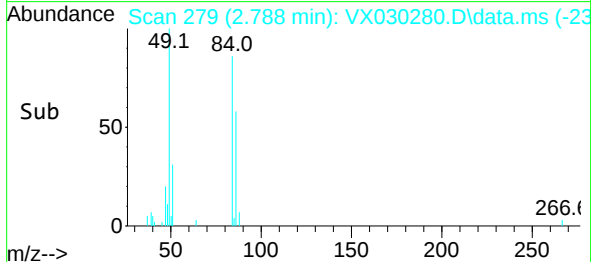

#25
2-Butanone
Concen: 0.774 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.025 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion:	43	Resp:	1942
Ion	Ratio	Lower	Upper
43	100		
72	12.2	21.7	32.5




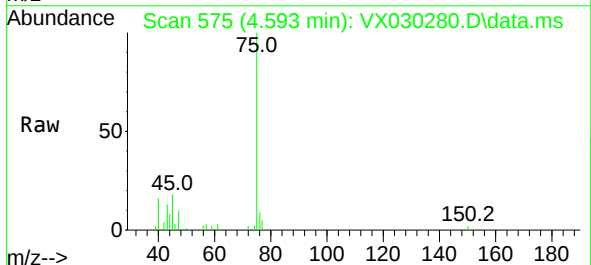




#31
Cyclohexane
Concen: 0.805 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.086 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 56 Resp: 3406
Ion Ratio Lower Upper
56 100
69 176.1 25.4 38.0#
84 143.5 68.9 103.3#

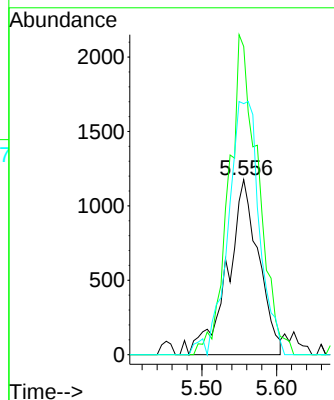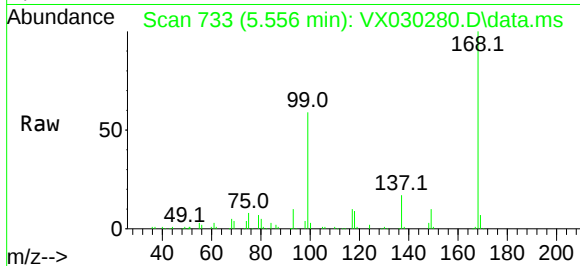

#33
1,2-Dichloroethane-d4
Concen: 52.386 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 65 Resp: 152707
Ion Ratio Lower Upper
65 100
67 54.8 0.0 109.6


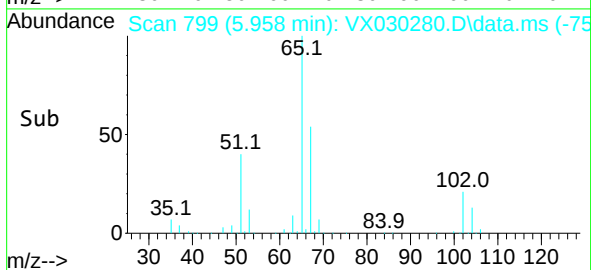
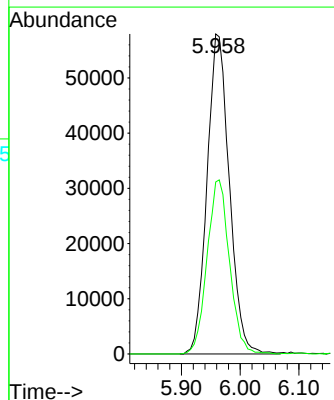
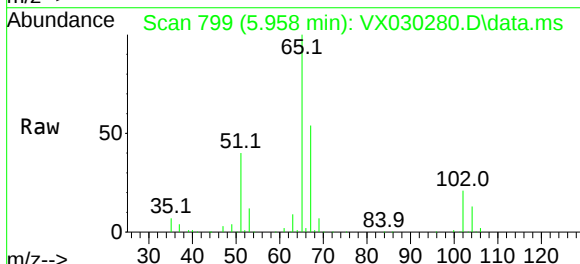


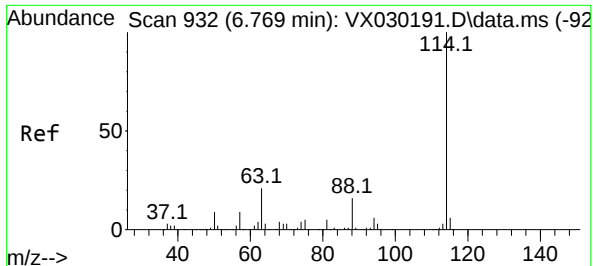

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion:114 Resp: 256564
Ion Ratio Lower Upper
114 100
63 22.4 0.0 38.4
88 17.3 0.0 31.8

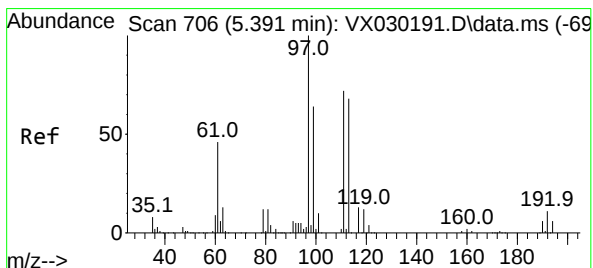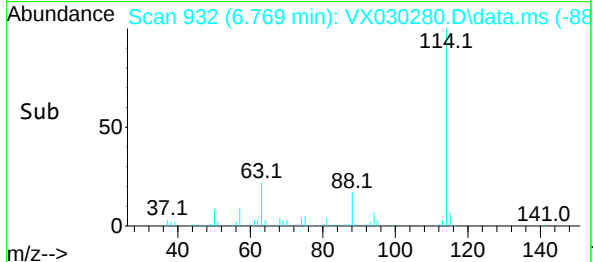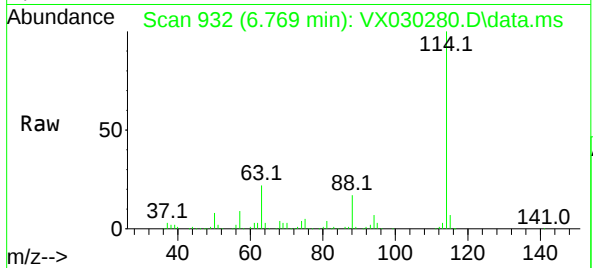

#35
Dibromofluoromethane
Concen: 49.626 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion:113 Resp: 121714
Ion Ratio Lower Upper
113 100
111 102.8 83.2 124.8
192 17.7 14.8 22.2


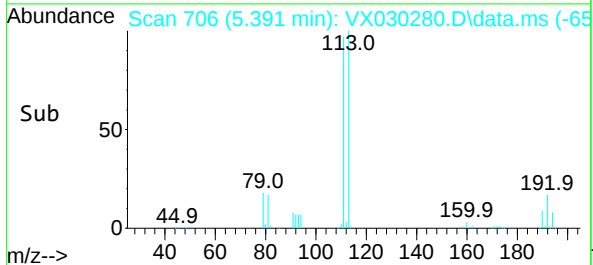

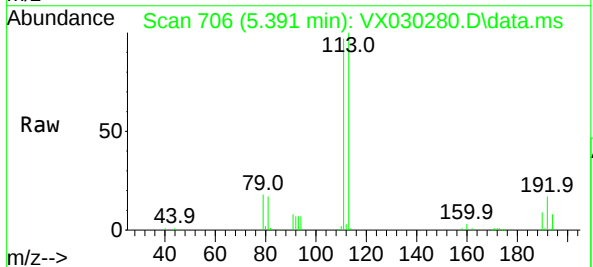




#36
1,1-Dichloropropene
Concen: 3.486 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.140 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 75 Resp: 12303
Ion Ratio Lower Upper
75 100
110 8.7 19.3 57.9#
77 0.0 24.4 36.6#



#38
Carbon Tetrachloride
Concen: 4.506 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.121 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 117 Resp: 14848
Ion Ratio Lower Upper
117 100
119 6.5 74.1 111.1#
121 0.0 25.8 38.8#

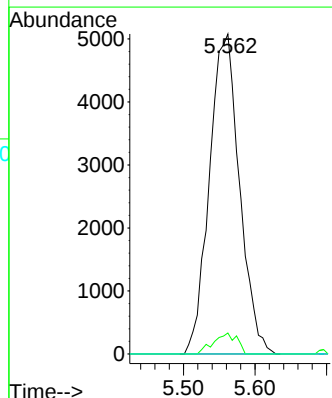



#40

Benzene

Concen: 1.329 ug/l

RT: 6.044 min Scan# 81

Delta R.T. 0.001 min

Lab File: VX030280.D

Acq: 28 Jul 2022 19:19

Instrument :

MSVOA_X

ClientSampleId :





METRO-DISPME

Tgt Ion: 78 Resp: 14758

Ion Ratio Lower Upper

78 100

77 21.9 18.0 27.0

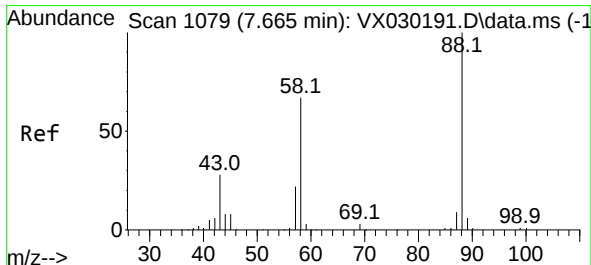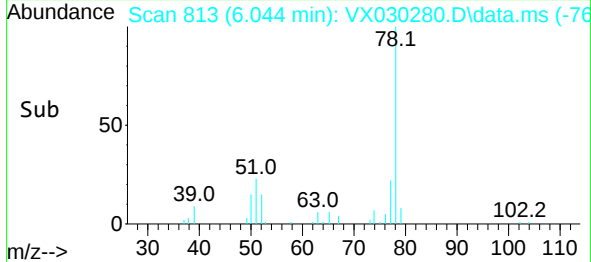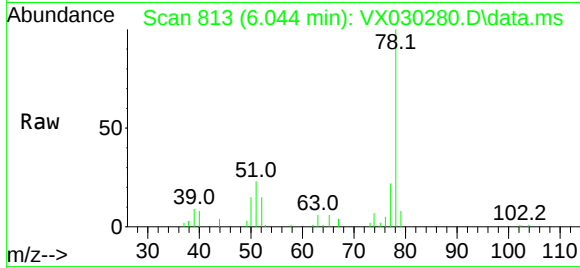

#49

1,4-Dioxane

Concen: 0.240 ug/l

RT: 7.470 min Scan# 1047

Delta R.T. -0.195 min

Lab File: VX030280.D

Acq: 28 Jul 2022 19:19




Tgt Ion: 88 Resp: 20


Ion Ratio Lower Upper

88 100

43 1940.0 23.8 35.8#

58 0.0 53.8 80.6#

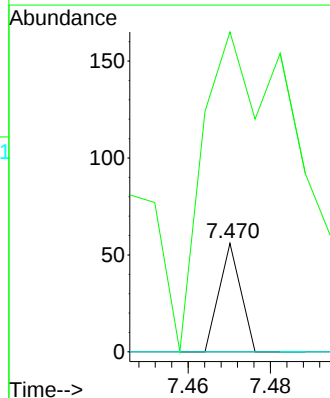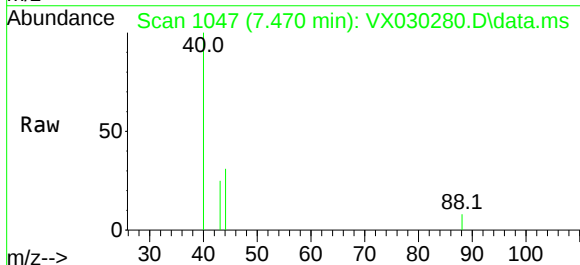

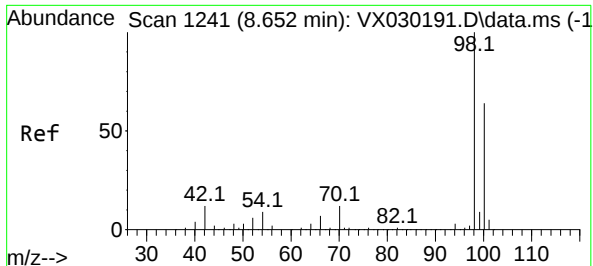

#50

Toluene-d8

Concen: 50.019 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.001 min

Lab File: VX030280.D

Acq: 28 Jul 2022 19:19

Instrument :

MSVOA_X

ClientSampleId :





METRO-DISPME

Tgt Ion: 98 Resp: 475085

Ion Ratio Lower Upper

98 100

100 64.5 52.3 78.5

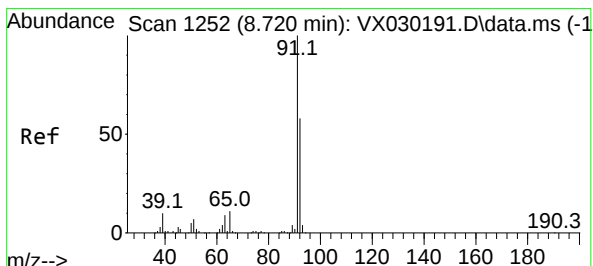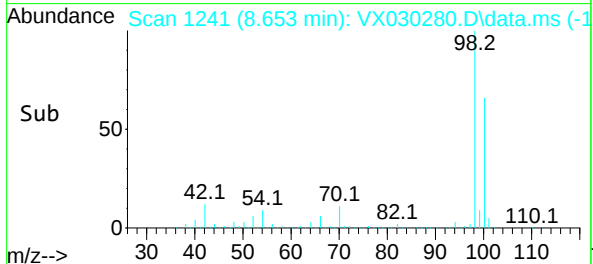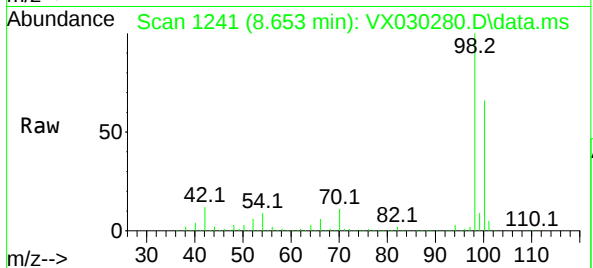

#52

Toluene

Concen: 0.541 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX030280.D




Acq: 28 Jul 2022 19:19


Tgt Ion: 92 Resp: 3666

Ion Ratio Lower Upper

92 100

91 177.8 139.2 208.8


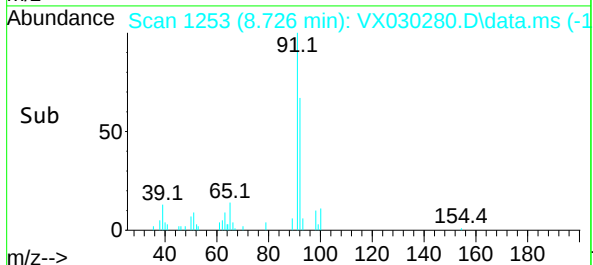

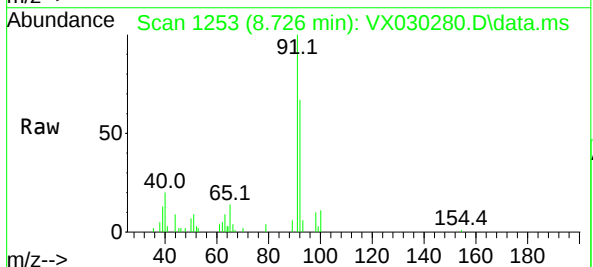




#62
4-Bromofluorobenzene
Concen: 53.432 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 95 Resp: 188349
Ion Ratio Lower Upper
95 100
174 69.8 0.0 149.0
176 67.8 0.0 146.0

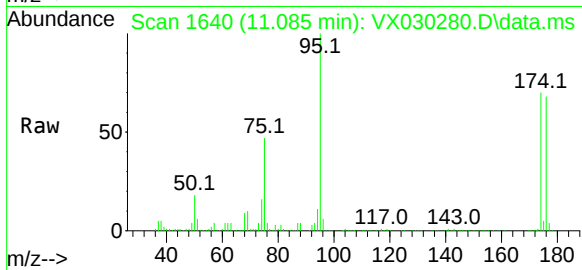

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 117 Resp: 263564
Ion Ratio Lower Upper
117 100
82 58.2 42.7 64.1
119 33.0 25.4 38.2


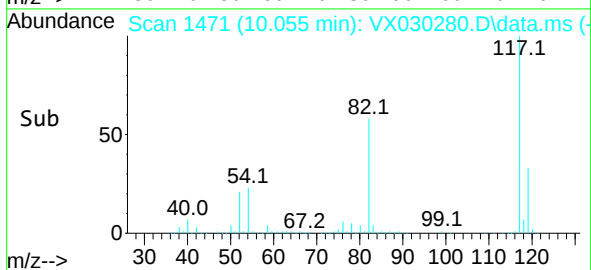

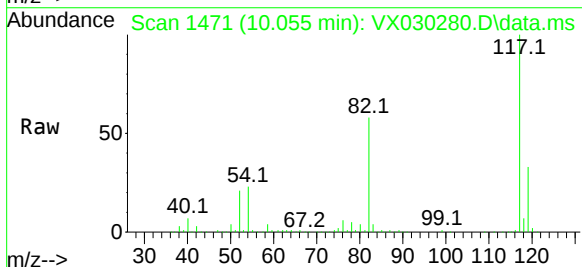




#67
Ethyl Benzene
Concen: 32.347 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 91 Resp: 378623
Ion Ratio Lower Upper
91 100
106 30.8 25.5 38.3

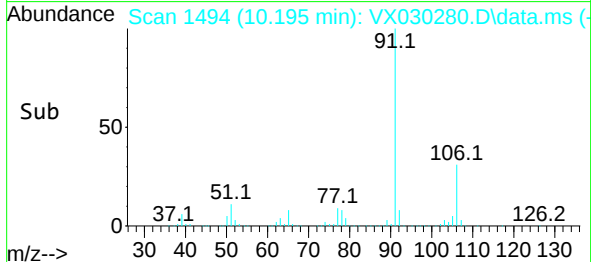

#68
m/p-Xylenes
Concen: 8.429 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 106 Resp: 40879
Ion Ratio Lower Upper
106 100
91 205.8 158.2 237.4


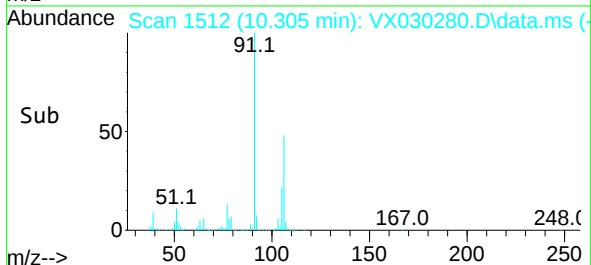

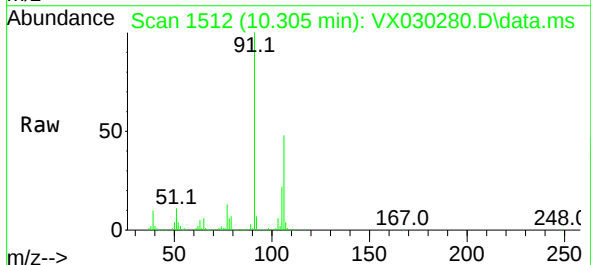


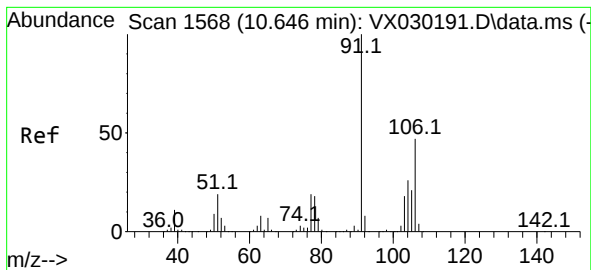

#69
o-Xylene
Concen: 18.757 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion:106 Resp: 89661
Ion Ratio Lower Upper
106 100
91 218.6 103.8 311.6

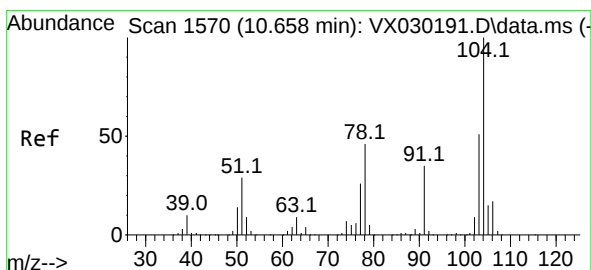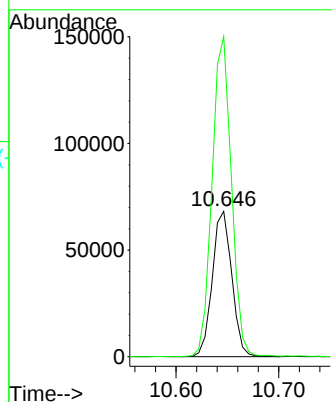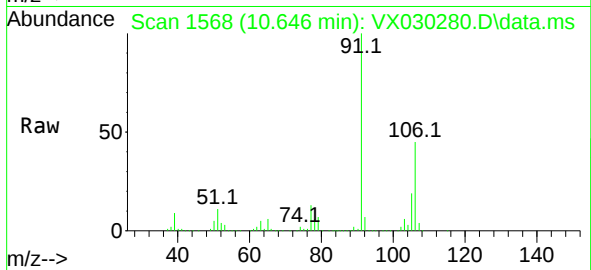

#70
Styrene
Concen: 0.725 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion:104 Resp: 5696
Ion Ratio Lower Upper
104 100
78 244.9 37.8 56.8#
103 226.6 44.5 66.7#









#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion:152 Resp: 172169
Ion Ratio Lower Upper
152 100
115 65.9 40.5 121.5
150 158.4 0.0 347.0

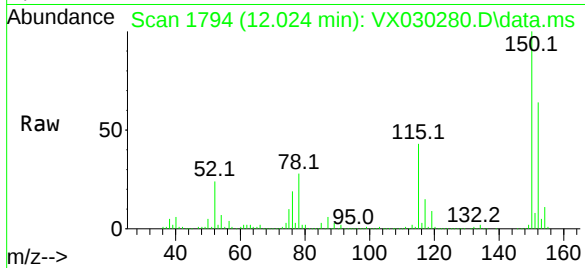

#73
Isopropylbenzene
Concen: 6.743 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion:105 Resp: 90624
Ion Ratio Lower Upper
105 100
120 25.3 13.5 40.4



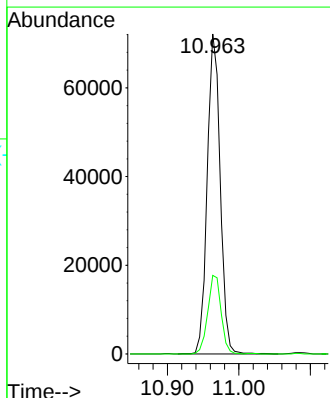
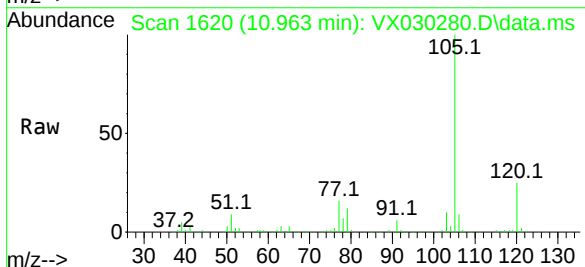




#76
1,2,3-Trichloropropane
Concen: 19.995 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.158 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 75 Resp: 90742
Ion Ratio Lower Upper
75 100
77 1.7 19.8 59.3#

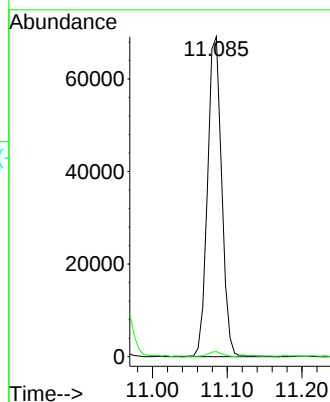

#78
n-propylbenzene
Concen: 2.258 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.005 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 91 Resp: 36218
Ion Ratio Lower Upper
91 100
120 21.9 11.6 34.8


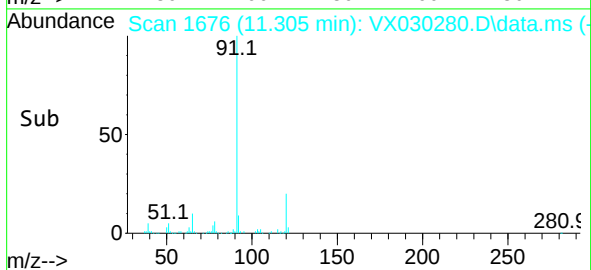
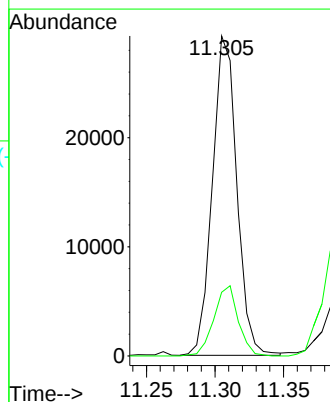





#79
2-Chlorotoluene
Concen: 3.891 ug/l
RT: 11.402 min Scan# 1
Delta R.T. 0.037 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME


Tgt Ion: 91 Resp: 39415
Ion Ratio Lower Upper
91 100
126 2.3 17.4 52.3#

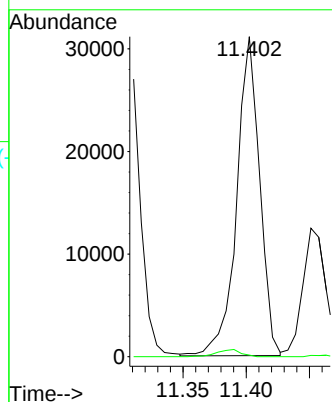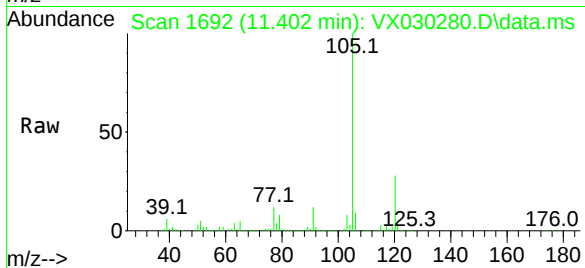

#80
1,3,5-Trimethylbenzene
Concen: 13.486 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 105 Resp: 151779
Ion Ratio Lower Upper
105 100
120 47.0 24.4 73.2


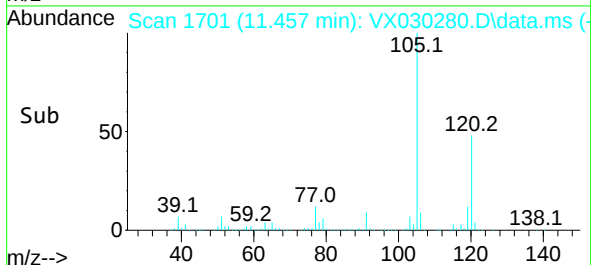

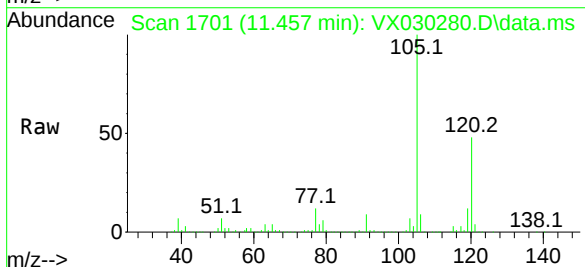




#81
 trans-1,4-Dichloro-2-butene
 Concen: 59.983 ug/l
 RT: 11.085 min Scan# 1
 Delta R.T. 0.061 min
 Lab File: VX030280.D
 Acq: 28 Jul 2022 19:19




Instrument :
 MSVOA_X
 ClientSampleId :
 METRO-DISPME


Tgt Ion: 75 Resp: 90742
 Ion Ratio Lower Upper
 75 100
 53 0.5 74.2 111.4#
 89 0.0 34.8 52.2#

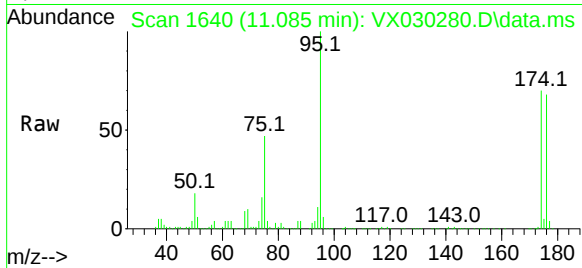

#82
 4-Chlorotoluene
 Concen: 1.470 ug/l
 RT: 11.451 min Scan# 1700
 Delta R.T. -0.006 min
 Lab File: VX030280.D
 Acq: 28 Jul 2022 19:19

Tgt Ion: 91 Resp: 16275
 Ion Ratio Lower Upper
 91 100
 126 0.9 15.3 45.9#


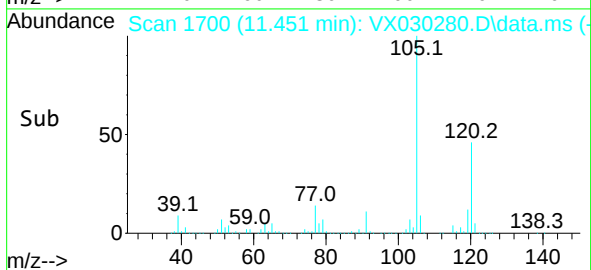

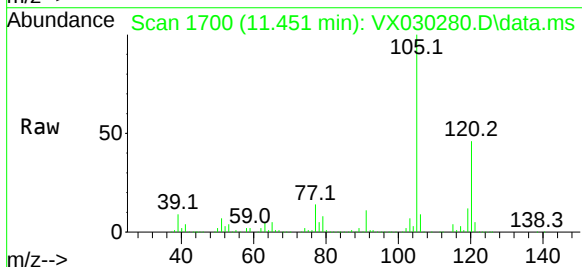




#83
 tert-Butylbenzene
 Concen: 3.516 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.037 min
 Lab File: VX030280.D
 Acq: 28 Jul 2022 19:19




Instrument :
 MSVOA_X
 ClientSampleId :
 METRO-DISPME


Tgt Ion:119 Resp: 36673
 Ion Ratio Lower Upper
 119 100
 91 97.3 28.3 84.9#
 134 0.0 11.2 33.5#

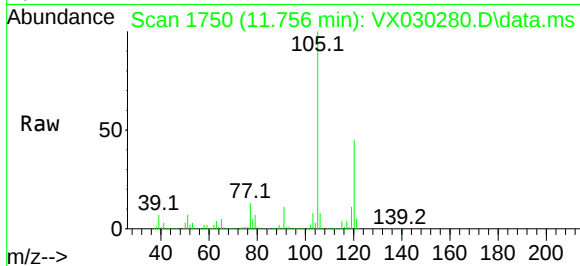

#84
 1,2,4-Trimethylbenzene
 Concen: 28.378 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.000 min
 Lab File: VX030280.D
 Acq: 28 Jul 2022 19:19

Tgt Ion:105 Resp: 318633
 Ion Ratio Lower Upper
 105 100
 120 45.2 22.9 68.8




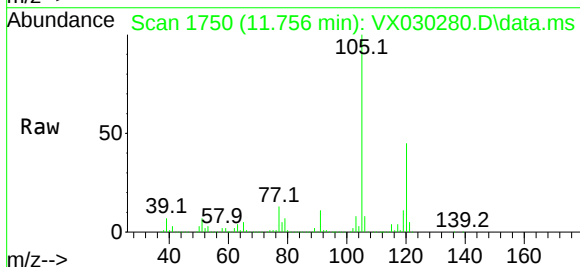




#85
 sec-Butylbenzene
 Concen: 22.317 ug/l
 RT: 11.756 min Scan# 11756
 Delta R.T. -0.140 min
 Lab File: VX030280.D
 Acq: 28 Jul 2022 19:19




Instrument :
 MSVOA_X
 ClientSampleId :
 METRO-DISPME


Tgt Ion:105 Resp: 318633
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#

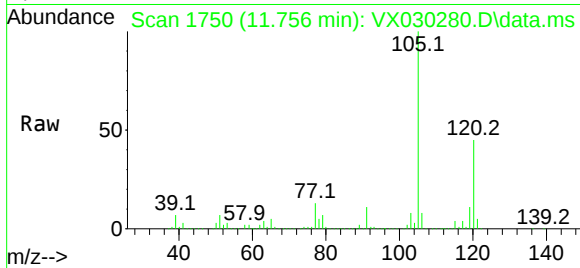

#86
 p-Isopropyltoluene
 Concen: 6.639 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX030280.D
 Acq: 28 Jul 2022 19:19

Tgt Ion:119 Resp: 75835
 Ion Ratio Lower Upper
 119 100
 134 26.5 13.9 41.6
 91 26.0 11.8 35.3

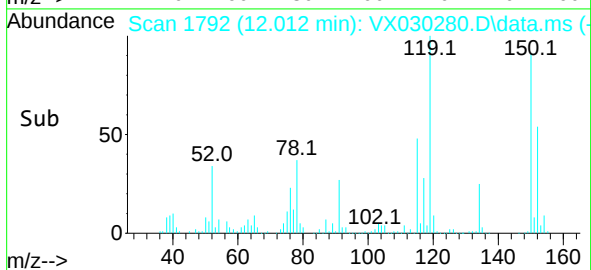



#89

n-Butylbenzene

Concen: 6.462 ug/l

RT: 12.323 min Scan# 11

Delta R.T. -0.012 min

Lab File: VX030280.D

Acq: 28 Jul 2022 19:19

Instrument :

MSVOA_X

ClientSampleId :

METRO-DISPME





Tgt Ion: 91 Resp: 68717

Ion Ratio Lower Upper

91 100

92 18.9 26.2 78.5#

134 140.8 12.6 37.8#

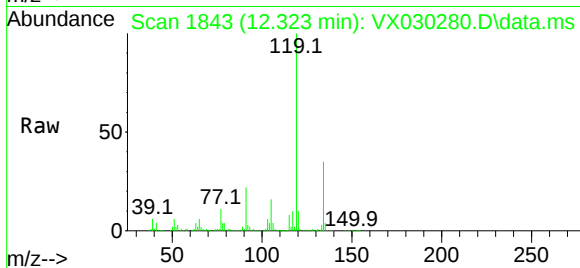

#90

Hexachloroethane

Concen: 52.725 ug/l

RT: 12.701 min Scan# 1905

Delta R.T. 0.159 min

Lab File: VX030280.D




Acq: 28 Jul 2022 19:19


Tgt Ion: 117 Resp: 103697

Ion Ratio Lower Upper

117 100

201 0.0 34.2 102.5#


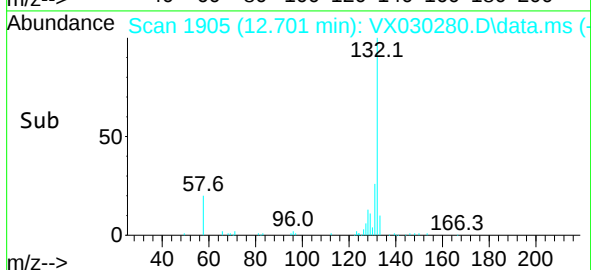

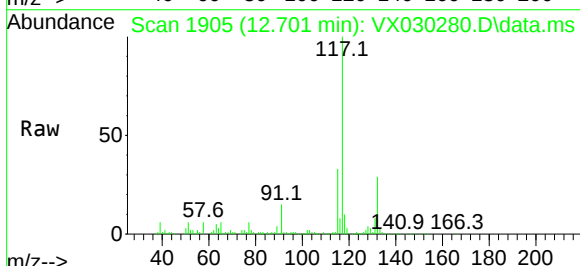




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.445 ug/l
RT: 12.920 min Scan# 1945
Delta R.T. -0.024 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Instrument :
MSVOA_X
ClientSampleId :
METRO-DISPME

Tgt Ion: 75 Resp: 525
Ion Ratio Lower Upper
75 100
155 0.0 45.0 134.8#
157 0.0 56.9 170.7#

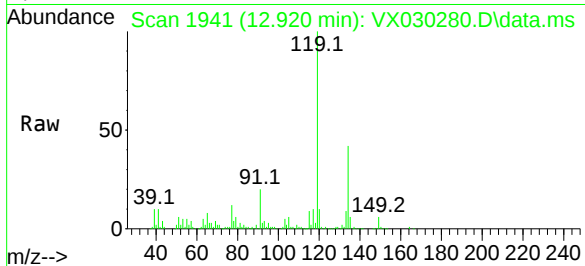

#95
Naphthalene
Concen: 954.085 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.006 min
Lab File: VX030280.D
Acq: 28 Jul 2022 19:19

Tgt Ion: 128 Resp: 13014688
Ion Ratio Lower Upper
128 100
127 16.8 10.2 15.2#
129 14.5 8.6 13.0#

