

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
 Data File : VX030267.D
 Acq On : 28 Jul 2022 13:17
 Operator : JC/MD
 Sample : VX0728WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0728WBL01

Quant Time: Jul 29 05:56:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 25 16:49:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	133997	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	232554	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	232881	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	128667	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	146979	54.573	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.140%
35) Dibromofluoromethane	5.391	113	116096	52.223	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.440%
50) Toluene-d8	8.653	98	421186	48.922	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.840%
62) 4-Bromofluorobenzene	11.085	95	149781	46.878	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072822\
Data File : VX030267.D
Acq On : 28 Jul 2022 13:17
Operator : JC/MD
Sample : VX0728WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0728WBL01

Quant Time: Jul 29 05:56:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 25 16:49:17 2022
Response via : Initial Calibration




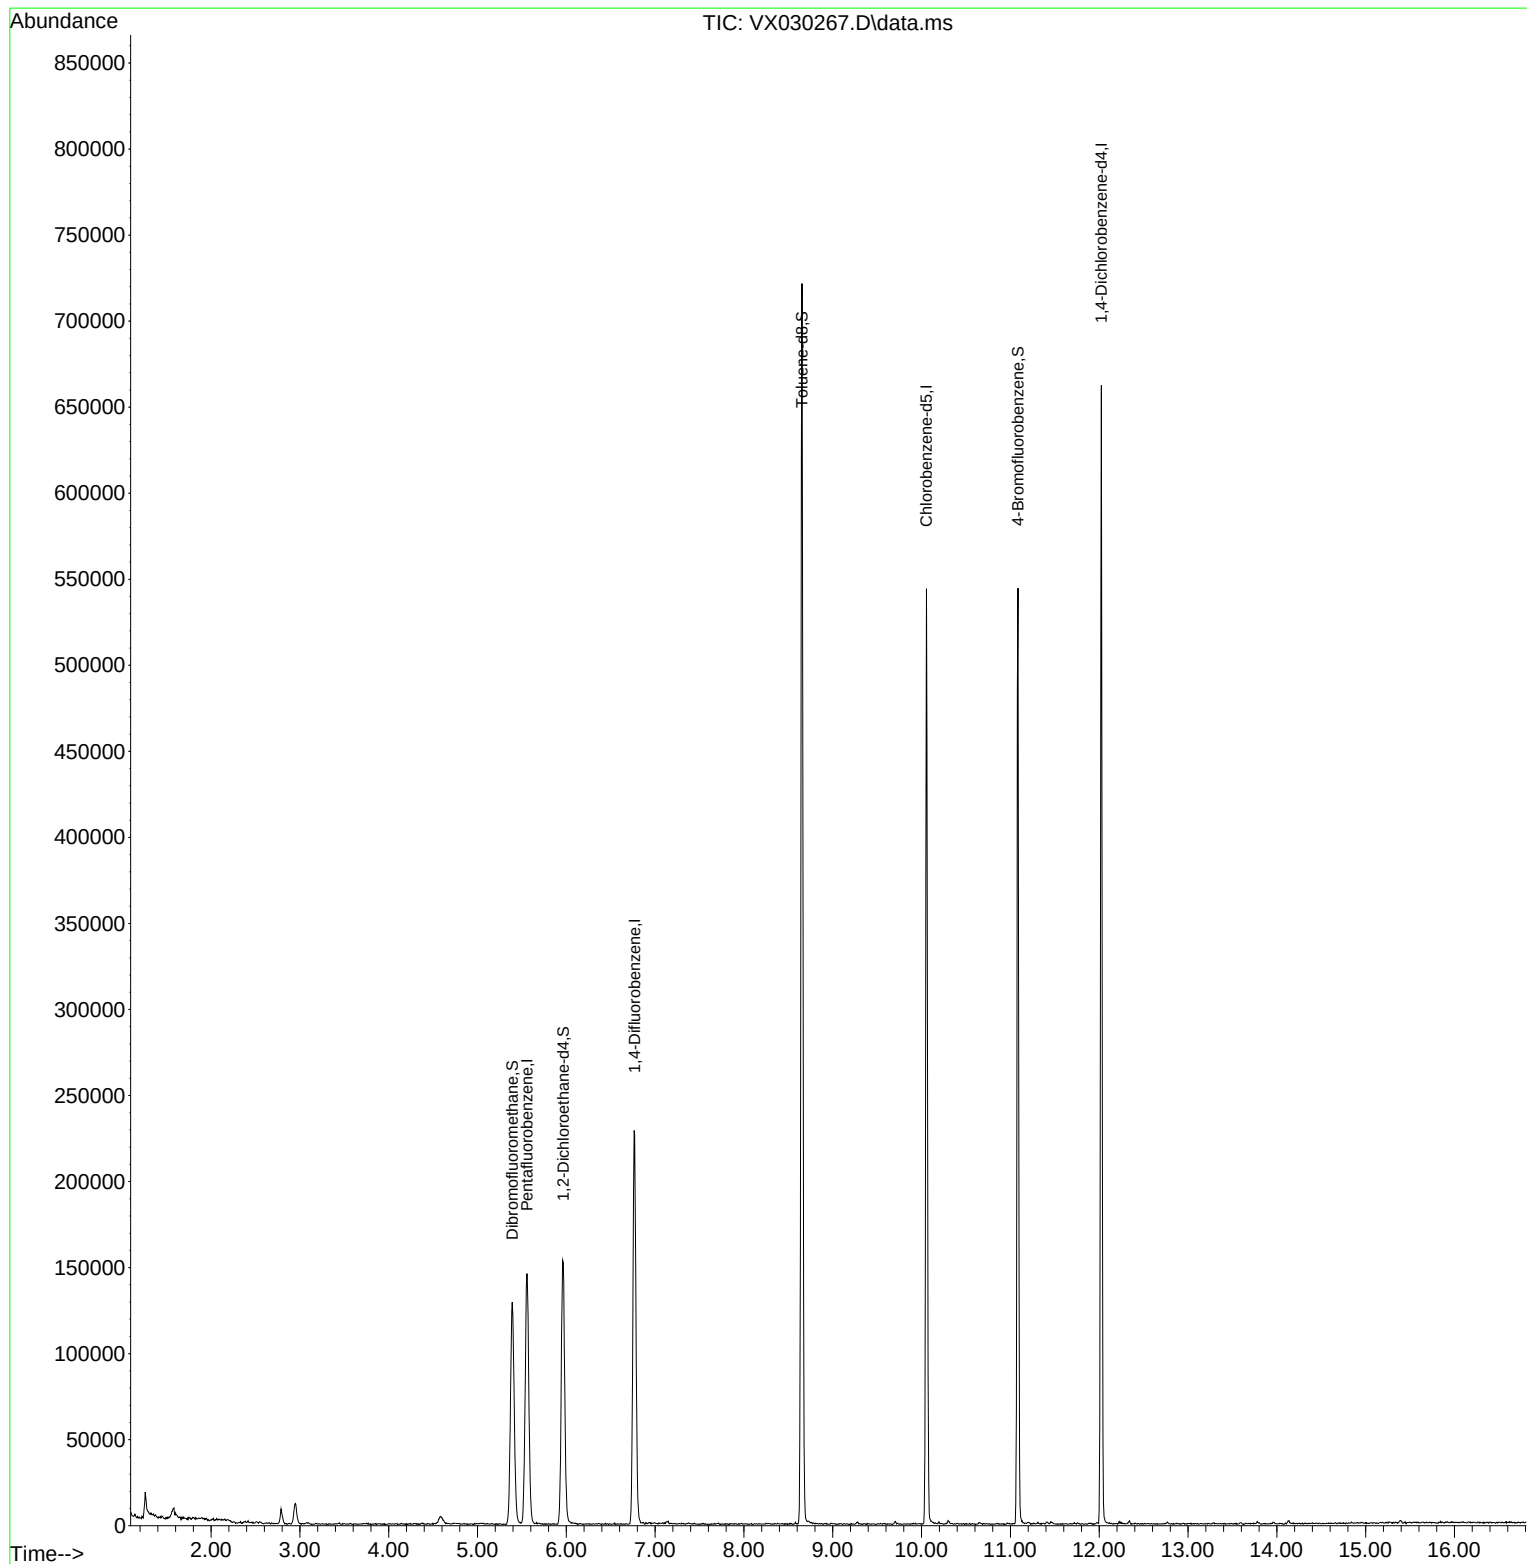


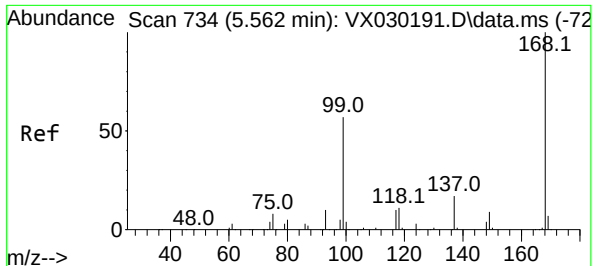

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17




Instrument :
MSVOA_X
ClientSampleId :
VX0728WBL01


Tgt Ion:168 Resp: 133997
Ion Ratio Lower Upper
168 100
99 61.7 44.0 66.0

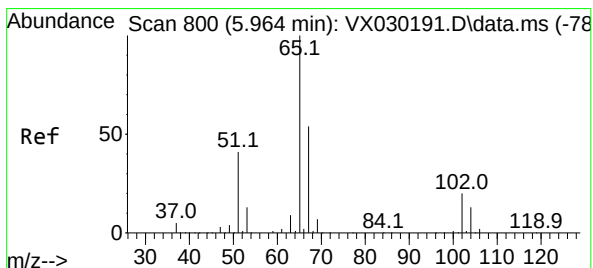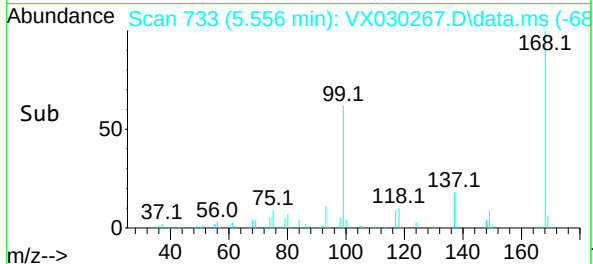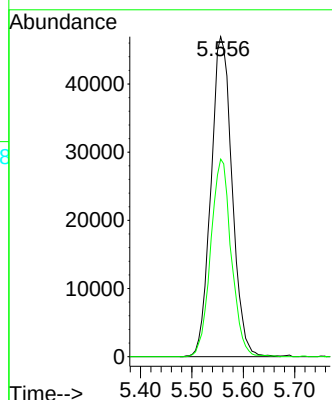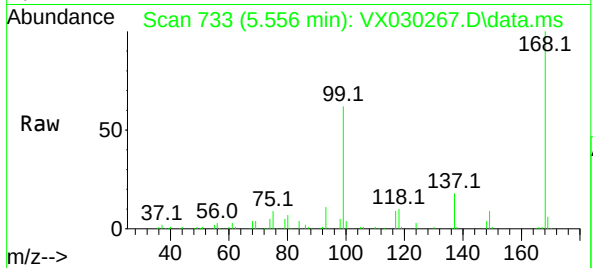

#33
1,2-Dichloroethane-d4
Concen: 54.573 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17

Tgt Ion: 65 Resp: 146979
Ion Ratio Lower Upper
65 100
67 53.2 0.0 109.6


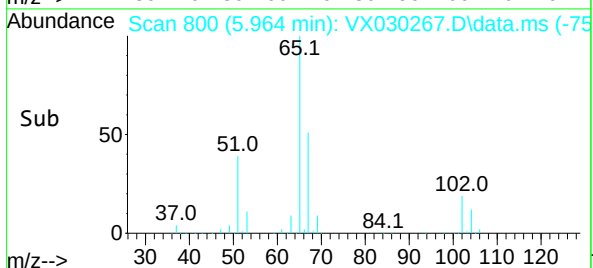
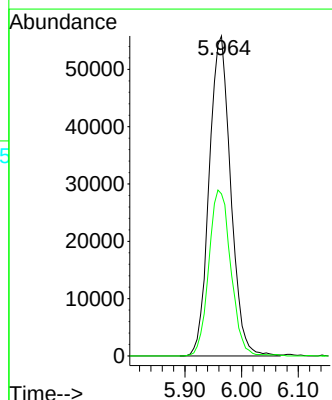
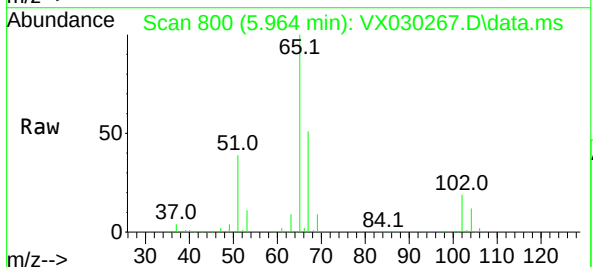


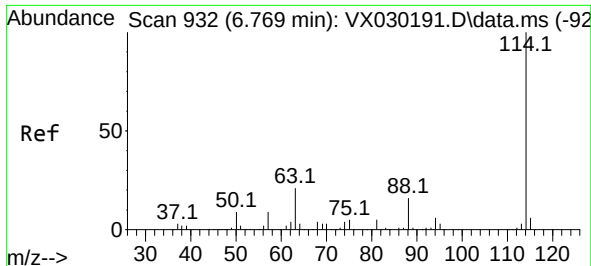

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17




Instrument :
MSVOA_X
ClientSampleId :
VX0728WBL01


Tgt Ion:114 Resp: 232554
Ion Ratio Lower Upper
114 100
63 20.0 0.0 38.4
88 15.3 0.0 31.8

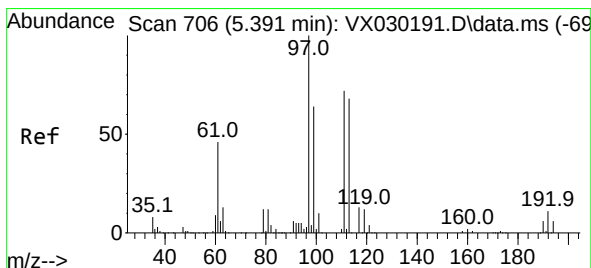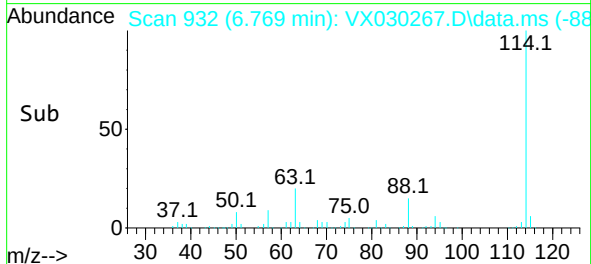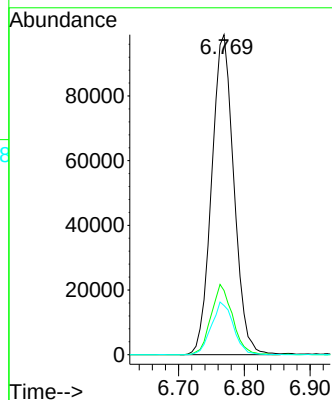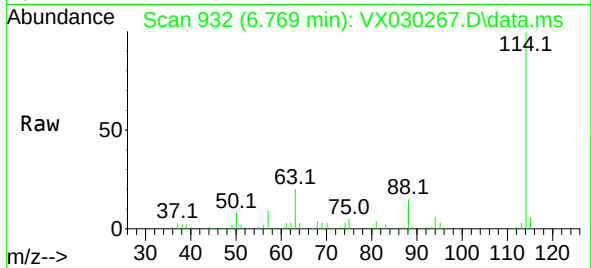

#35
Dibromofluoromethane
Concen: 52.223 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17

Tgt Ion:113 Resp: 116096
Ion Ratio Lower Upper
113 100
111 102.9 83.2 124.8
192 16.8 14.8 22.2


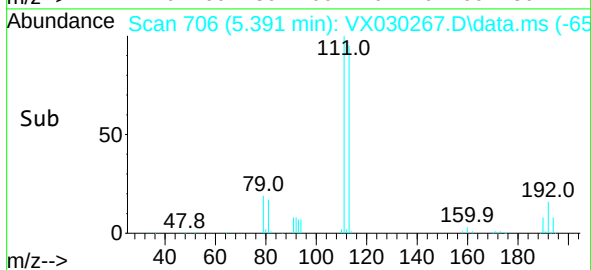
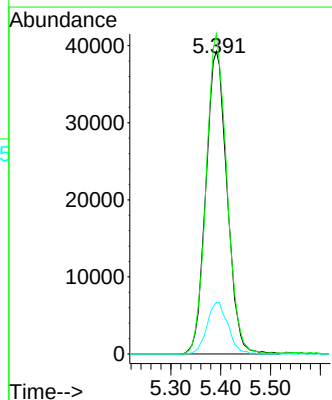
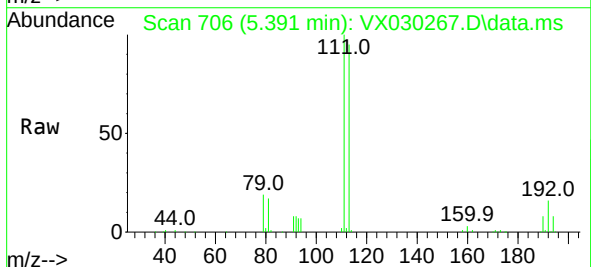


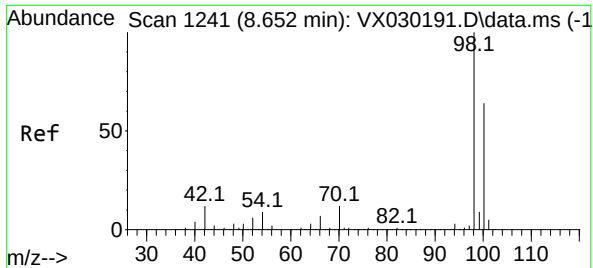

#50
Toluene-d8
Concen: 48.922 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.001 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17




Instrument :
MSVOA_X
ClientSampleId :
VX0728WBL01


Tgt Ion: 98 Resp: 421186
Ion Ratio Lower Upper
98 100
100 64.4 52.3 78.5

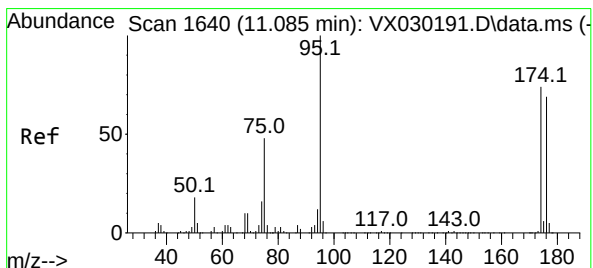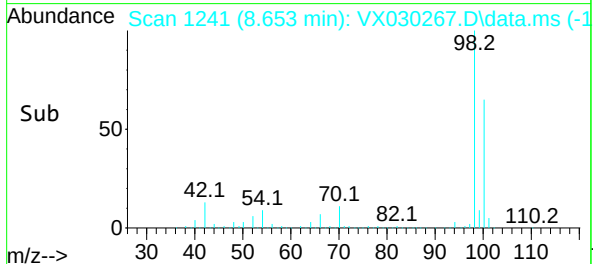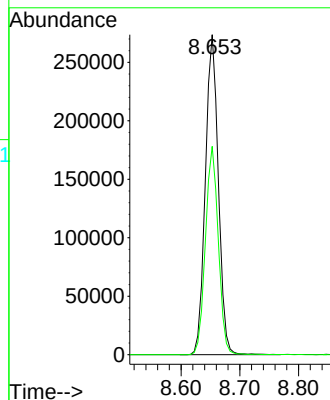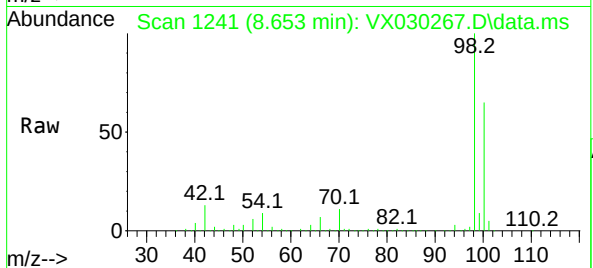

#62
4-Bromofluorobenzene
Concen: 46.878 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17

Tgt Ion: 95 Resp: 149781
Ion Ratio Lower Upper
95 100
174 69.5 0.0 149.0
176 67.1 0.0 146.0


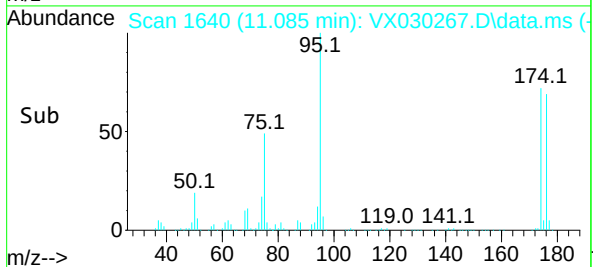
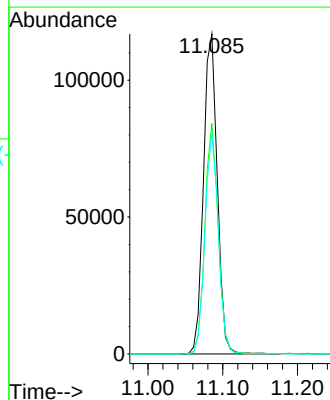
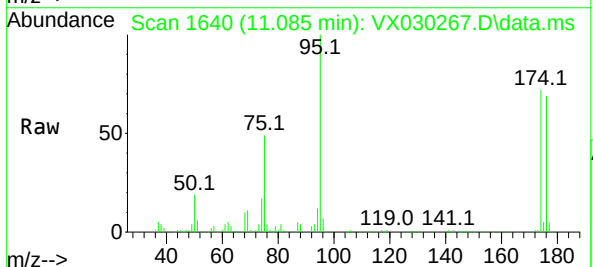


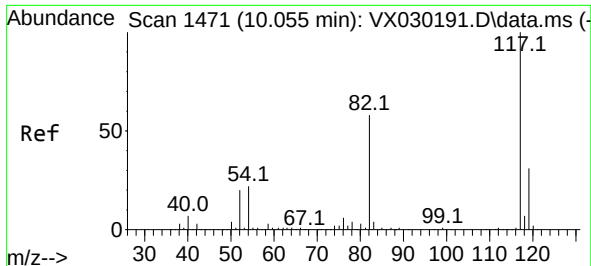

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17

Instrument :
MSVOA_X
ClientSampleId :
VX0728WBL01

Tgt Ion:117 Resp: 232881
Ion Ratio Lower Upper
117 100
82 57.8 42.7 64.1
119 32.3 25.4 38.2

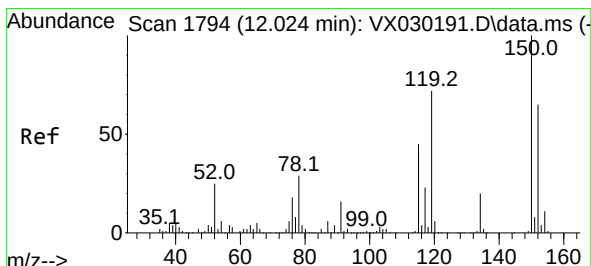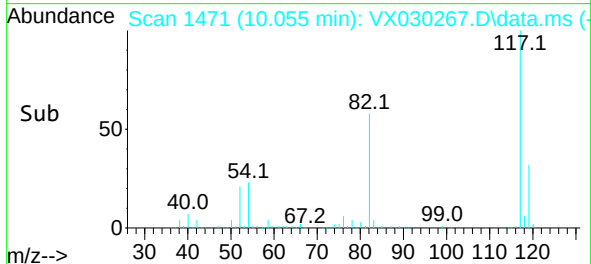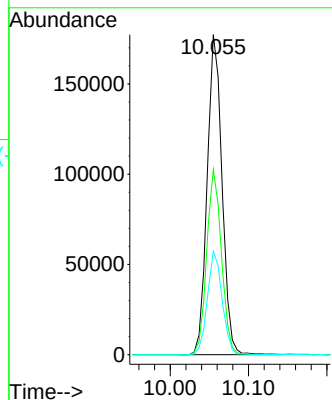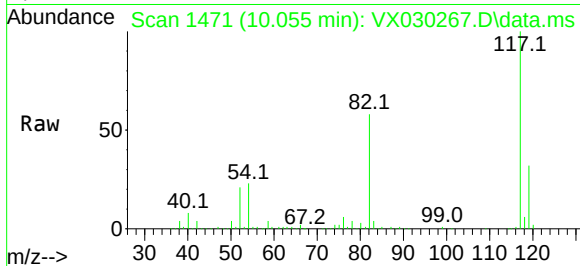

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030267.D
Acq: 28 Jul 2022 13:17

Tgt Ion:152 Resp: 128667
Ion Ratio Lower Upper
152 100
115 62.2 40.5 121.5
150 158.6 0.0 347.0

