

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042603.D
 Acq On : 26 Jul 2024 17:19
 Operator : JC/MD
 Sample : VX0726WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 27 01:24:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 01:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	172698	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	156355	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	63975	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	42411	40.422	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.840%		
7) Chloroethane-d5	1.648	69	20055	46.387	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.780%		
11) 1,1-Dichloroethene-d2	2.294	65	23894	46.221	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.440%		
21) 2-Butanone-d5	4.459	46	84556	108.736	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.740%		
24) Chloroform-d	5.050	84	111095	48.376	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.760%		
26) 1,2-Dichloroethane-d4	5.952	65	71952	48.564	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.120%		
32) Benzene-d6	5.964	84	219012	50.471	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.940%		
36) 1,2-Dichloropropane-d6	7.306	67	67372	52.459	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.920%		
41) Toluene-d8	8.647	98	193314	49.686	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.380%		
43) trans-1,3-Dichloroprop...	8.952	79	29368	48.865	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.720%		
47) 2-Hexanone-d5	9.385	63	61977	107.936	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	107.940%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	96720	52.306	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.620%		
66) 1,2-Dichlorobenzene-d4	12.323	152	65452	54.135	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.280%		
Target Compounds			Qvalue			
37) 1,2-Dichloropropane	7.306	63	7736	6.221	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042603.D
Acq On : 26 Jul 2024 17:19
Operator : JC/MD
Sample : VX0726WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 27 01:24:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 01:23:37 2024
Response via : Initial Calibration

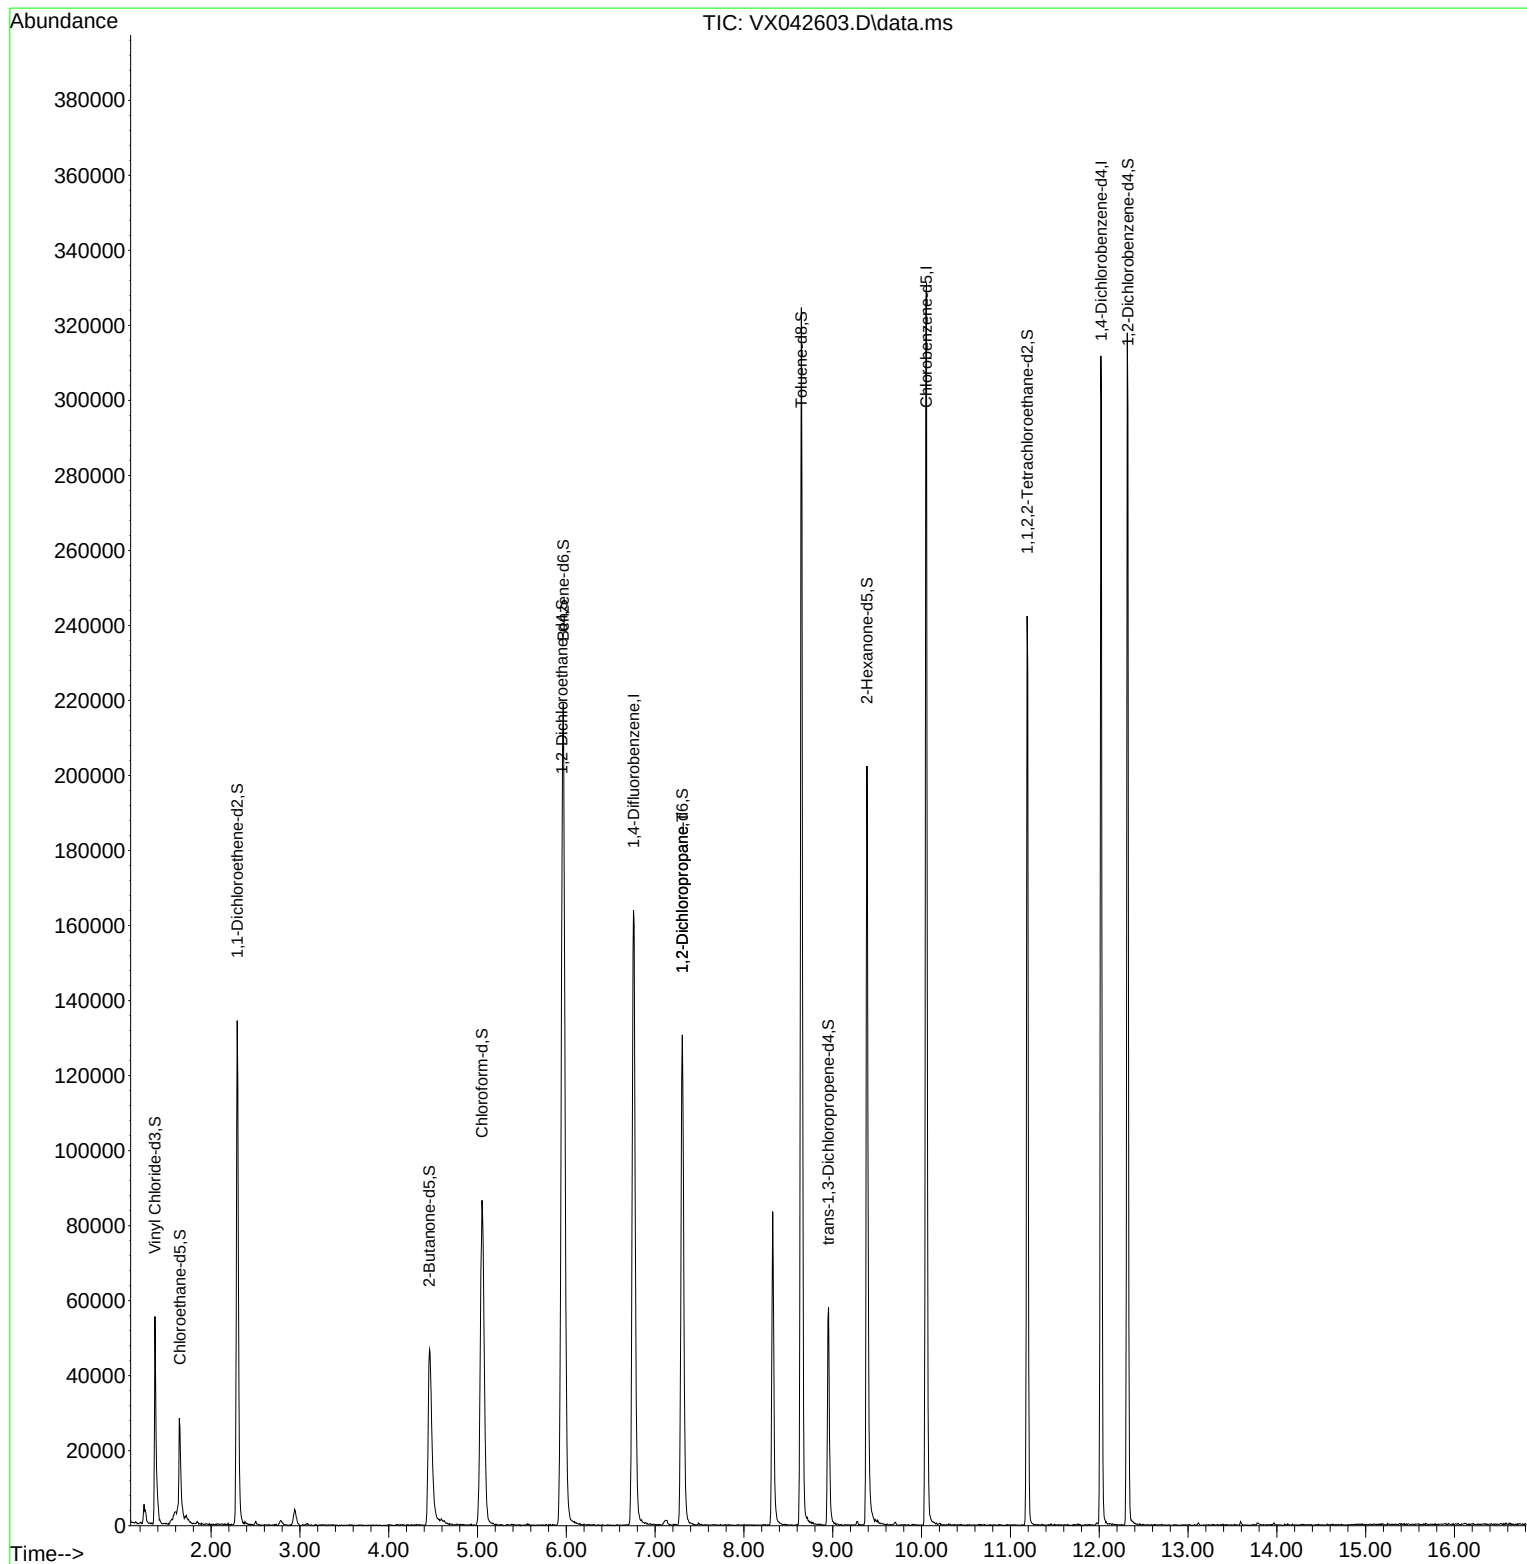

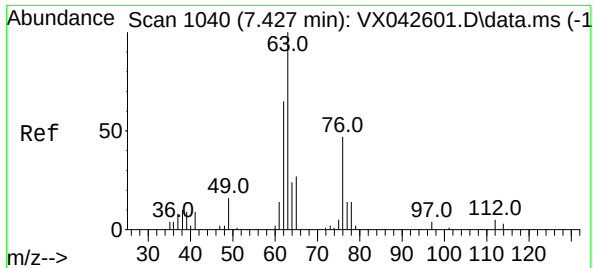

#37
 1,2-Dichloropropane
 Concen: 6.221 ug/L
 RT: 7.306 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX042603.D
 Acq: 26 Jul 2024 17:19

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 7736
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.7 5.5#

