

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042607.D
 Acq On : 26 Jul 2024 18:52
 Operator : JC/MD
 Sample : P3334-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 27 01:34:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 01:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	165115	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	143388	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	52496	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	44539	44.400	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	88.800%	
7) Chloroethane-d5	1.648	69	20464	49.506	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	99.020%	
11) 1,1-Dichloroethene-d2	2.300	65	23304	47.150	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.300%	
21) 2-Butanone-d5	4.464	46	80419	108.166	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	108.170%	
24) Chloroform-d	5.056	84	107566	48.990	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.980%	
26) 1,2-Dichloroethane-d4	5.958	65	73418	51.829	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.660%	
32) Benzene-d6	5.970	84	216672	54.447	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	108.900%	
36) 1,2-Dichloropropane-d6	7.311	67	65471	55.589	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	111.180%	
41) Toluene-d8	8.647	98	181928	50.988	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.980%	
43) trans-1,3-Dichloroprop...	8.951	79	27106	49.180	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	98.360%	
47) 2-Hexanone-d5	9.384	63	59592	113.167	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	113.170%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	93261	54.996	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	110.000%	
66) 1,2-Dichlorobenzene-d4	12.317	152	56349	56.797	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	113.600%	
Target Compounds						Qvalue
13) Acetone	2.392	43	3087	5.312	ug/L	99
61) 1,2,3-Trichloropropane	12.018	75	6772	5.576	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042607.D
Acq On : 26 Jul 2024 18:52
Operator : JC/MD
Sample : P3334-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 27 01:34:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 01:23:37 2024
Response via : Initial Calibration

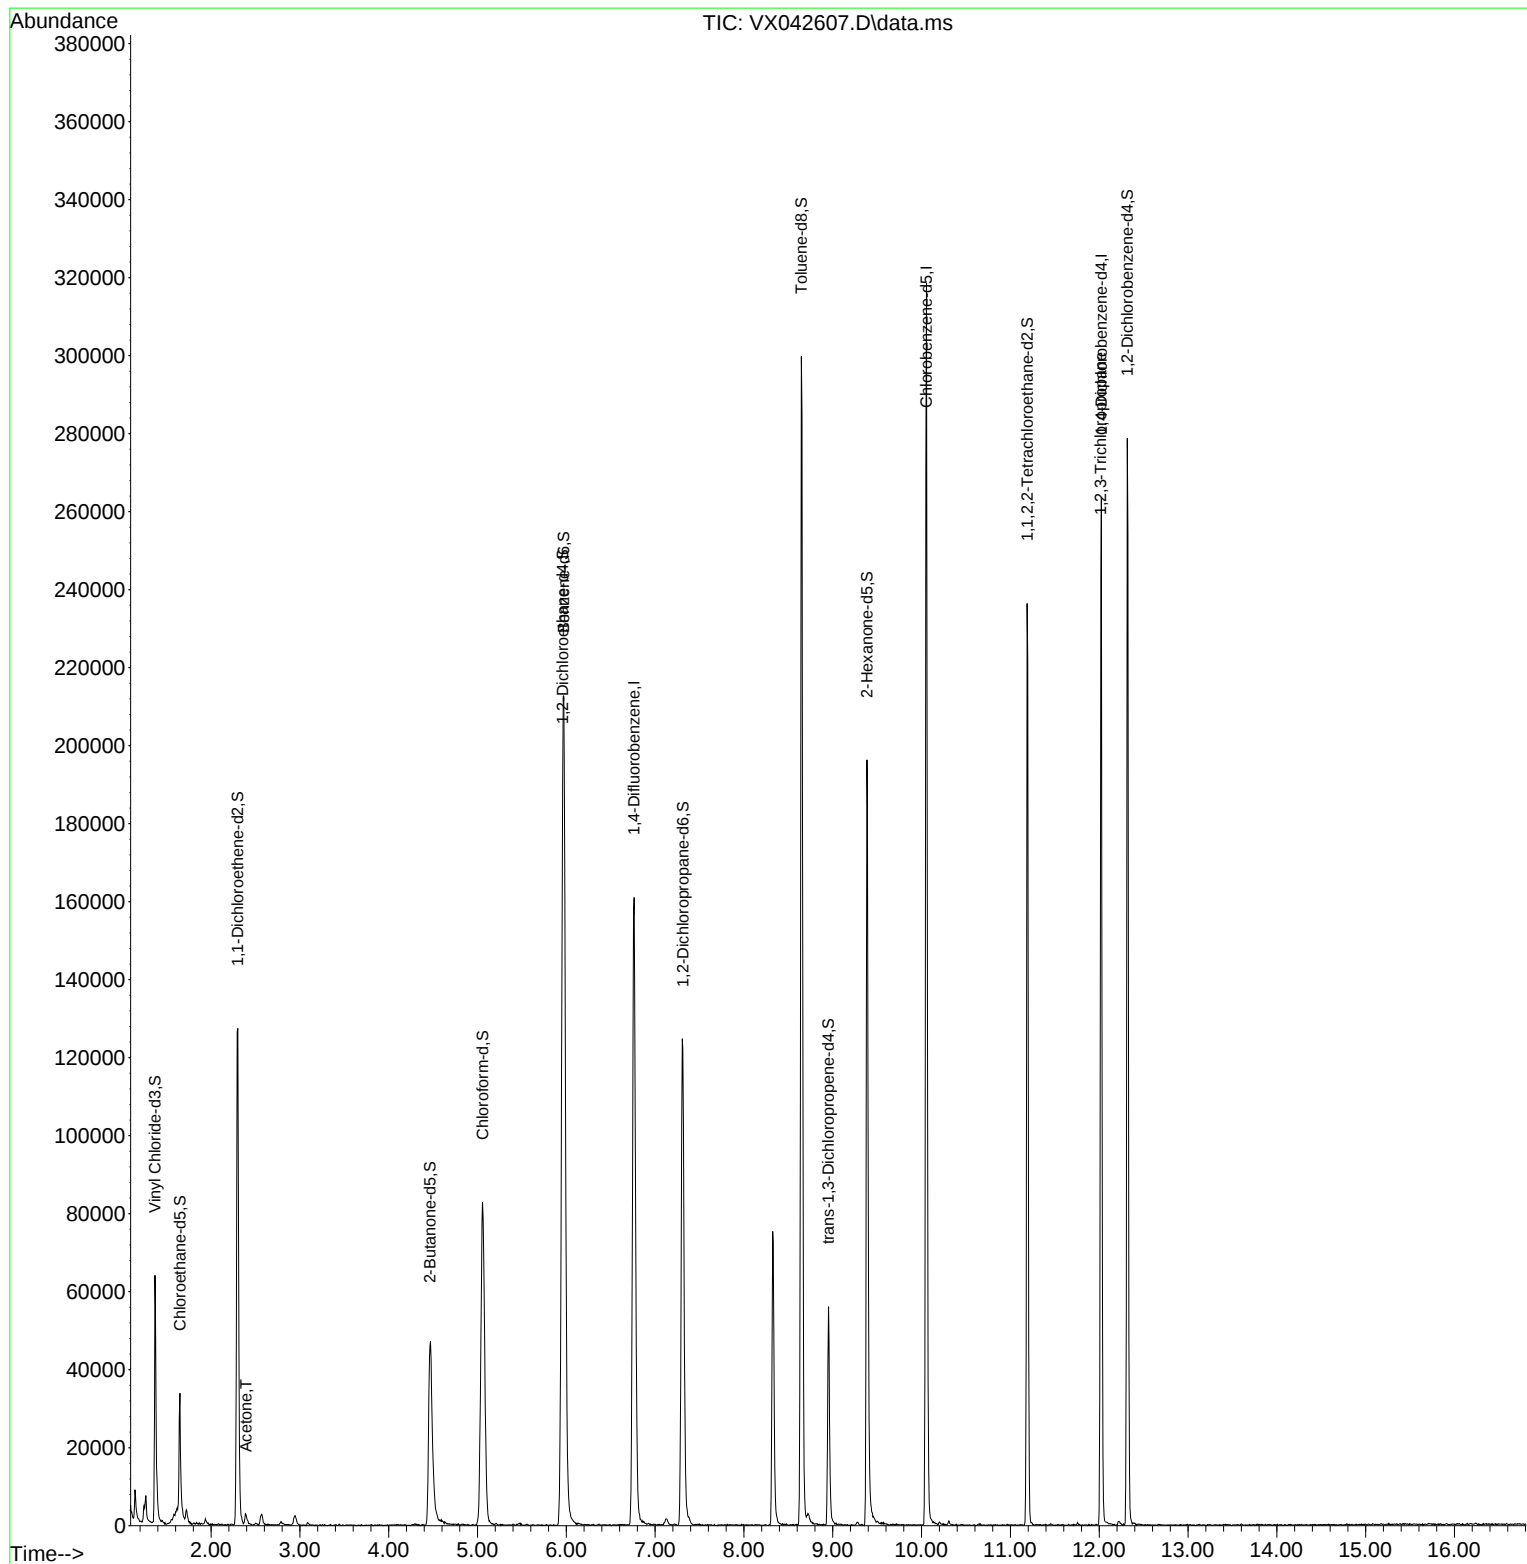



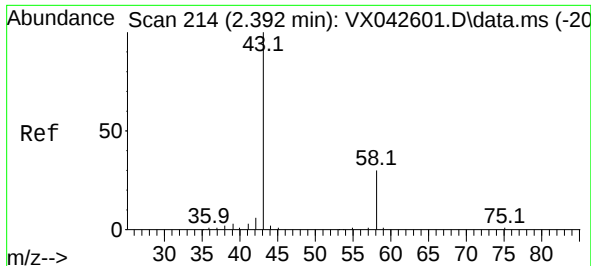


#13
Acetone
Concen: 5.312 ug/L
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX042607.D
Acq: 26 Jul 2024 18:52

Instrument :
MSVOA_X
ClientSampleId :

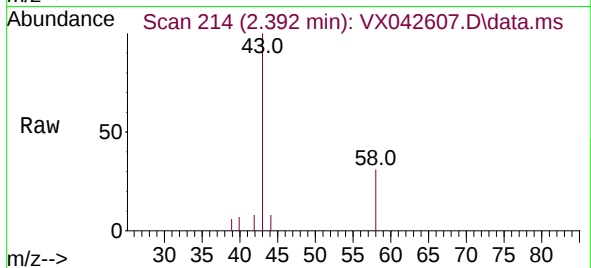

Tgt Ion: 43 Resp: 3087
Ion Ratio Lower Upper
43 100
58 31.9 0.0 62.4

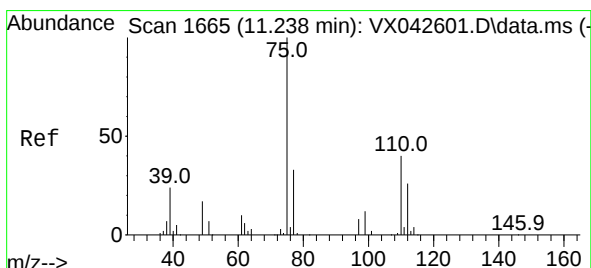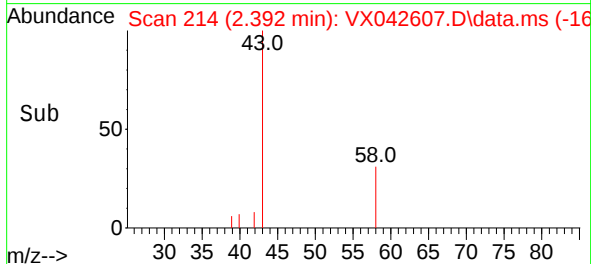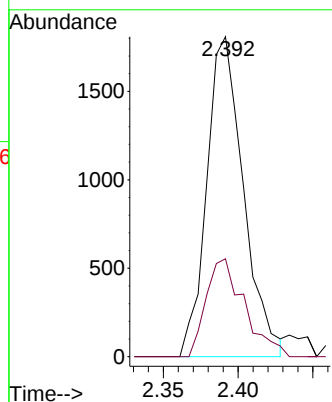

#61
1,2,3-Trichloropropane
Concen: 5.576 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX042607.D
Acq: 26 Jul 2024 18:52

Tgt Ion: 75 Resp: 6772
Ion Ratio Lower Upper
75 100
77 34.5 26.2 39.4
110 5.4 33.0 49.4#

