

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042618.D
 Acq On : 26 Jul 2024 23:08
 Operator : JC/MD
 Sample : P3335-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 27 01:37:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 01:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	156207	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	139286	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	55222	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	38802	40.887	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.780%
7) Chloroethane-d5	1.648	69	19174	49.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.060%
11) 1,1-Dichloroethene-d2	2.294	65	21716	46.443	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.880%
21) 2-Butanone-d5	4.459	46	68989	98.084	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.080%
24) Chloroform-d	5.062	84	99736	48.014	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.020%
26) 1,2-Dichloroethane-d4	5.952	65	65262	48.699	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.400%
32) Benzene-d6	5.971	84	201481	52.121	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.240%
36) 1,2-Dichloropropane-d6	7.306	67	60459	52.845	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.700%
41) Toluene-d8	8.647	98	177176	51.119	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.240%
43) trans-1,3-Dichloroprop...	8.952	79	24302	45.391	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.780%
47) 2-Hexanone-d5	9.385	63	50366	98.464	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.460%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	84659	51.394	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.780%
66) 1,2-Dichlorobenzene-d4	12.317	152	58863	56.402	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.800%
Target Compounds						
					Qvalue	
13) Acetone	2.386	43	2124	3.863	ug/L	92
37) 1,2-Dichloropropane	7.306	63	6461	5.832	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042618.D
Acq On : 26 Jul 2024 23:08
Operator : JC/MD
Sample : P3335-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 27 01:37:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 01:23:37 2024
Response via : Initial Calibration

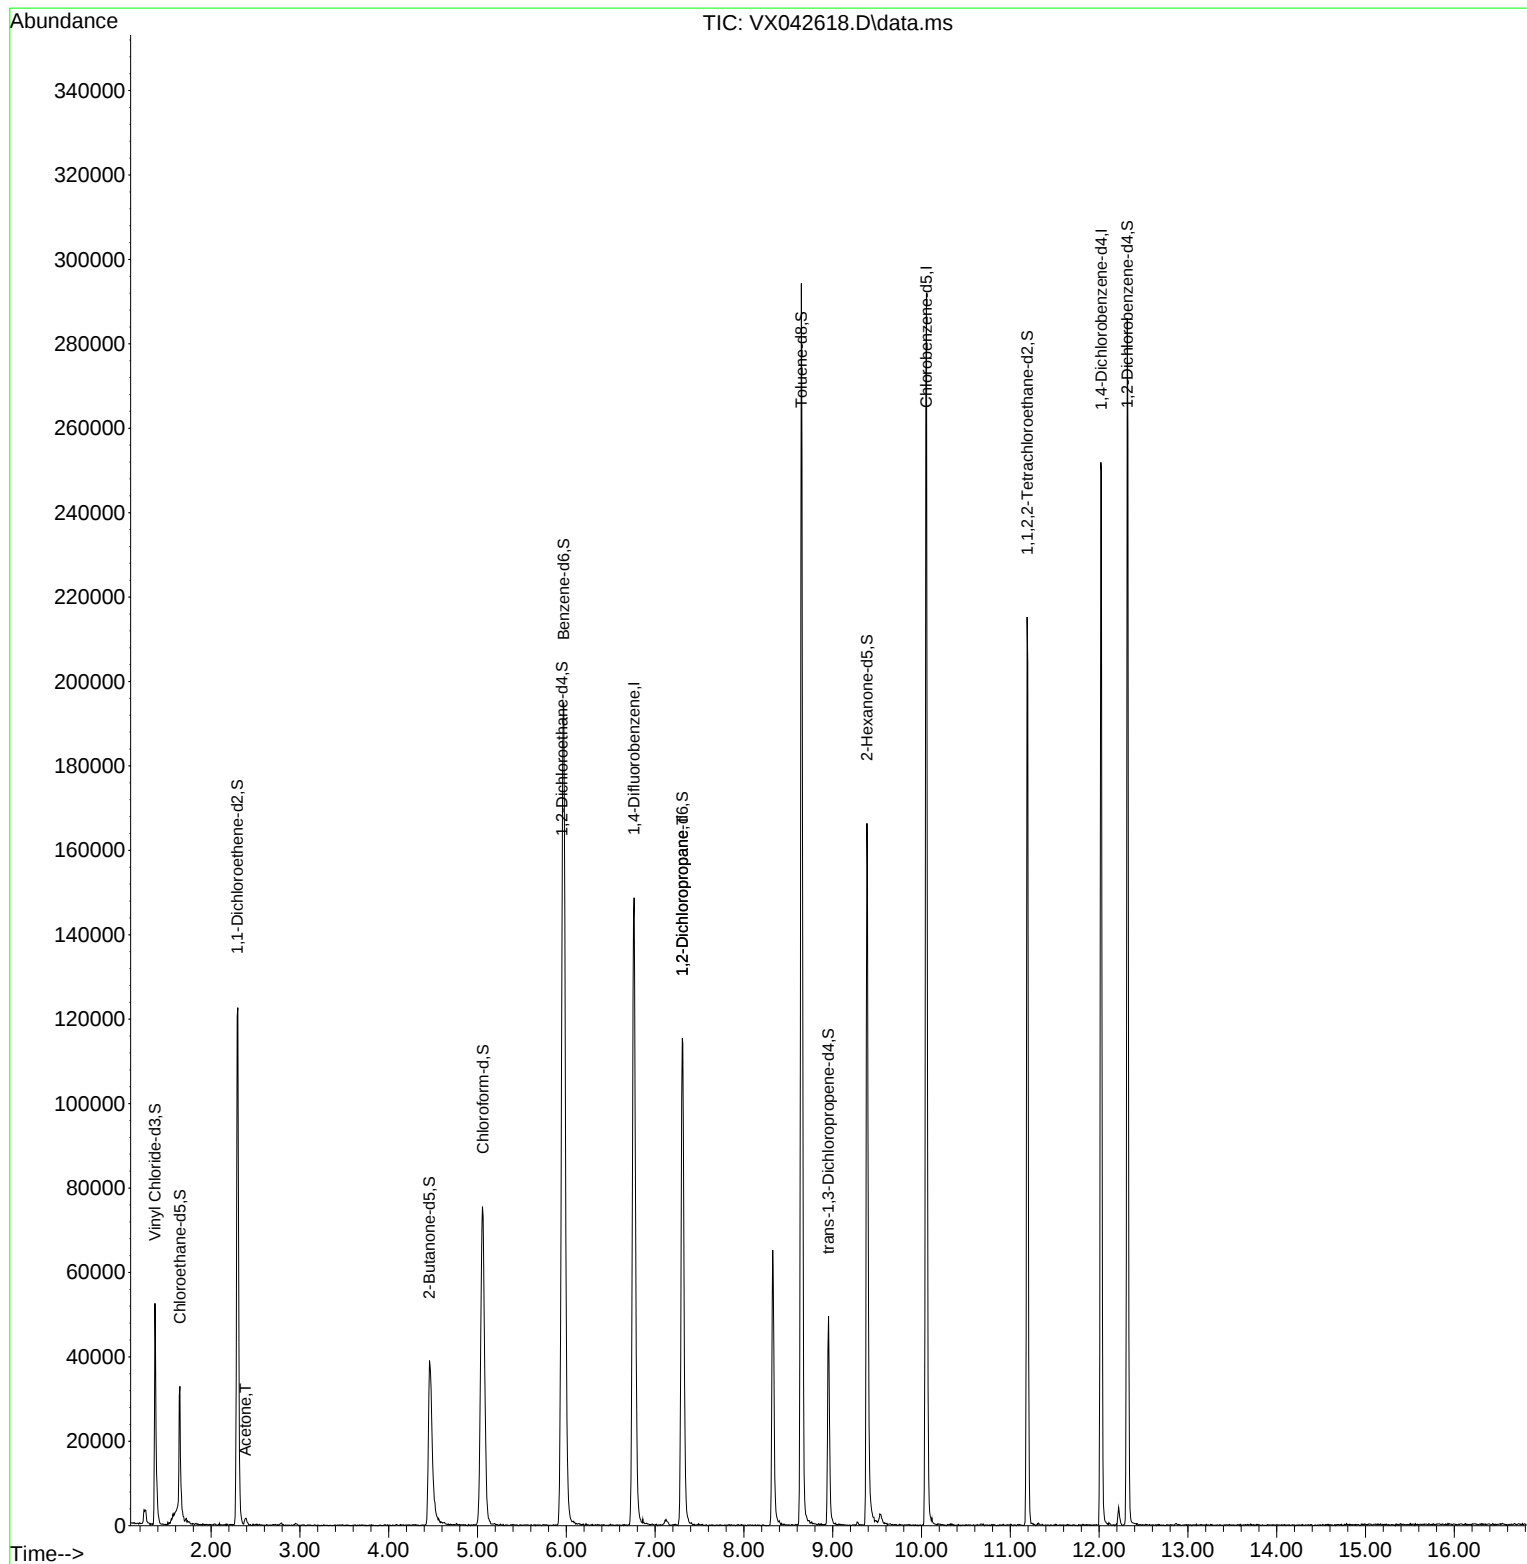

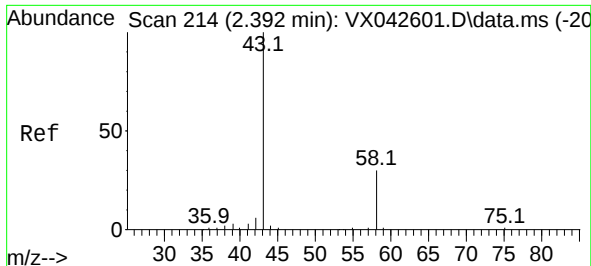

#13

Acetone

Concen: 3.863 ug/L

RT: 2.386 min Scan# 21

Delta R.T. -0.006 min


Lab File: VX042618.D

Acq: 26 Jul 2024 23:08

Instrument :

MSVOA_X

ClientSampleId :



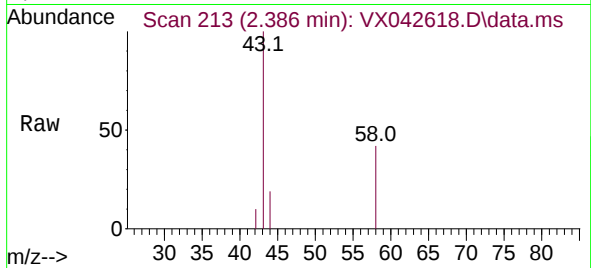


Tgt Ion: 43 Resp: 2124

Ion Ratio Lower Upper

43 100

58 35.7 0.0 62.4

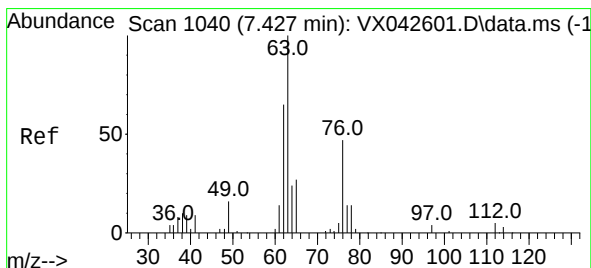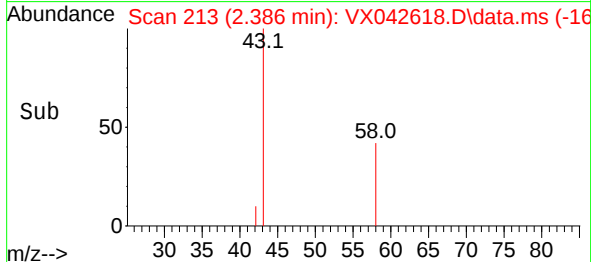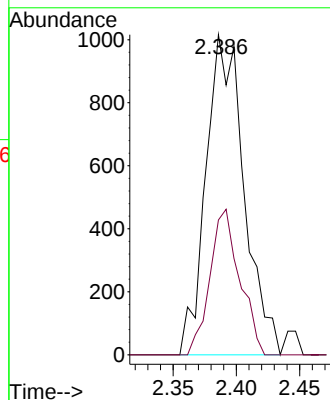

#37

1,2-Dichloropropane

Concen: 5.832 ug/L

RT: 7.306 min Scan# 1020

Delta R.T. -0.122 min

Lab File: VX042618.D

Acq: 26 Jul 2024 23:08

Tgt Ion: 63 Resp: 6461

Ion Ratio Lower Upper

63 100

112 0.0 3.7 5.5#

