

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072824\  
 Data File : VX042632.D  
 Acq On : 27 Jul 2024 04:31  
 Operator : JC/MD  
 Sample : P3328-01ME  
 Misc : 8.79g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 42 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: Jul 29 01:29:09 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML072624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Jul 27 03:03:38 2024  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc     | Units | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|-------|----------|
| -----                         |                |      |            |          |       |          |
| Internal Standards            |                |      |            |          |       |          |
| 1) 1,4-Difluorobenzene        | 6.757          | 114  | 163769     | 50.000   | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 10.055         | 117  | 147323     | 50.000   | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 59699      | 50.000   | ug/L  | 0.00     |
|                               |                |      |            |          |       |          |
| System Monitoring Compounds   |                |      |            |          |       |          |
| 4) Vinyl Chloride-d3          | 1.392          | 65   | 29725      | 29.876   | ug/L  | 0.02     |
| Spiked Amount 50.000          | Range 60 - 135 |      | Recovery = | 59.760%# |       |          |
| 7) Chloroethane-d5            | 1.648          | 69   | 3325       | 8.110    | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 70 - 130 |      | Recovery = | 16.220%# |       |          |
| 11) 1,1-Dichloroethene-d2     | 2.276          | 65   | 14176      | 28.917   | ug/L  | -0.02    |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 57.840%# |       |          |
| 21) 2-Butanone-d5             | 4.489          | 46   | 46628      | 63.231   | ug/L  | 0.02     |
| Spiked Amount 100.000         | Range 40 - 130 |      | Recovery = | 63.230%  |       |          |
| 24) Chloroform-d              | 5.056          | 84   | 75826      | 34.818   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 69.640%# |       |          |
| 26) 1,2-Dichloroethane-d4     | 5.952          | 65   | 50855      | 36.196   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 72.400%  |       |          |
| 32) Benzene-d6                | 5.964          | 84   | 157024     | 38.404   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 76.800%  |       |          |
| 36) 1,2-Dichloropropane-d6    | 7.306          | 67   | 45570      | 37.658   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 70 - 120 |      | Recovery = | 75.320%  |       |          |
| 41) Toluene-d8                | 8.647          | 98   | 136389     | 37.204   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 74.400%# |       |          |
| 43) trans-1,3-Dichloroprop... | 8.952          | 79   | 16801      | 29.669   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 59.340%# |       |          |
| 47) 2-Hexanone-d5             | 9.391          | 63   | 36906      | 68.214   | ug/L  | 0.00     |
| Spiked Amount 100.000         | Range 45 - 130 |      | Recovery = | 68.210%  |       |          |
| 56) 1,1,2,2-Tetrachloroeth... | 11.195         | 84   | 63914      | 36.683   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 65 - 120 |      | Recovery = | 73.360%  |       |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.323         | 152  | 47302      | 41.926   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 83.860%  |       |          |
|                               |                |      |            |          |       |          |
| Target Compounds              |                |      |            |          |       | Qvalue   |
| 61) 1,2,3-Trichloropropane    | 12.018         | 75   | 6976       | 5.051    | ug/L  | # 64     |
| -----                         |                |      |            |          |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072824\  
Data File : VX042632.D  
Acq On : 27 Jul 2024 04:31  
Operator : JC/MD  
Sample : P3328-01ME  
Misc : 8.79g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 42 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :

Quant Time: Jul 29 01:29:09 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML072624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Jul 27 03:03:38 2024  
Response via : Initial Calibration

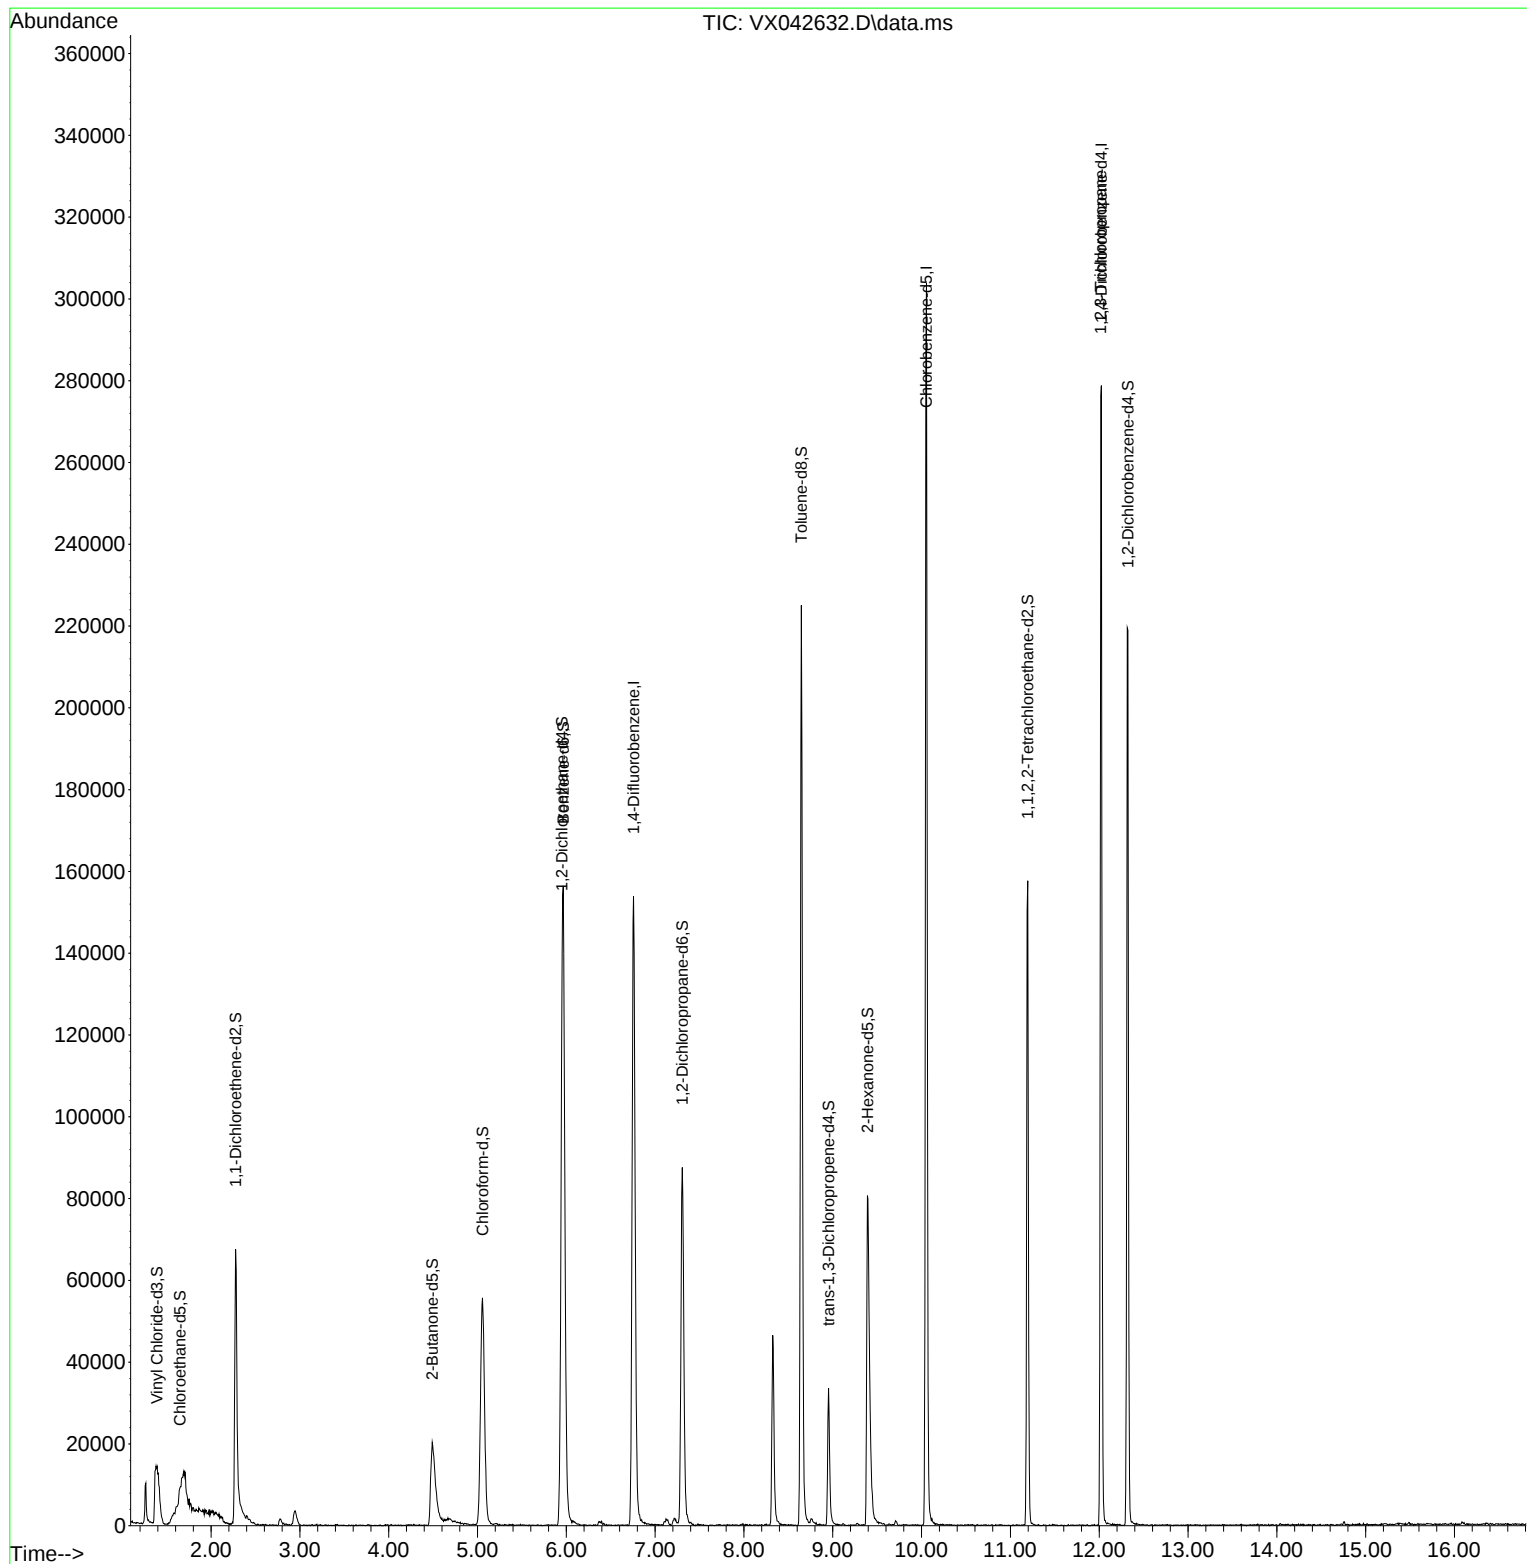

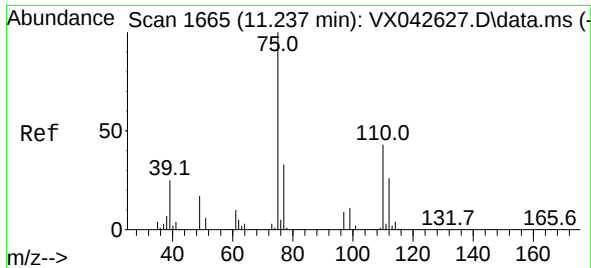

#61

1,2,3-Trichloropropane

Concen: 5.051 ug/L

RT: 12.018 min Scan# 11

Delta R.T. 0.781 min


Lab File: VX042632.D

Acq: 27 Jul 2024 04:31

Instrument :

MSVOA\_X

ClientSampleId :

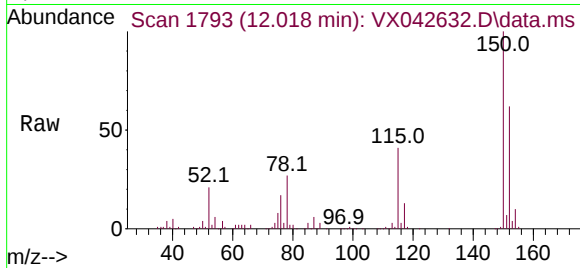

Tgt Ion: 75 Resp: 6976

Ion Ratio Lower Upper

75 100

77 36.4 26.2 39.4

110 4.1 33.0 49.4#

