

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042633.D
 Acq On : 27 Jul 2024 04:53
 Operator : JC/MD
 Sample : P3328-06ME
 Misc : 8.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 01:29:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 03:03:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	135005	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	121444	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	48901	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.386	65	19195	23.403	ug/L	0.02
Spiked Amount	50.000	Range	60 - 135	Recovery	=	46.800%#
7) Chloroethane-d5	1.679	69	2000	5.917	ug/L	0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	11.840%#
11) 1,1-Dichloroethene-d2	2.276	65	8484	20.994	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	41.980%#
21) 2-Butanone-d5	4.495	46	26221	43.134	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	43.130%
24) Chloroform-d	5.062	84	45255	25.208	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	50.420%#
26) 1,2-Dichloroethane-d4	5.952	65	31961	27.595	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	55.180%#
32) Benzene-d6	5.964	84	95588	28.360	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	56.720%#
36) 1,2-Dichloropropane-d6	7.299	67	28091	28.161	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	56.320%#
41) Toluene-d8	8.647	98	82507	27.302	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	54.600%#
43) trans-1,3-Dichloroprop...	8.952	79	9943	21.300	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	42.600%#
47) 2-Hexanone-d5	9.391	63	20872	46.799	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	46.800%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	38088	26.519	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	53.040%#
66) 1,2-Dichlorobenzene-d4	12.323	152	28111	30.418	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	60.840%#
Target Compounds						Qvalue
34) Trichloroethene	7.117	95	53995	54.379	ug/L	96
61) 1,2,3-Trichloropropane	12.018	75	5731	5.066	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042633.D
Acq On : 27 Jul 2024 04:53
Operator : JC/MD
Sample : P3328-06ME
Misc : 8.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 29 01:29:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 03:03:38 2024
Response via : Initial Calibration

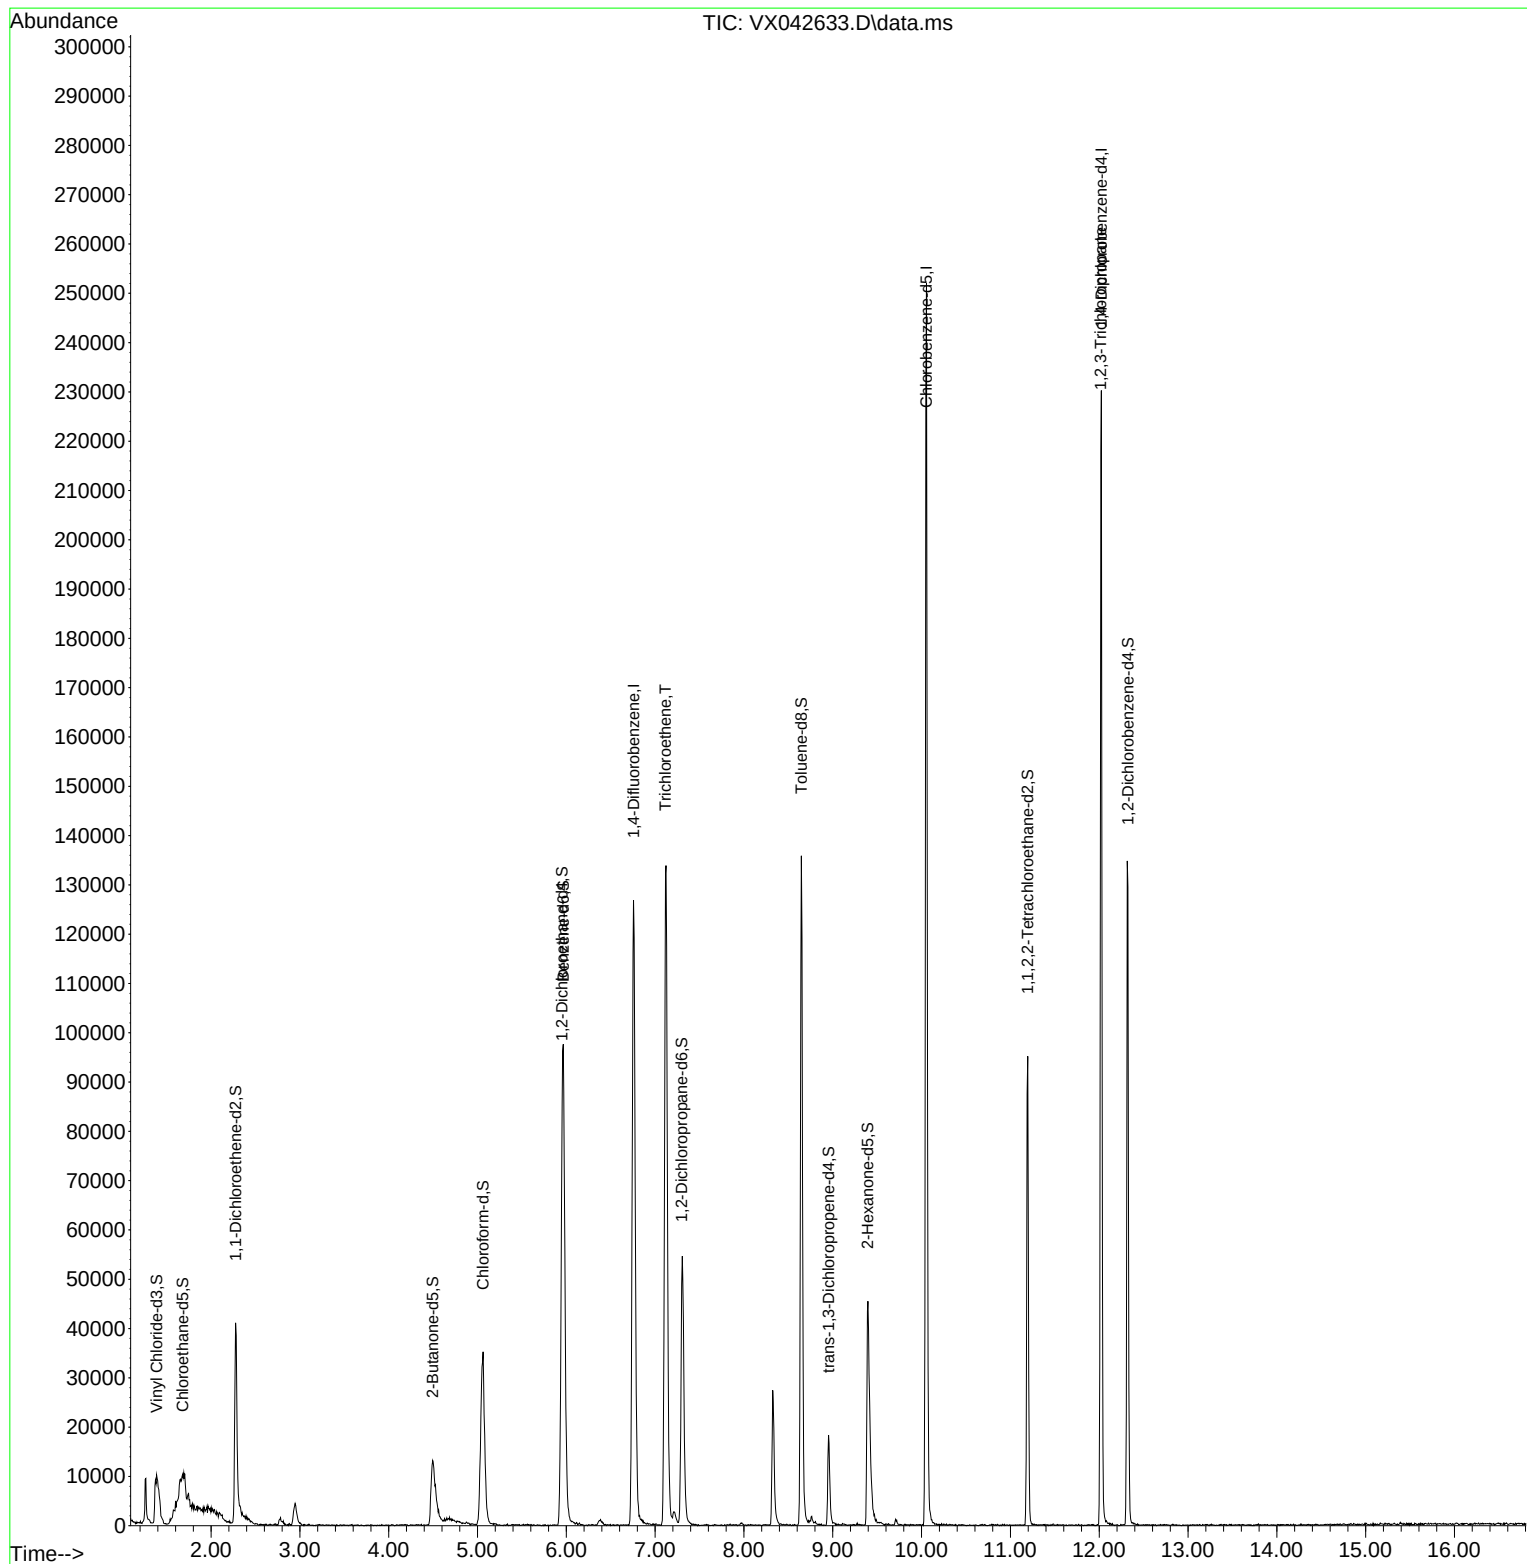



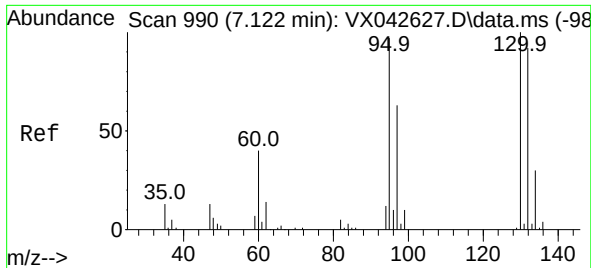


#34
Trichloroethene
Concen: 54.379 ug/L
RT: 7.117 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX042633.D
Acq: 27 Jul 2024 04:53

Instrument :
MSVOA_X
ClientSampleId :

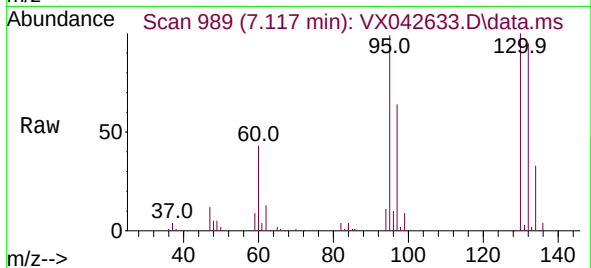

Tgt Ion:	95	Resp:	53995
Ion	Ratio	Lower	Upper
95	100		
97	65.1	46.3	86.1
132	95.8	64.3	119.5
130	101.2	67.0	124.4

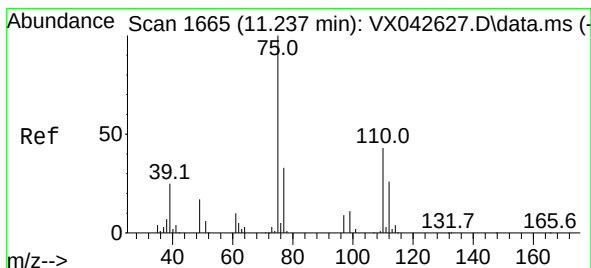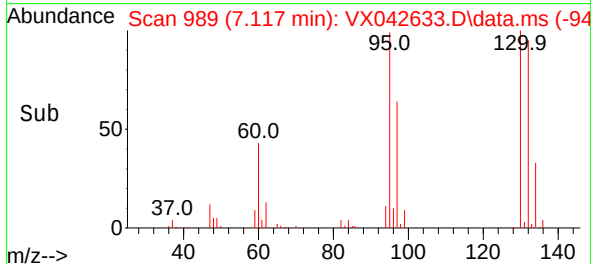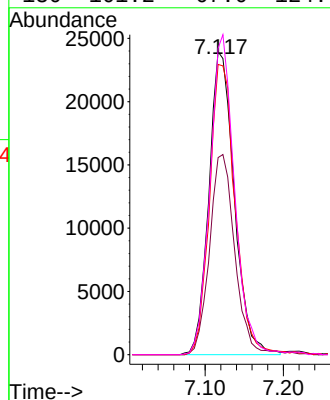

#61
1,2,3-Trichloropropane
Concen: 5.066 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.781 min
Lab File: VX042633.D
Acq: 27 Jul 2024 04:53

Tgt Ion:	75	Resp:	5731
Ion	Ratio	Lower	Upper
75	100		
77	35.5	26.2	39.4
110	2.8	33.0	49.4

