

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042634.D
 Acq On : 27 Jul 2024 05:17
 Operator : JC/MD
 Sample : P3328-08ME
 Misc : 9.02g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 01:29:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 03:03:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	161596	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	146339	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	58756	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.380	65	15712	16.004	ug/L	0.01
Spiked Amount	50.000	Range	60 - 135	Recovery	=	32.000%#
7) Chloroethane-d5	1.654	69	3087	7.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	15.260%#
11) 1,1-Dichloroethene-d2	2.276	65	13150	27.185	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.380%#
21) 2-Butanone-d5	4.495	46	44508	61.168	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	61.170%
24) Chloroform-d	5.056	84	75184	34.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	69.980%#
26) 1,2-Dichloroethane-d4	5.958	65	51474	37.129	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.260%
32) Benzene-d6	5.970	84	153146	37.708	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.420%
36) 1,2-Dichloropropane-d6	7.305	67	46229	38.460	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	76.920%
41) Toluene-d8	8.647	98	136725	37.547	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.100%#
43) trans-1,3-Dichloroprop...	8.951	79	16561	29.441	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.880%#
47) 2-Hexanone-d5	9.397	63	36318	67.578	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.580%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	63247	36.545	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	73.080%
66) 1,2-Dichlorobenzene-d4	12.323	152	45531	41.004	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.000%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.024	75	7074	5.204	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042634.D
Acq On : 27 Jul 2024 05:17
Operator : JC/MD
Sample : P3328-08ME
Misc : 9.02g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 29 01:29:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 03:03:38 2024
Response via : Initial Calibration

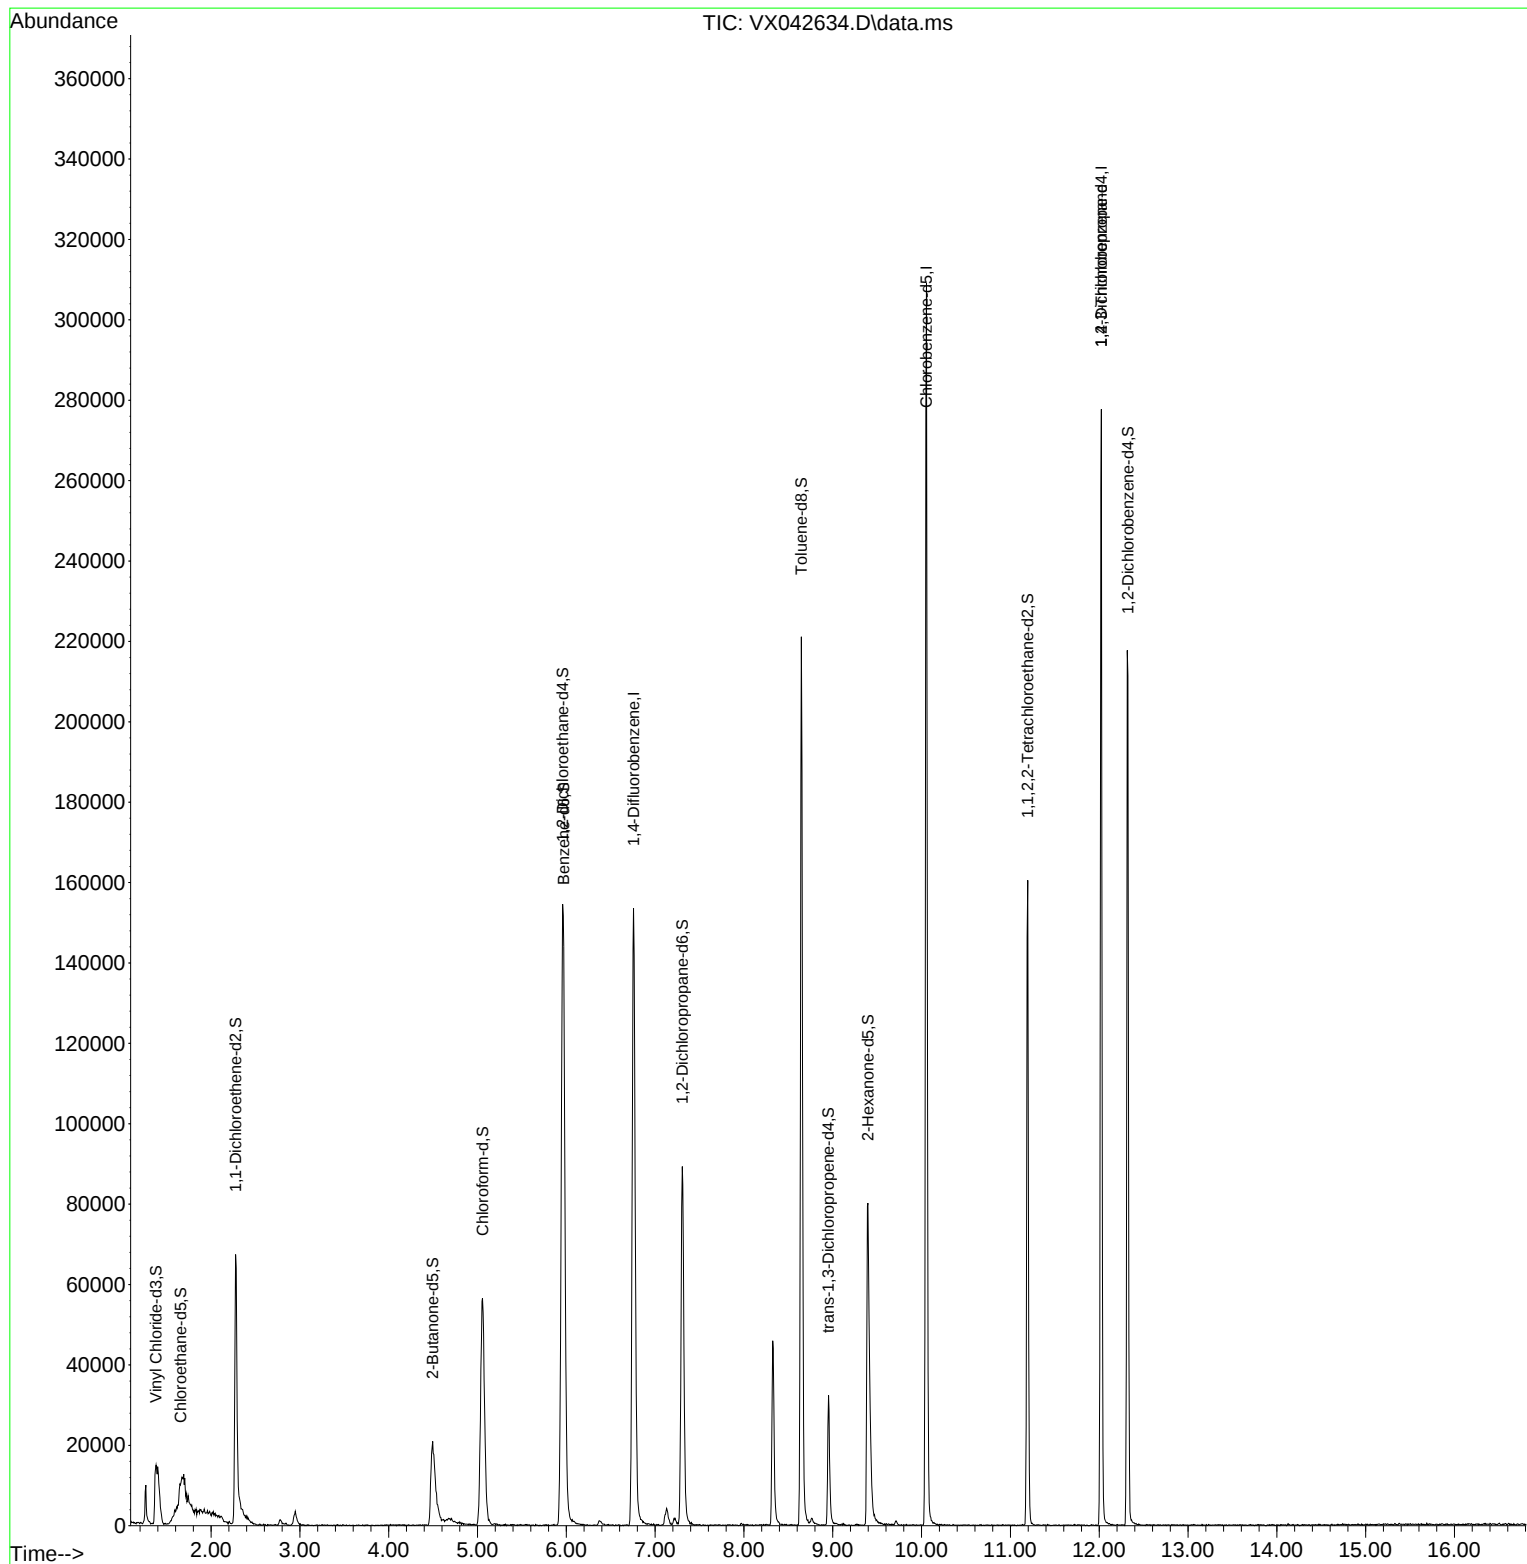

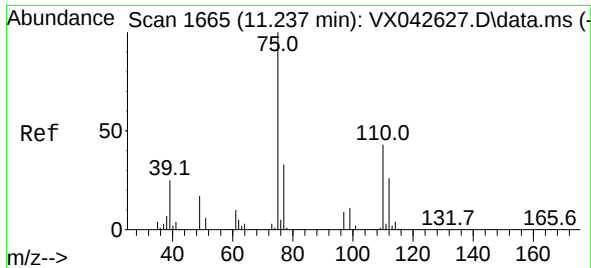

#61

1,2,3-Trichloropropane

Concen: 5.204 ug/L

RT: 12.024 min Scan# 11

Delta R.T. 0.787 min


Lab File: VX042634.D

Acq: 27 Jul 2024 05:17

Instrument :

MSVOA_X

ClientSampleId :

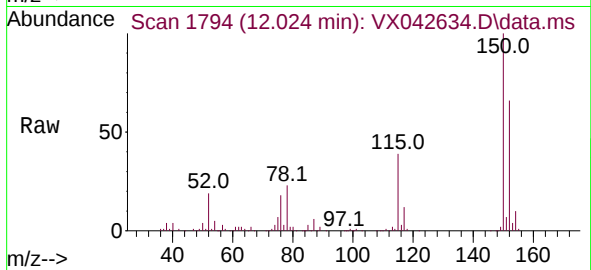

Tgt Ion: 75 Resp: 7074

Ion Ratio Lower Upper

75 100

77 37.2 26.2 39.4

110 3.3 33.0 49.4#

