

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042648.D
 Acq On : 27 Jul 2024 19:36
 Operator : JC/MD
 Sample : P3373-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 02:46:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 02:34:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	177747	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	160936	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	60933	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	34605	32.045	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.100%		
7) Chloroethane-d5	1.648	69	17962	40.365	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.740%		
11) 1,1-Dichloroethene-d2	2.300	65	20190	37.947	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.900%		
21) 2-Butanone-d5	4.465	46	67614	84.480	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.480%		
24) Chloroform-d	5.056	84	95739	40.505	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.000%		
26) 1,2-Dichloroethane-d4	5.958	65	63396	41.574	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.140%		
32) Benzene-d6	5.971	84	187307	41.936	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.880%		
36) 1,2-Dichloropropane-d6	7.312	67	57308	43.352	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.700%		
41) Toluene-d8	8.647	98	163334	40.786	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.580%		
43) trans-1,3-Dichloroprop...	8.952	79	22955	37.107	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.220%		
47) 2-Hexanone-d5	9.385	63	49158	83.174	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.170%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	80793	42.449	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.900%		
66) 1,2-Dichlorobenzene-d4	12.317	152	53443	46.409	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.820%		
Target Compounds					Qvalue	
13) Acetone	2.386	43	1779	2.844	ug/L	93
61) 1,2,3-Trichloropropane	12.024	75	7356	5.218	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042648.D
Acq On : 27 Jul 2024 19:36
Operator : JC/MD
Sample : P3373-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 29 02:46:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 02:34:37 2024
Response via : Initial Calibration

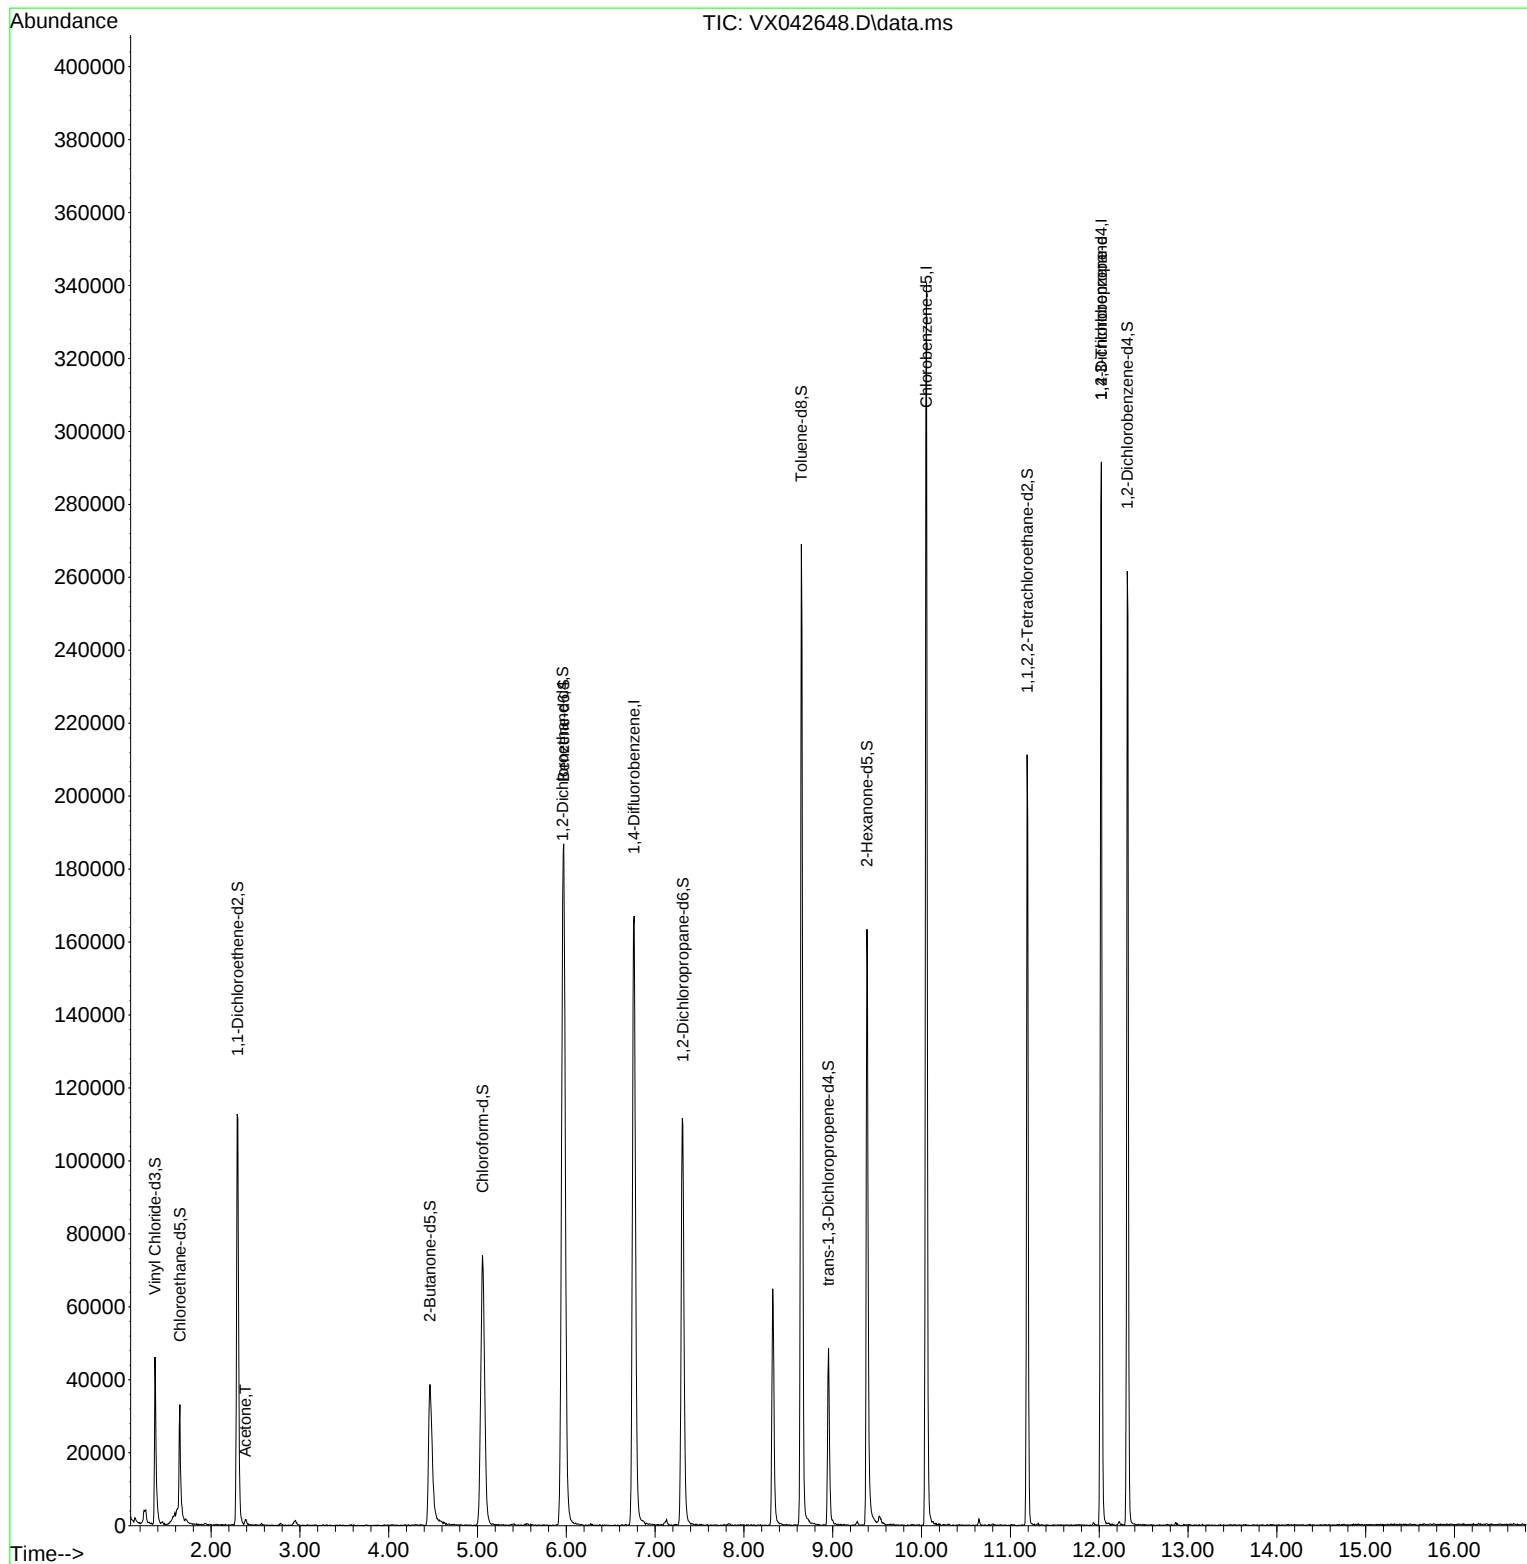

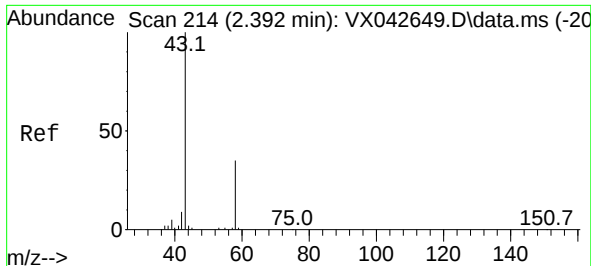

#13

Acetone

Concen: 2.844 ug/L

RT: 2.386 min Scan# 21

Delta R.T. -0.006 min


Lab File: VX042648.D

Acq: 27 Jul 2024 19:36

Instrument :

MSVOA_X

ClientSampleId :



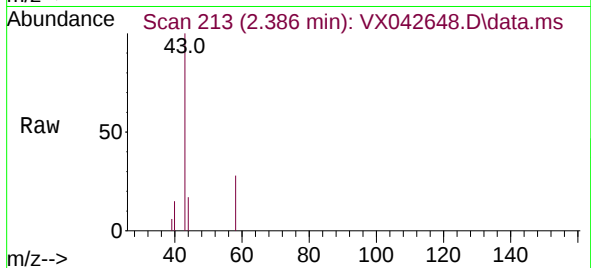


Tgt Ion: 43 Resp: 1779

Ion Ratio Lower Upper

43 100

58 34.8 0.0 62.4

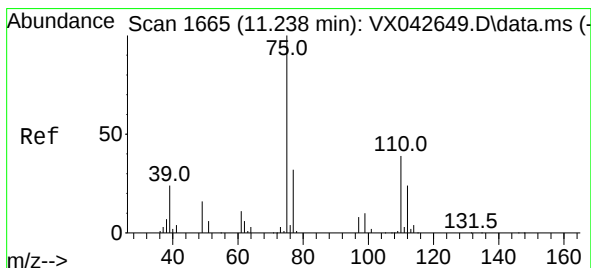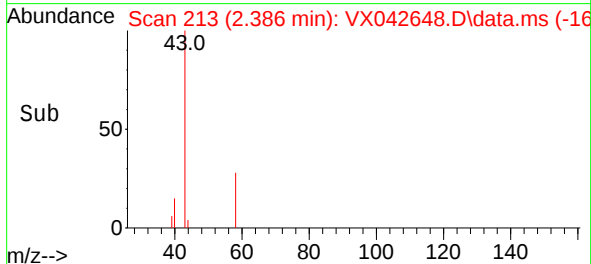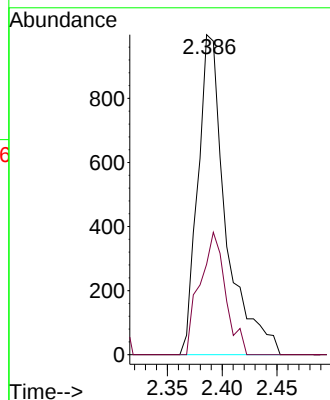

#61

1,2,3-Trichloropropane

Concen: 5.218 ug/L

RT: 12.024 min Scan# 1794

Delta R.T. 0.787 min

Lab File: VX042648.D

Acq: 27 Jul 2024 19:36

Tgt Ion: 75 Resp: 7356

Ion Ratio Lower Upper

75 100

77 34.2 26.2 39.4

110 3.4 33.0 49.4#

