

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042651.D
 Acq On : 27 Jul 2024 20:45
 Operator : JC/MD
 Sample : VX0728WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 03:11:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	165236	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	146242	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	56292	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	38404	38.256	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.520%		
7) Chloroethane-d5	1.648	69	18471	44.652	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.300%		
11) 1,1-Dichloroethene-d2	2.294	65	21275	43.013	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.020%		
21) 2-Butanone-d5	4.471	46	71322	95.860	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.860%		
24) Chloroform-d	5.056	84	100496	45.736	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.480%		
26) 1,2-Dichloroethane-d4	5.958	65	67274	47.457	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.920%		
32) Benzene-d6	5.971	84	197921	48.764	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.520%		
36) 1,2-Dichloropropane-d6	7.306	67	60117	50.047	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.100%		
41) Toluene-d8	8.647	98	169965	46.706	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.420%		
43) trans-1,3-Dichloroprop...	8.952	79	23141	41.166	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.340%		
47) 2-Hexanone-d5	9.385	63	52494	97.743	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.740%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	84765	49.010	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.020%		
66) 1,2-Dichlorobenzene-d4	12.323	152	55193	51.880	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.760%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	7.312	63	6848	5.888	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042651.D
Acq On : 27 Jul 2024 20:45
Operator : JC/MD
Sample : VX0728WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 29 03:11:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration

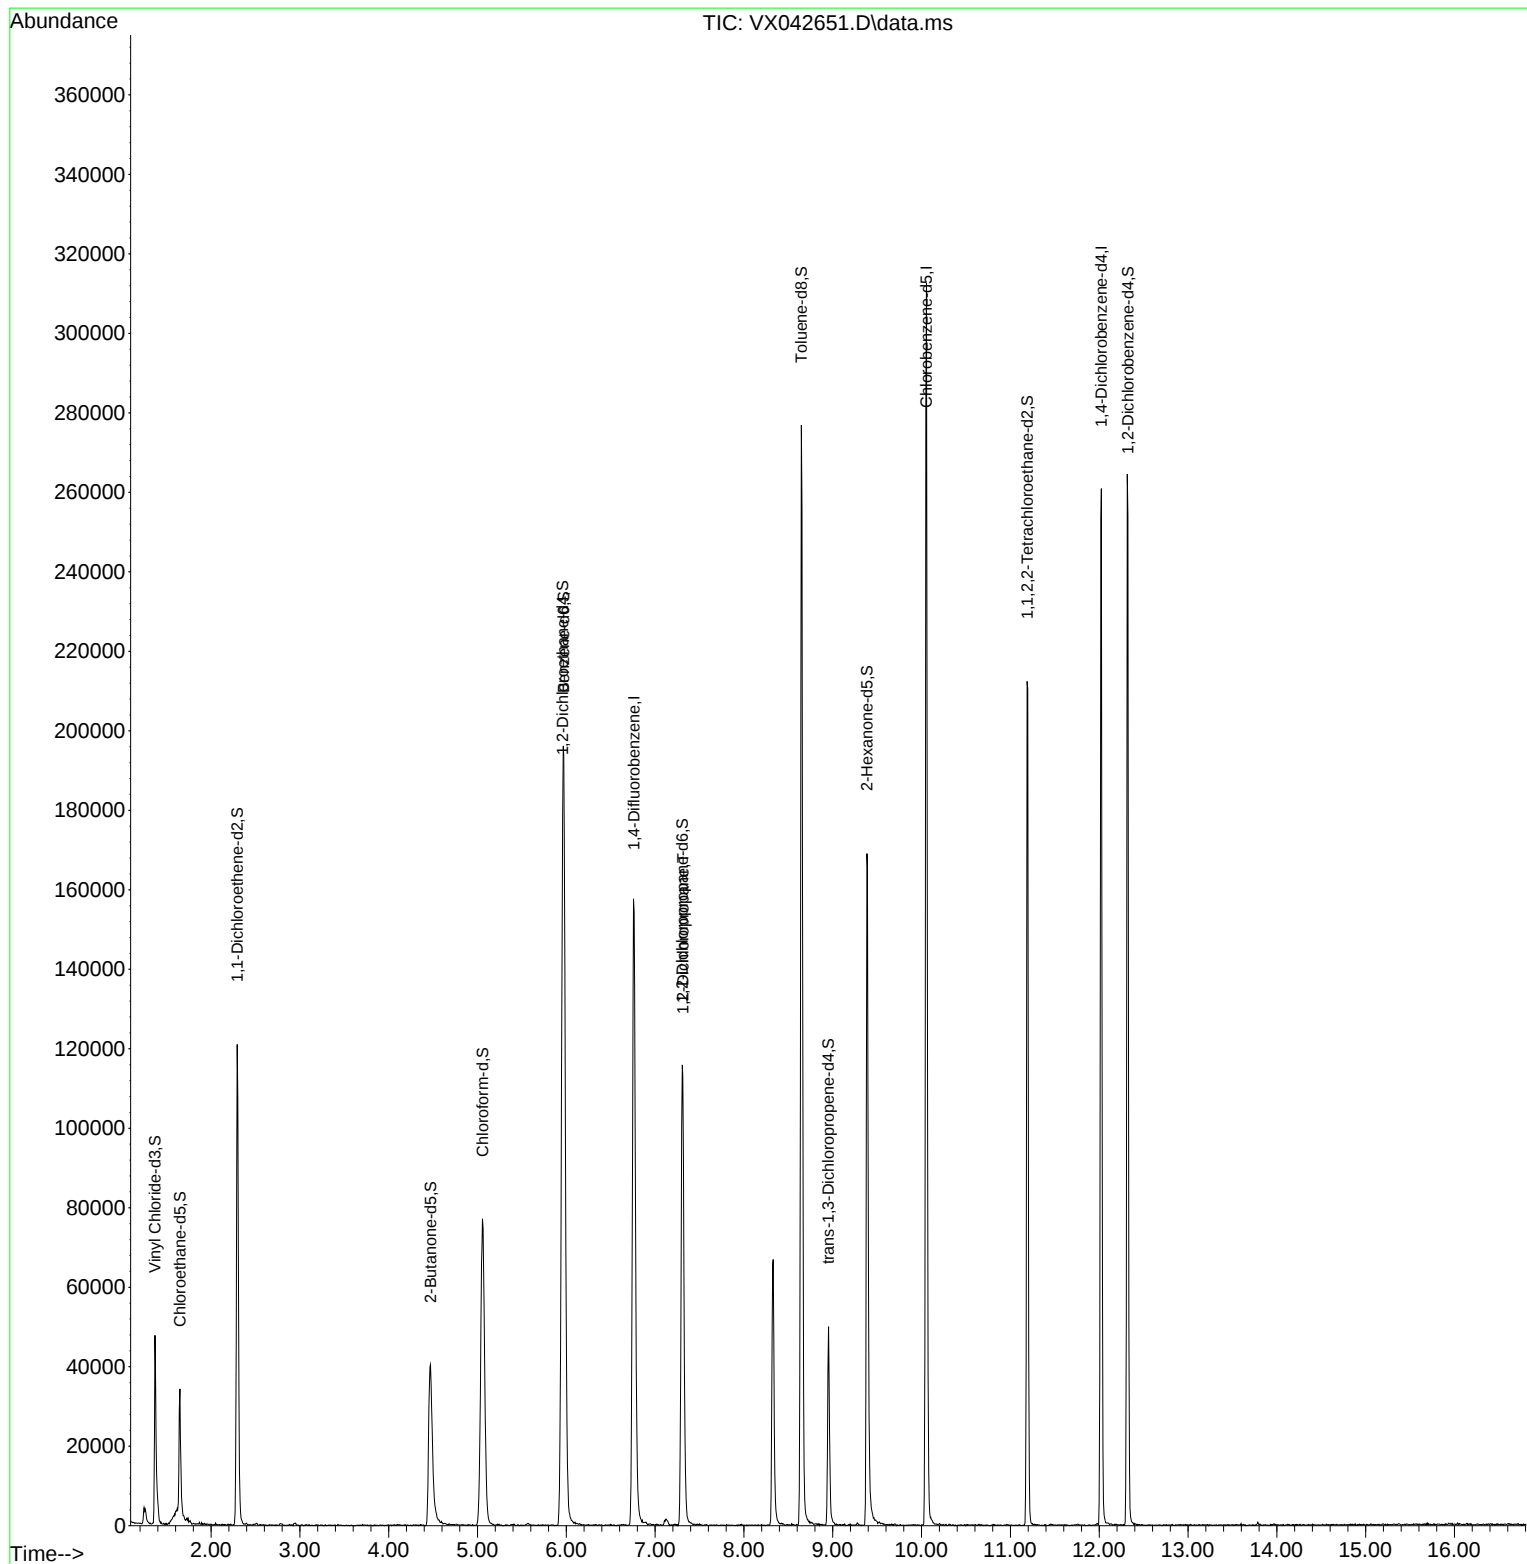

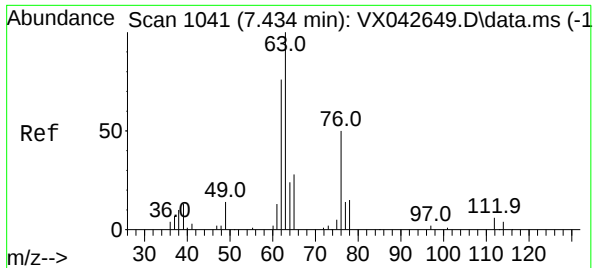

#37
 1,2-Dichloropropane
 Concen: 5.888 ug/L
 RT: 7.312 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX042651.D
 Acq: 27 Jul 2024 20:45

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 6848
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.7 5.5#

