

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042658.D
 Acq On : 27 Jul 2024 23:28
 Operator : JC/MD
 Sample : P3388-08 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 04:25:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	169882	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	151696	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	57556	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	37188	36.032	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.060%		
7) Chloroethane-d5	1.648	69	17605	41.395	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.780%		
11) 1,1-Dichloroethene-d2	2.294	65	20732	40.769	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.540%		
21) 2-Butanone-d5	4.465	46	72989	95.417	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.420%		
24) Chloroform-d	5.056	84	100340	44.417	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.840%		
26) 1,2-Dichloroethane-d4	5.958	65	67711	46.459	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.920%		
32) Benzene-d6	5.970	84	196564	46.689	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.380%		
36) 1,2-Dichloropropane-d6	7.306	67	60448	48.513	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.020%		
41) Toluene-d8	8.647	98	169269	44.842	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.680%		
43) trans-1,3-Dichloroprop...	8.952	79	24105	41.340	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.680%		
47) 2-Hexanone-d5	9.384	63	50808	91.202	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.200%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	84840	47.290	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.580%		
66) 1,2-Dichlorobenzene-d4	12.317	152	54538	50.139	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.280%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.306	63	6902	5.721	ug/L #	86
61) 1,2,3-Trichloropropane	12.018	75	7404	5.560	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042658.D
Acq On : 27 Jul 2024 23:28
Operator : JC/MD
Sample : P3388-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 29 04:25:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration




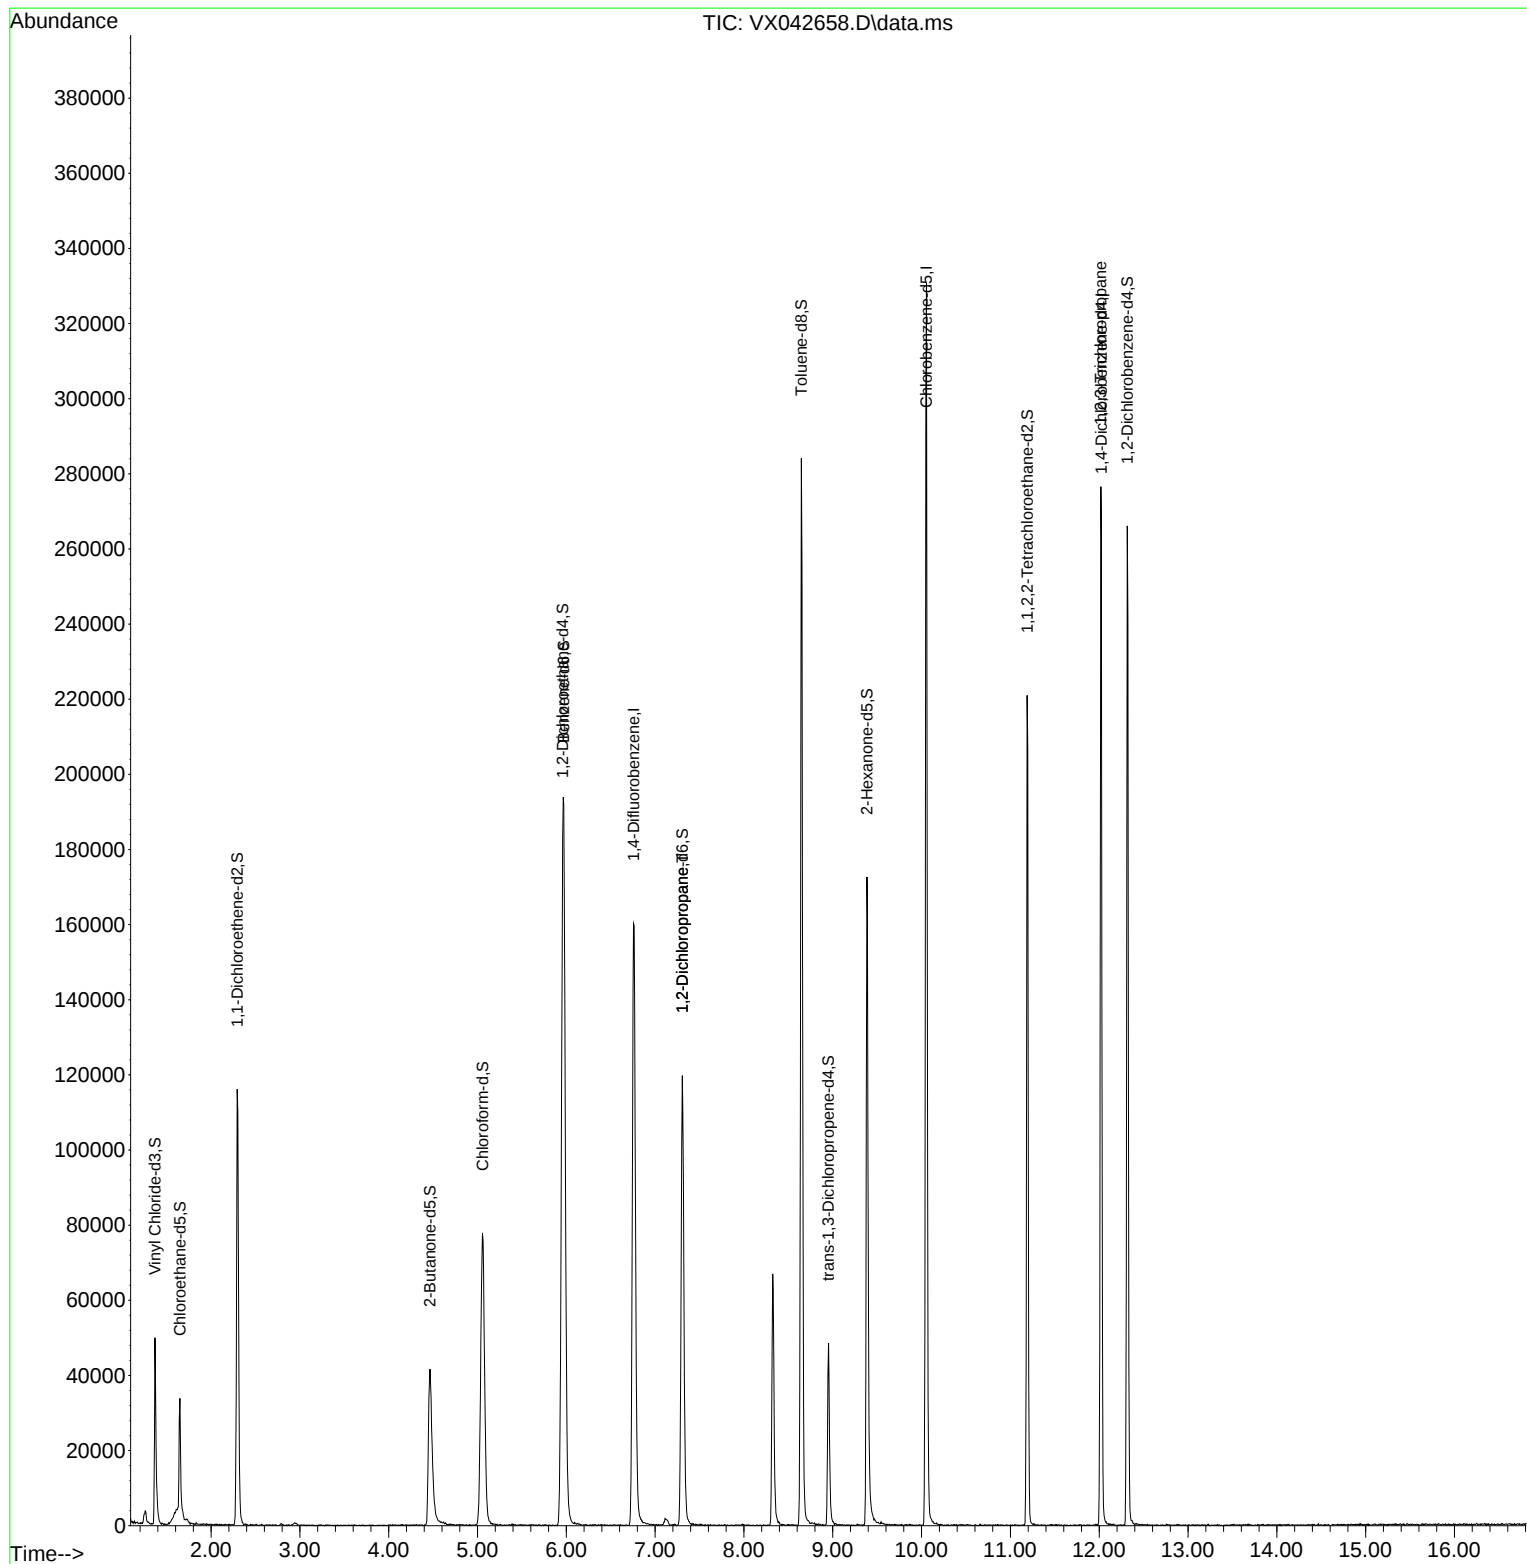


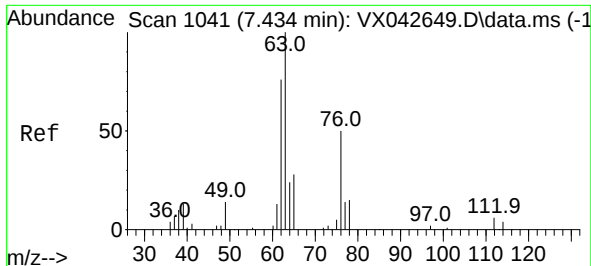

#37
1,2-Dichloropropane
Concen: 5.721 ug/L
RT: 7.306 min Scan# 1
Delta R.T. -0.128 min
Lab File: VX042658.D
Acq: 27 Jul 2024 23:28

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 6902
Ion Ratio Lower Upper
63 100
112 0.0 3.7 5.5#

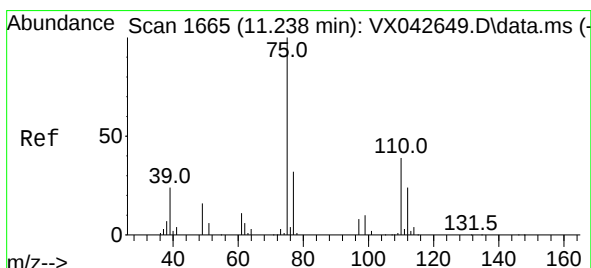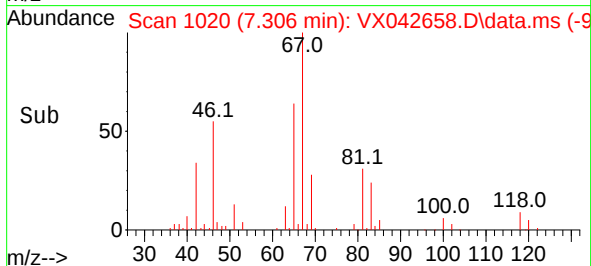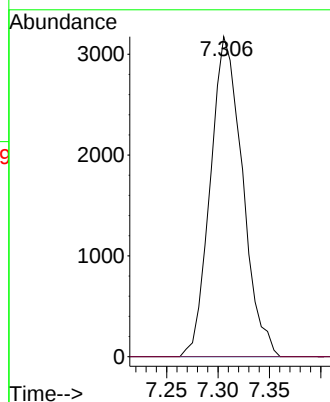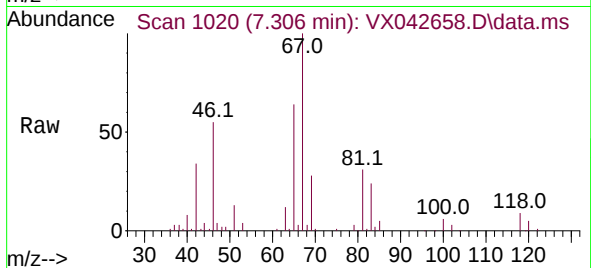

#61
1,2,3-Trichloropropane
Concen: 5.560 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX042658.D
Acq: 27 Jul 2024 23:28

Tgt Ion: 75 Resp: 7404
Ion Ratio Lower Upper
75 100
77 29.7 26.2 39.4
110 2.6 33.0 49.4#

