

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042665.D
 Acq On : 28 Jul 2024 02:09
 Operator : JC/MD
 Sample : P3388-17 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 04:26:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	174162	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	157598	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	62624	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	33972	32.107	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	64.220%
7) Chloroethane-d5	1.648	69	16317	37.423	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	74.840%
11) 1,1-Dichloroethene-d2	2.294	65	19669	37.728	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.460%
21) 2-Butanone-d5	4.464	46	66693	85.044	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.040%
24) Chloroform-d	5.056	84	92832	40.083	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.160%
26) 1,2-Dichloroethane-d4	5.952	65	63538	42.525	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.040%
32) Benzene-d6	5.970	84	184806	42.252	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.500%
36) 1,2-Dichloropropane-d6	7.305	67	57350	44.303	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.600%
41) Toluene-d8	8.647	98	158040	40.300	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.600%
43) trans-1,3-Dichloroprop...	8.951	79	22389	36.959	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.920%
47) 2-Hexanone-d5	9.384	63	48799	84.315	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.320%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	81550	43.754	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.500%
66) 1,2-Dichlorobenzene-d4	12.317	152	53311	45.045	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.080%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.018	75	7716	5.326	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042665.D
Acq On : 28 Jul 2024 02:09
Operator : JC/MD
Sample : P3388-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 29 04:26:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration

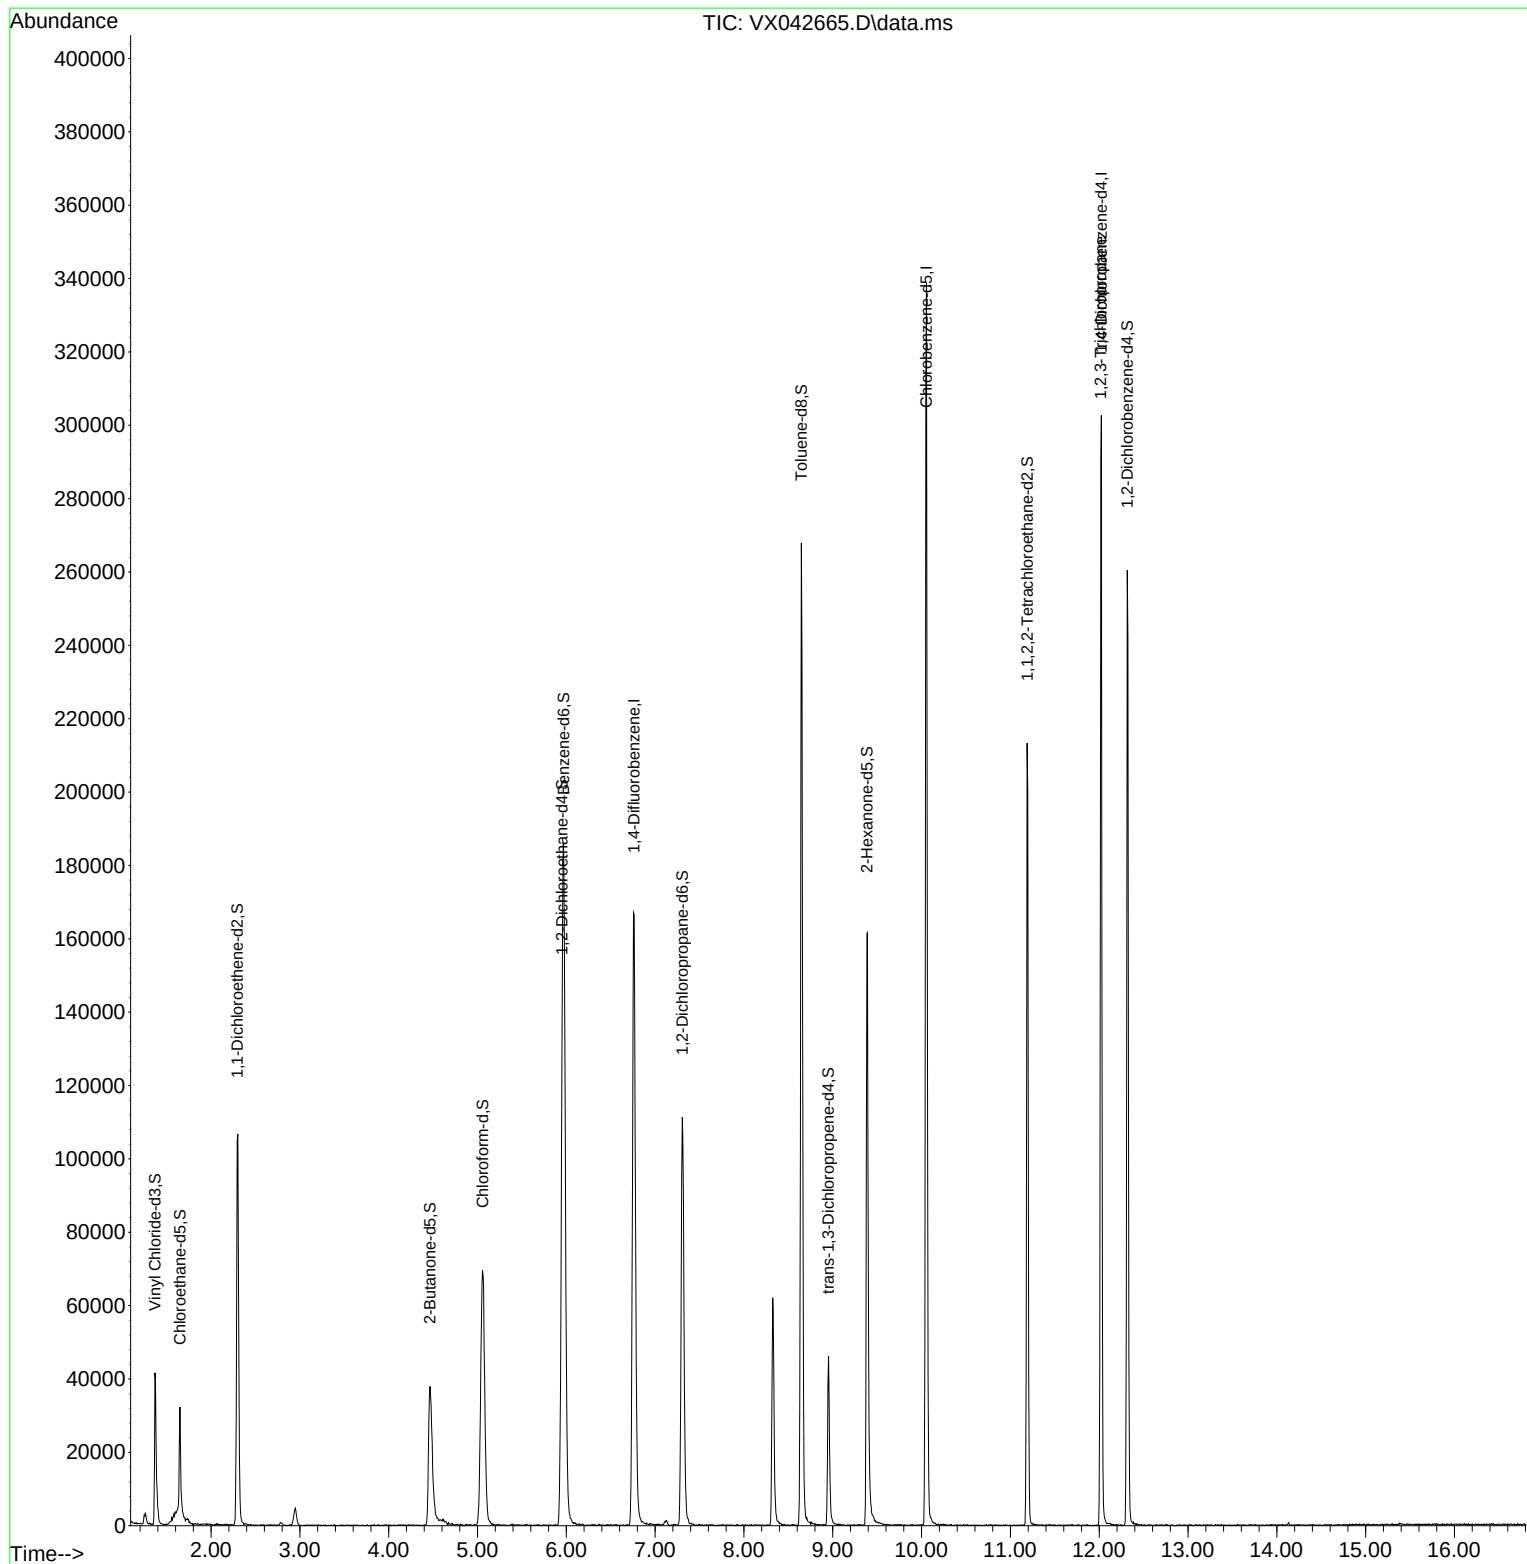

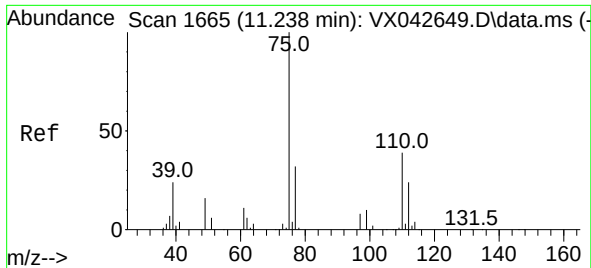

#61
 1,2,3-Trichloropropane
 Concen: 5.326 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX042665.D
 Acq: 28 Jul 2024 02:09

Instrument :
 MSVOA_X
 ClientSampleId :

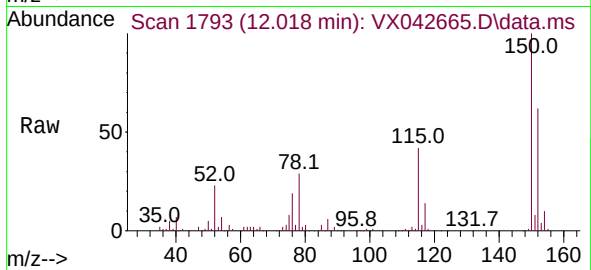

Tgt Ion: 75	Resp:	7716
Ion Ratio	Lower	Upper
75	100	
77	33.1	26.2 39.4
110	3.3	33.0 49.4#

