

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042670.D
 Acq On : 28 Jul 2024 04:04
 Operator : JC/MD
 Sample : P3389-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 04:27:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	163810	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	144274	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	55455	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	33620	33.782	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.560%		
7) Chloroethane-d5	1.648	69	16599	40.476	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.960%		
11) 1,1-Dichloroethene-d2	2.294	65	18887	38.518	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.040%		
21) 2-Butanone-d5	4.465	46	67987	92.173	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.170%		
24) Chloroform-d	5.056	84	93347	42.853	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.700%		
26) 1,2-Dichloroethane-d4	5.952	65	64094	45.608	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.220%		
32) Benzene-d6	5.970	84	184936	46.187	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.380%		
36) 1,2-Dichloropropane-d6	7.306	67	56288	47.498	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.000%		
41) Toluene-d8	8.647	98	158373	44.114	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.220%		
43) trans-1,3-Dichloroprop...	8.952	79	21899	39.488	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.980%		
47) 2-Hexanone-d5	9.384	63	48840	92.179	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.180%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	79613	46.659	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.320%		
66) 1,2-Dichlorobenzene-d4	12.317	152	51053	48.713	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.420%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	7.306	63	6609	5.760	ug/L #	86
61) 1,2,3-Trichloropropane	12.018	75	6906	5.383	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042670.D
Acq On : 28 Jul 2024 04:04
Operator : JC/MD
Sample : P3389-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 29 04:27:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration




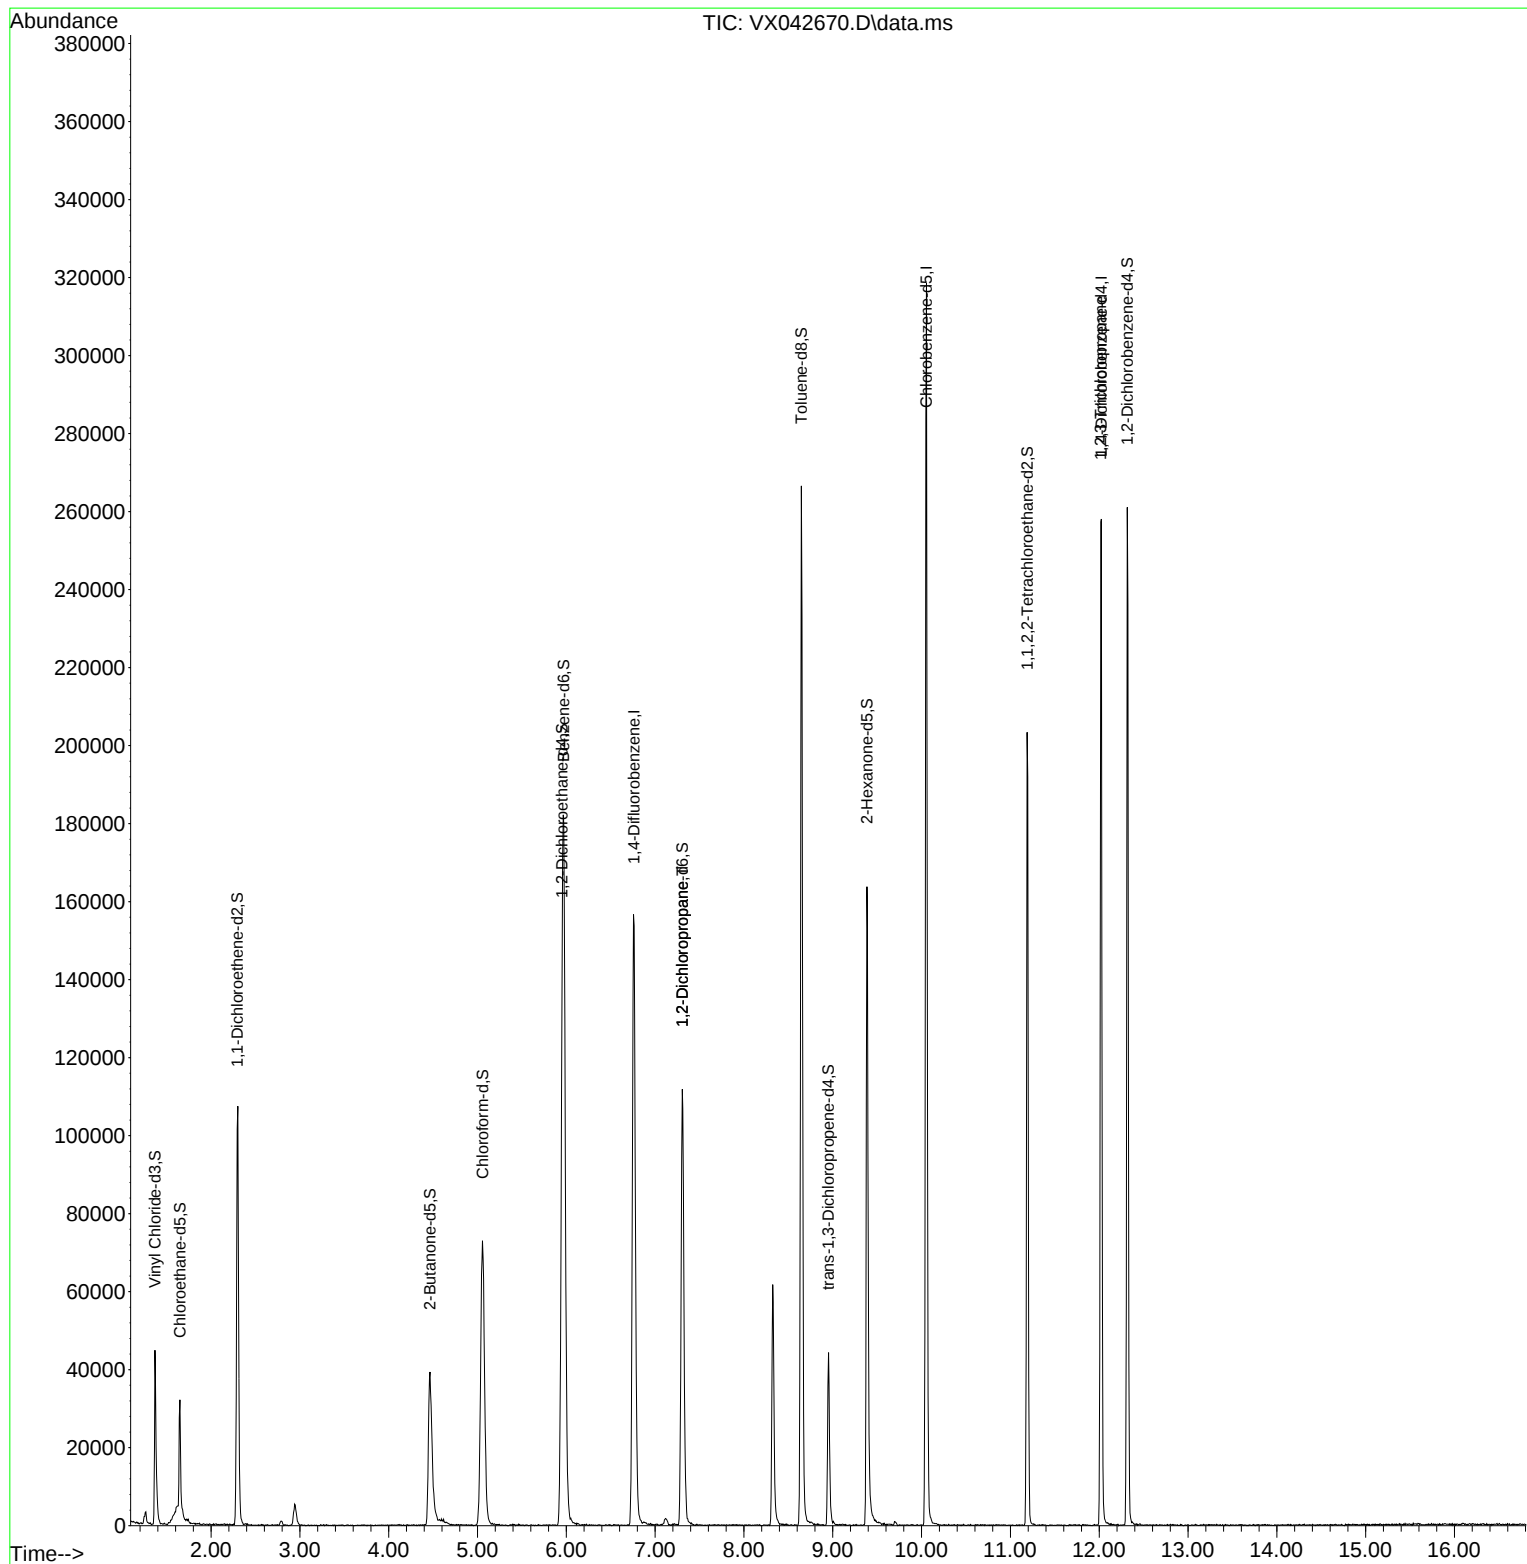


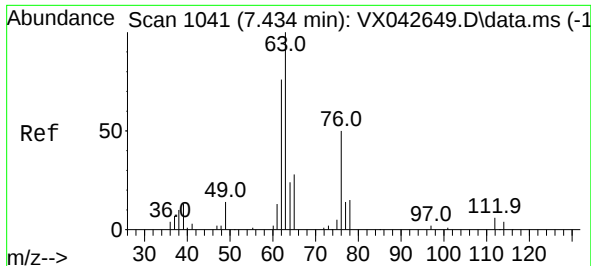

#37
1,2-Dichloropropane
Concen: 5.760 ug/L
RT: 7.306 min Scan# 11
Delta R.T. -0.128 min
Lab File: VX042670.D
Acq: 28 Jul 2024 04:04

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 6609
Ion Ratio Lower Upper
63 100
112 0.0 3.7 5.5#

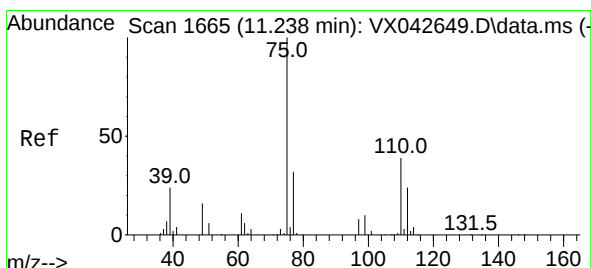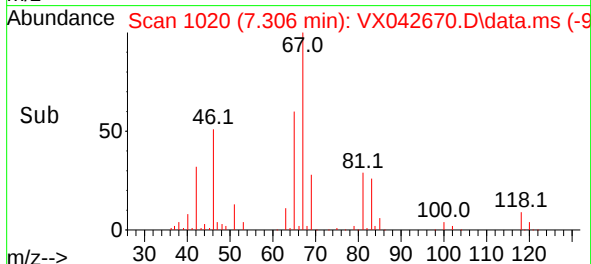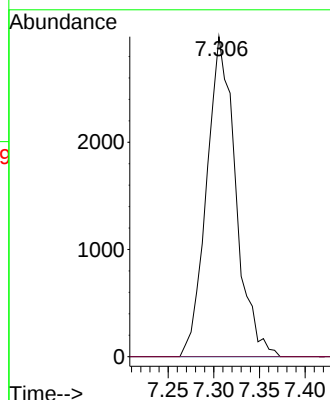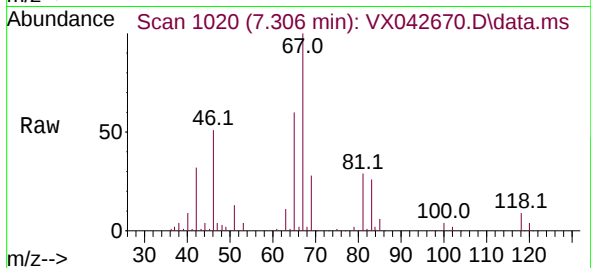

#61
1,2,3-Trichloropropane
Concen: 5.383 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX042670.D
Acq: 28 Jul 2024 04:04

Tgt Ion: 75 Resp: 6906
Ion Ratio Lower Upper
75 100
77 33.0 26.2 39.4
110 3.0 33.0 49.4#

