

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042604.D
 Acq On : 26 Jul 2024 17:42
 Operator : JC/MD
 Sample : P3327-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20D8

Quant Time: Jul 27 01:34:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 01:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	182934	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	163818	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	64155	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	47540	42.775	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.560%		
7) Chloroethane-d5	1.648	69	21312	46.536	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.080%		
11) 1,1-Dichloroethene-d2	2.294	65	25771	47.063	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.120%		
21) 2-Butanone-d5	4.465	46	83125	100.915	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.910%		
24) Chloroform-d	5.056	84	116300	47.808	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.620%		
26) 1,2-Dichloroethane-d4	5.958	65	74713	47.606	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.220%		
32) Benzene-d6	5.970	84	232148	51.061	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.120%		
36) 1,2-Dichloropropane-d6	7.306	67	69887	51.938	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	103.880%		
41) Toluene-d8	8.647	98	203295	49.871	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.740%		
43) trans-1,3-Dichloroprop...	8.952	79	29189	46.354	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.700%		
47) 2-Hexanone-d5	9.384	63	59991	99.717	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.720%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	94446	48.749	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.500%		
66) 1,2-Dichlorobenzene-d4	12.317	152	64907	53.534	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.060%		
Target Compounds					Qvalue	
13) Acetone	2.386	43	2332	3.622	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042604.D
Acq On : 26 Jul 2024 17:42
Operator : JC/MD
Sample : P3327-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20D8

Quant Time: Jul 27 01:34:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 01:23:37 2024
Response via : Initial Calibration

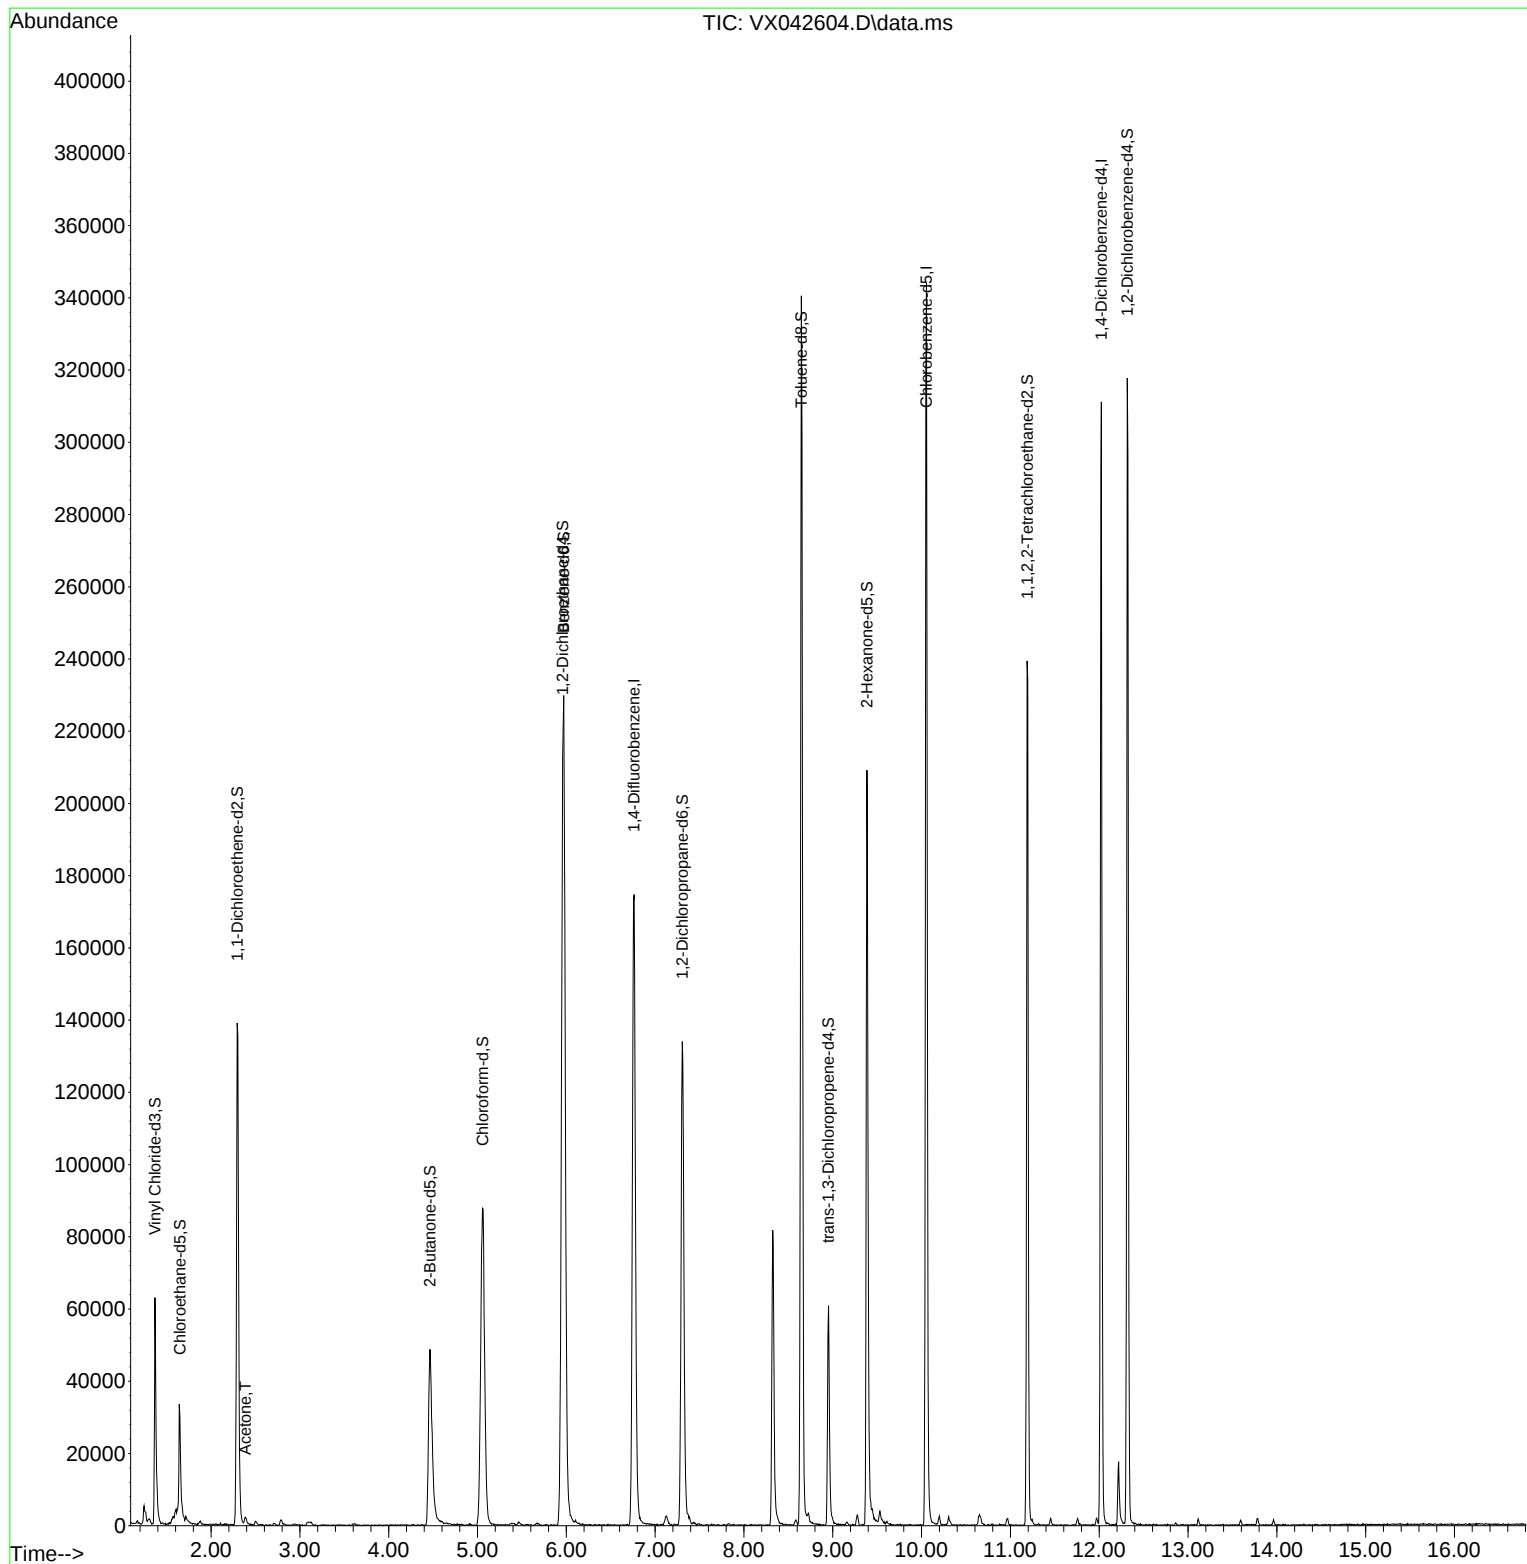

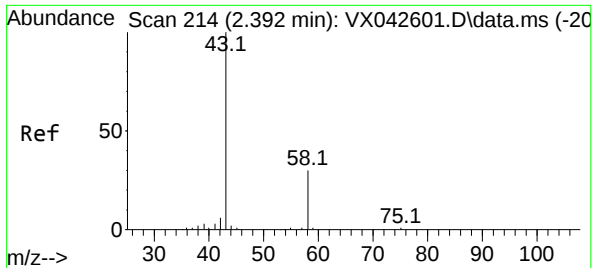

#13
 Acetone
 Concen: 3.622 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VX042604.D
 Acq: 26 Jul 2024 17:42

Instrument :
 MSVOA_X
 ClientSampleId :
 E20D8

Tgt Ion: 43 Resp: 2332
 Ion Ratio Lower Upper
 43 100
 58 35.2 0.0 62.4

