

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042607.D
 Acq On : 26 Jul 2024 18:52
 Operator : JC/MD
 Sample : P3334-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Quant Time: Jul 27 01:34:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 27 01:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	165115	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	143388	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	52496	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	44539	44.400	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.800%
7) Chloroethane-d5	1.648	69	20464	49.506	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.020%
11) 1,1-Dichloroethene-d2	2.300	65	23304	47.150	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.300%
21) 2-Butanone-d5	4.464	46	80419	108.166	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.170%
24) Chloroform-d	5.056	84	107566	48.990	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.980%
26) 1,2-Dichloroethane-d4	5.958	65	73418	51.829	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.660%
32) Benzene-d6	5.970	84	216672	54.447	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.900%
36) 1,2-Dichloropropane-d6	7.311	67	65471	55.589	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.180%
41) Toluene-d8	8.647	98	181928	50.988	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.980%
43) trans-1,3-Dichloroprop...	8.951	79	27106	49.180	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.360%
47) 2-Hexanone-d5	9.384	63	59592	113.167	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.170%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	93261	54.996	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.000%
66) 1,2-Dichlorobenzene-d4	12.317	152	56349	56.797	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.600%
Target Compounds						
13) Acetone	2.392	43	3087	5.312	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042607.D
Acq On : 26 Jul 2024 18:52
Operator : JC/MD
Sample : P3334-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Time: Jul 27 01:34:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 27 01:23:37 2024
Response via : Initial Calibration

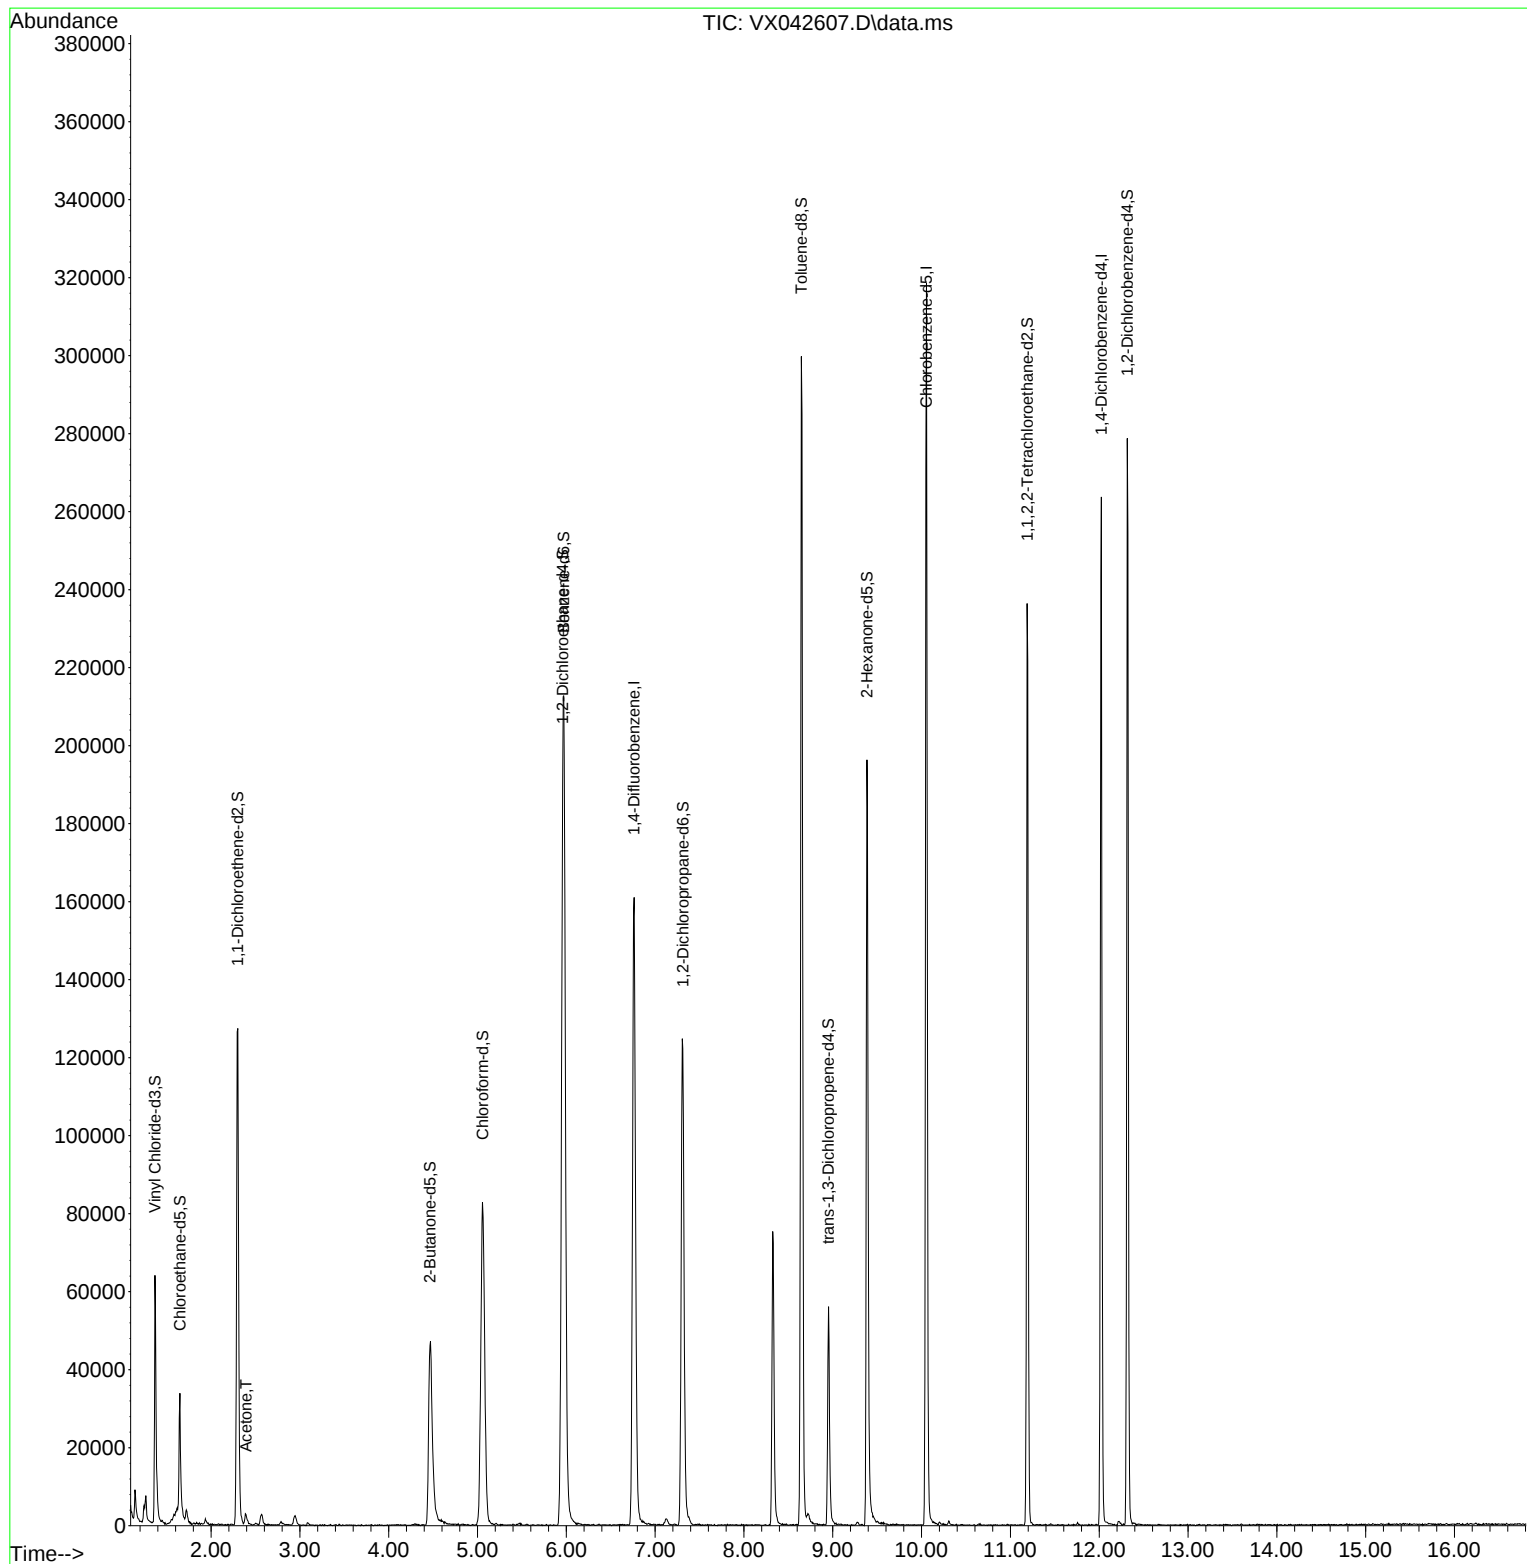

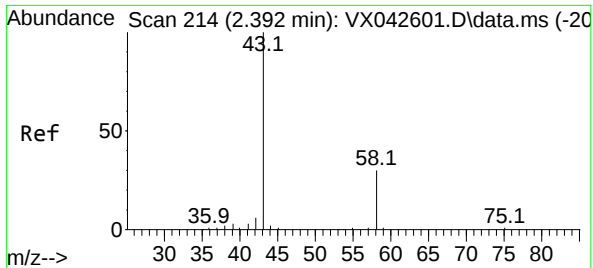

#13
 Acetone
 Concen: 5.312 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX042607.D
 Acq: 26 Jul 2024 18:52

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Tgt Ion: 43	Resp: 3087
Ion Ratio	Lower Upper
43	100
58	31.9 0.0 62.4

