

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042605.D
 Acq On : 26 Jul 2024 18:06
 Operator : JC/MD
 Sample : P3327-31 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	28	rBV	5276	6951	1.05%	0.132%
2	1.368	42	46	62	rVB	59143	78169	11.85%	1.481%
3	1.483	64	65	69	rBV2	445	380	0.06%	0.007%
4	1.605	74	85	87	rVV4	3774	10689	1.62%	0.203%
5	1.648	88	92	101	rVV	33546	50292	7.63%	0.953%
6	1.715	101	103	112	rVB5	2022	3851	0.58%	0.073%
7	2.099	163	166	168	rBV3	393	438	0.07%	0.008%
8	2.130	168	171	173	rBV2	731	622	0.09%	0.012%
9	2.178	177	179	181	rBV	306	214	0.03%	0.004%
10	2.294	192	198	211	rBV	140812	226192	34.30%	4.286%
11	2.660	254	258	260	rBV2	185	291	0.04%	0.006%
12	2.733	268	270	274	rBV	169	224	0.03%	0.004%
13	2.782	274	278	286	rBV5	2101	4216	0.64%	0.080%
14	2.947	297	305	314	rVB	6259	14136	2.14%	0.268%
15	3.087	324	328	336	rVB3	1366	2469	0.37%	0.047%
16	3.605	405	413	423	rVB2	9276	22907	3.47%	0.434%
17	3.727	430	433	436	rBV	204	311	0.05%	0.006%
18	3.757	436	438	441	rVB	201	232	0.04%	0.004%
19	3.806	441	446	448	rBV	380	509	0.08%	0.010%
20	3.879	456	458	462	rVB2	189	282	0.04%	0.005%
21	4.111	492	496	497	rBV	185	229	0.03%	0.004%
22	4.227	513	515	518	rBV2	220	301	0.05%	0.006%
23	4.367	535	538	543	rVB2	211	383	0.06%	0.007%
24	4.410	543	545	546	rBV	305	252	0.04%	0.005%
25	4.483	546	557	571	rBV3	147366	451497	68.47%	8.555%
26	4.824	610	613	616	rVB2	340	364	0.06%	0.007%
27	4.946	630	633	639	rVB2	283	432	0.07%	0.008%
28	5.062	639	652	672	rBV2	86585	267407	40.55%	5.067%
29	5.318	692	694	696	rBV2	224	227	0.03%	0.004%
30	5.397	704	707	708	rBV3	304	280	0.04%	0.005%
31	5.550	728	732	733	rBV	581	701	0.11%	0.013%
32	5.720	759	760	765	rVB2	188	233	0.04%	0.004%
33	5.757	765	766	768	rBV	249	233	0.04%	0.004%
34	5.848	780	781	783	rBV	215	215	0.03%	0.004%
35	5.964	789	800	816	rBV2	225304	659411	100.00%	12.495%
36	6.300	848	855	859	rBV2	297	750	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042605.D
Acq On : 26 Jul 2024 18:06
Operator : JC/MD
Sample : P3327-31 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Title : VOC Analysis

37	6.367	864	866	870	rBV2	361	439	0.07%	0.008%
38	6.763	921	931	948	rBV	177392	429259	65.10%	8.134%
39	7.129	983	991	1004	rBV3	30761	74163	11.25%	1.405%
40	7.306	1012	1020	1038	rBV	131099	294986	44.73%	5.590%
41	7.482	1044	1049	1050	rBV2	280	395	0.06%	0.007%
42	7.586	1065	1066	1069	rBV	218	262	0.04%	0.005%
43	7.696	1080	1084	1086	rVB2	237	247	0.04%	0.005%
44	7.964	1124	1128	1131	rBV2	228	353	0.05%	0.007%
45	8.019	1133	1137	1140	rBV2	209	389	0.06%	0.007%
46	8.324	1181	1187	1198	rVV	81132	135069	20.48%	2.559%
47	8.580	1227	1229	1231	rBV2	538	445	0.07%	0.008%
48	8.647	1234	1240	1256	rBV	330782	524378	79.52%	9.936%
49	8.805	1264	1266	1271	rBV4	430	452	0.07%	0.009%
50	8.952	1285	1290	1301	rBV	57390	89419	13.56%	1.694%
51	9.080	1309	1311	1314	rBV2	236	319	0.05%	0.006%
52	9.275	1337	1343	1348	rVB4	1211	1864	0.28%	0.035%
53	9.317	1348	1350	1354	rBV	226	267	0.04%	0.005%
54	9.384	1356	1361	1380	rBV	194331	297231	45.08%	5.632%
55	9.683	1406	1410	1411	rBV2	232	343	0.05%	0.006%
56	9.799	1427	1429	1432	rBV2	279	402	0.06%	0.008%
57	9.927	1446	1450	1452	rBV2	251	287	0.04%	0.005%
58	10.055	1465	1471	1479	rBV	351658	486288	73.75%	9.215%
59	10.250	1500	1503	1504	rBV	400	307	0.05%	0.006%
60	10.268	1504	1506	1508	rVV	258	214	0.03%	0.004%
61	10.287	1508	1509	1511	rVV	282	234	0.04%	0.004%
62	10.311	1511	1513	1517	rVB3	417	544	0.08%	0.010%
63	10.415	1529	1530	1533	rVB2	339	243	0.04%	0.005%
64	10.512	1544	1546	1549	rVB2	285	288	0.04%	0.005%
65	10.646	1564	1568	1571	rBV2	285	524	0.08%	0.010%
66	10.939	1611	1616	1618	rBV2	173	257	0.04%	0.005%
67	11.189	1652	1657	1666	rBV	236874	315874	47.90%	5.985%
68	11.293	1672	1674	1675	rBV	301	223	0.03%	0.004%
69	11.567	1715	1719	1722	rVB	166	247	0.04%	0.005%
70	11.628	1725	1729	1731	rBV	258	294	0.04%	0.006%
71	11.975	1784	1786	1788	rBV	315	352	0.05%	0.007%
72	12.024	1788	1794	1804	rVV	305100	398064	60.37%	7.543%
73	12.140	1812	1813	1816	rVB	422	213	0.03%	0.004%
74	12.164	1816	1817	1820	rVB2	314	282	0.04%	0.005%
75	12.201	1820	1823	1825	rBV	385	434	0.07%	0.008%
76	12.219	1825	1826	1832	rVB2	691	775	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042605.D
 Acq On : 26 Jul 2024 18:06
 Operator : JC/MD
 Sample : P3327-31 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1857	rBV	315794	405715	61.53%	7.688%
78	12.603	1886	1889	1890	rBV	277	321	0.05%	0.006%
79	12.683	1899	1902	1903	rBV2	208	216	0.03%	0.004%
80	13.122	1970	1974	1978	rVB3	530	809	0.12%	0.015%
81	13.158	1978	1980	1982	rBV2	298	372	0.06%	0.007%
82	13.451	2027	2028	2033	rVB2	384	444	0.07%	0.008%
83	13.500	2033	2036	2039	rBV2	208	375	0.06%	0.007%
84	13.756	2077	2078	2080	rBV2	308	237	0.04%	0.004%
85	13.786	2080	2083	2086	rVV3	457	633	0.10%	0.012%
86	14.127	2138	2139	2144	rBV	269	303	0.05%	0.006%
87	14.633	2220	2222	2225	rBV	243	245	0.04%	0.005%
88	14.670	2226	2228	2230	rBV	194	212	0.03%	0.004%
89	14.908	2263	2267	2269	rBV2	404	337	0.05%	0.006%
90	15.066	2290	2293	2294	rBV3	334	377	0.06%	0.007%
91	15.085	2294	2296	2298	rVV	270	222	0.03%	0.004%
92	15.109	2298	2300	2304	rVV3	266	406	0.06%	0.008%
93	15.170	2308	2310	2312	rBV	415	288	0.04%	0.005%
94	15.682	2391	2394	2395	rBV	329	290	0.04%	0.005%
95	15.749	2402	2405	2407	rBV2	492	585	0.09%	0.011%
96	15.792	2410	2412	2415	rBV2	242	268	0.04%	0.005%
97	15.950	2436	2438	2441	rBV2	240	254	0.04%	0.005%
98	16.359	2503	2505	2509	rVB2	484	570	0.09%	0.011%
99	16.401	2509	2512	2513	rBV	362	343	0.05%	0.006%
100	16.590	2540	2543	2544	rBV2	689	646	0.10%	0.012%




Sum of corrected areas: 5277384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042605.D
Acq On : 26 Jul 2024 18:06
Operator : JC/MD
Sample : P3327-31 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

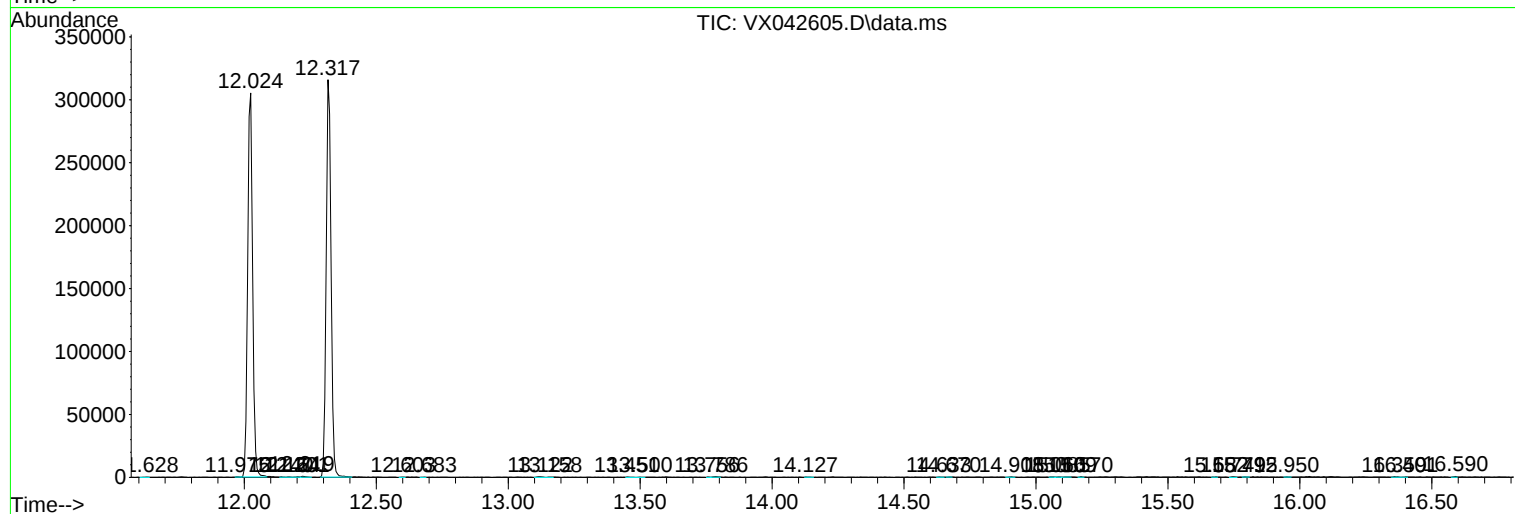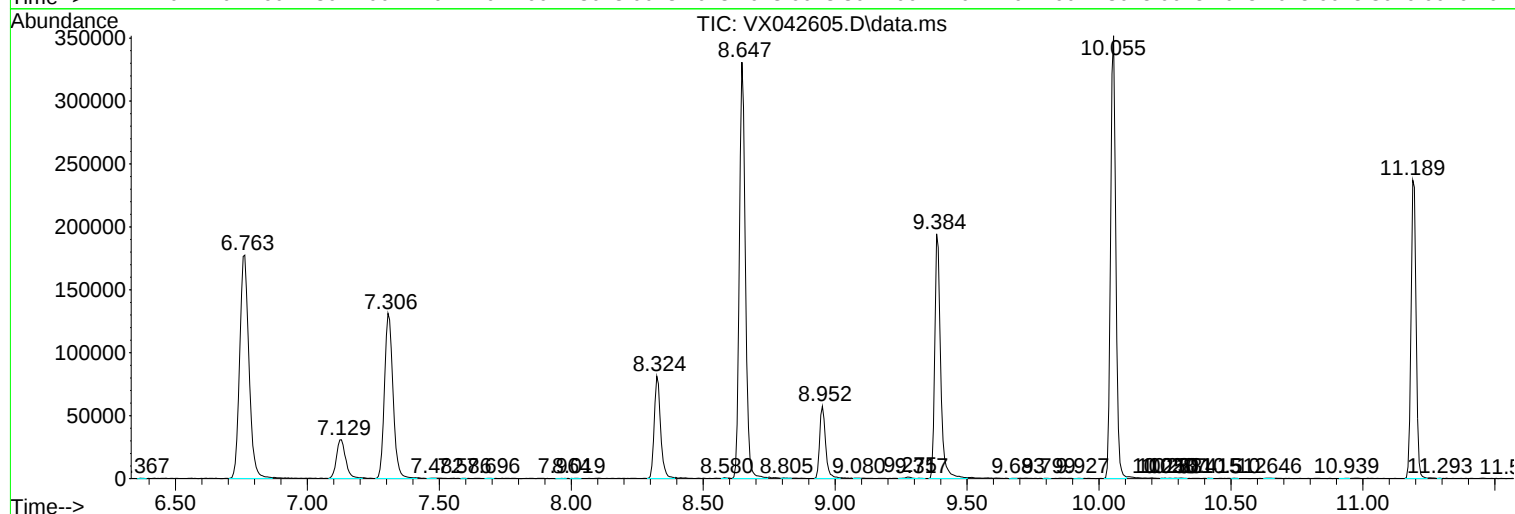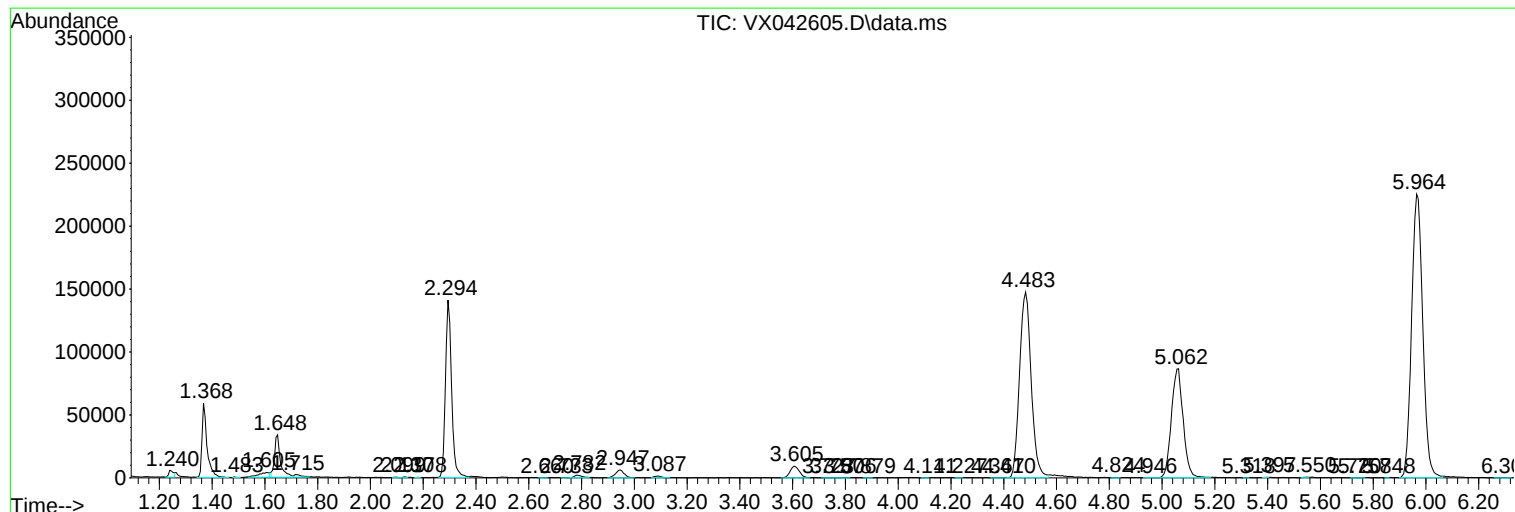

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042605.D
Acq On : 26 Jul 2024 18:06
Operator : JC/MD
Sample : P3327-31 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042605.D
Acq On : 26 Jul 2024 18:06
Operator : JC/MD
Sample : P3327-31 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc