

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042607.D
 Acq On : 26 Jul 2024 18:52
 Operator : JC/MD
 Sample : P3334-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rVB2	8121	11080	1.74%	0.246%
2	1.245	23	26	27	rBV	3922	4083	0.64%	0.091%
3	1.367	43	46	57	rBV	63157	77707	12.23%	1.726%
4	1.648	88	92	101	rVB	32269	41417	6.52%	0.920%
5	1.721	101	104	109	rVB3	3170	4660	0.73%	0.103%
6	1.934	136	139	146	rVB4	1587	2555	0.40%	0.057%
7	1.995	146	149	151	rBV	313	287	0.05%	0.006%
8	2.196	179	182	184	rBV	245	266	0.04%	0.006%
9	2.300	192	199	209	rBV	127238	206292	32.48%	4.582%
10	2.385	210	213	220	rVB	2566	4227	0.67%	0.094%
11	2.568	237	243	248	rBV3	2790	5544	0.87%	0.123%
12	2.788	275	279	281	rBV3	902	1159	0.18%	0.026%
13	2.946	298	305	313	rVB	2446	5433	0.86%	0.121%
14	3.087	325	328	333	rBV3	785	1293	0.20%	0.029%
15	3.227	348	351	353	rVB2	286	249	0.04%	0.006%
16	3.251	353	355	358	rBB	284	278	0.04%	0.006%
17	3.276	358	359	362	rBV	302	270	0.04%	0.006%
18	3.343	365	370	374	rBB	345	491	0.08%	0.011%
19	3.404	374	380	384	rBV2	276	574	0.09%	0.013%
20	3.440	384	386	390	rVB2	404	457	0.07%	0.010%
21	3.483	390	393	395	rBV	258	286	0.05%	0.006%
22	3.660	418	422	425	rBB	186	270	0.04%	0.006%
23	3.690	426	427	431	rBB	294	246	0.04%	0.005%
24	3.806	442	446	449	rVB2	279	386	0.06%	0.009%
25	3.849	450	453	456	rBV	229	312	0.05%	0.007%
26	4.275	518	523	524	rBV	277	408	0.06%	0.009%
27	4.294	524	526	532	rVB3	383	678	0.11%	0.015%
28	4.373	537	539	540	rBV	271	231	0.04%	0.005%
29	4.470	546	555	574	rBV	47099	144353	22.73%	3.206%
30	4.781	604	606	609	rVB2	455	389	0.06%	0.009%
31	4.818	609	612	613	rBV2	310	333	0.05%	0.007%
32	4.891	623	624	629	rVB	268	247	0.04%	0.005%
33	4.946	629	633	636	rBV2	274	409	0.06%	0.009%
34	5.056	640	651	668	rBV	82835	252553	39.76%	5.609%
35	5.397	705	707	711	rBV2	292	356	0.06%	0.008%
36	5.470	712	719	721	rVV3	495	825	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042607.D
 Acq On : 26 Jul 2024 18:52
 Operator : JC/MD
 Sample : P3334-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.489	721	722	725	rVB2	453	241	0.04%	0.005%
38	5.623	742	744	749	rVB	240	282	0.04%	0.006%
39	5.970	789	801	825	rBV3	212697	635179	100.00%	14.107%
40	6.129	825	827	829	rBV2	433	401	0.06%	0.009%
41	6.409	869	873	875	rBV2	168	301	0.05%	0.007%
42	6.763	922	931	946	rBV	160875	383383	60.36%	8.515%
43	7.122	985	990	999	rVV5	1646	4248	0.67%	0.094%
44	7.220	1002	1006	1011	rVB2	361	669	0.11%	0.015%
45	7.305	1012	1020	1041	rVV	124740	282053	44.41%	6.264%
46	7.494	1050	1051	1054	rVB2	422	292	0.05%	0.006%
47	7.970	1128	1129	1132	rBV	308	280	0.04%	0.006%
48	8.128	1152	1155	1158	rBV2	204	297	0.05%	0.007%
49	8.323	1182	1187	1199	rVV	75362	126574	19.93%	2.811%
50	8.433	1203	1205	1207	rVV2	429	376	0.06%	0.008%
51	8.451	1207	1208	1210	rVV	304	269	0.04%	0.006%
52	8.476	1211	1212	1216	rVB2	362	265	0.04%	0.006%
53	8.647	1234	1240	1249	rBV	299694	475629	74.88%	10.563%
54	8.896	1279	1281	1285	rBV	305	403	0.06%	0.009%
55	8.951	1285	1290	1302	rBV	55952	83544	13.15%	1.855%
56	9.274	1337	1343	1348	rBV5	799	1359	0.21%	0.030%
57	9.384	1356	1361	1378	rBV	196379	296855	46.74%	6.593%
58	9.671	1407	1408	1412	rBV2	264	314	0.05%	0.007%
59	9.921	1447	1449	1452	rVB	249	258	0.04%	0.006%
60	10.055	1465	1471	1483	rBV	318229	427875	67.36%	9.503%
61	10.201	1492	1495	1499	rBV2	738	1024	0.16%	0.023%
62	10.305	1509	1512	1519	rVB3	1067	1492	0.23%	0.033%
63	10.591	1557	1559	1562	rVB2	319	334	0.05%	0.007%
64	10.646	1562	1568	1569	rBV2	451	684	0.11%	0.015%
65	10.756	1584	1586	1589	rBV	185	237	0.04%	0.005%
66	10.963	1617	1620	1622	rBV	263	284	0.04%	0.006%
67	11.189	1652	1657	1664	rBV	236304	305278	48.06%	6.780%
68	11.298	1671	1675	1680	rBV2	187	357	0.06%	0.008%
69	11.451	1695	1700	1707	rBV4	429	838	0.13%	0.019%
70	11.536	1712	1714	1717	rBV	232	229	0.04%	0.005%
71	11.652	1731	1733	1736	rBV	318	263	0.04%	0.006%
72	11.713	1742	1743	1746	rBV2	304	280	0.04%	0.006%
73	11.756	1746	1750	1752	rVV2	668	635	0.10%	0.014%
74	11.884	1769	1771	1773	rBV	356	257	0.04%	0.006%
75	11.914	1773	1776	1777	rBV	268	252	0.04%	0.006%
76	12.024	1789	1794	1807	rBV	263318	330991	52.11%	7.351%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042607.D
 Acq On : 26 Jul 2024 18:52
 Operator : JC/MD
 Sample : P3334-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.219	1823	1826	1833	rBV4	1068	2142	0.34%	0.048%
78	12.274	1833	1835	1837	rBV4	408	388	0.06%	0.009%
79	12.317	1837	1842	1851	rVV	278511	357900	56.35%	7.949%
80	12.439	1859	1862	1863	rBV	364	414	0.07%	0.009%
81	12.597	1886	1888	1892	rBV2	140	247	0.04%	0.005%
82	13.030	1955	1959	1961	rBV	226	304	0.05%	0.007%
83	13.219	1989	1990	1992	rBV	248	235	0.04%	0.005%
84	13.359	2012	2013	2017	rBV2	224	253	0.04%	0.006%
85	13.402	2017	2020	2023	rBV	280	348	0.05%	0.008%
86	13.499	2035	2036	2039	rBV	232	310	0.05%	0.007%
87	13.603	2049	2053	2057	rVB3	322	440	0.07%	0.010%
88	13.786	2080	2083	2084	rBV2	247	276	0.04%	0.006%
89	14.036	2120	2124	2125	rBV2	249	304	0.05%	0.007%
90	14.133	2137	2140	2142	rBV	259	324	0.05%	0.007%
91	14.530	2202	2205	2206	rBV	255	266	0.04%	0.006%
92	14.706	2231	2234	2235	rBV2	230	251	0.04%	0.006%
93	14.786	2246	2247	2251	rBV2	313	290	0.05%	0.006%
94	15.426	2348	2352	2354	rBV3	276	267	0.04%	0.006%
95	15.493	2362	2363	2368	rVB2	264	230	0.04%	0.005%
96	15.639	2385	2387	2388	rVB	431	240	0.04%	0.005%
97	15.676	2388	2393	2394	rBV2	358	590	0.09%	0.013%
98	16.090	2460	2461	2465	rVB2	333	272	0.04%	0.006%
99	16.328	2497	2500	2502	rBV2	357	362	0.06%	0.008%
100	16.584	2540	2542	2548	rBV2	422	550	0.09%	0.012%

Sum of corrected areas: 4502589




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042607.D
Acq On : 26 Jul 2024 18:52
Operator : JC/MD
Sample : P3334-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

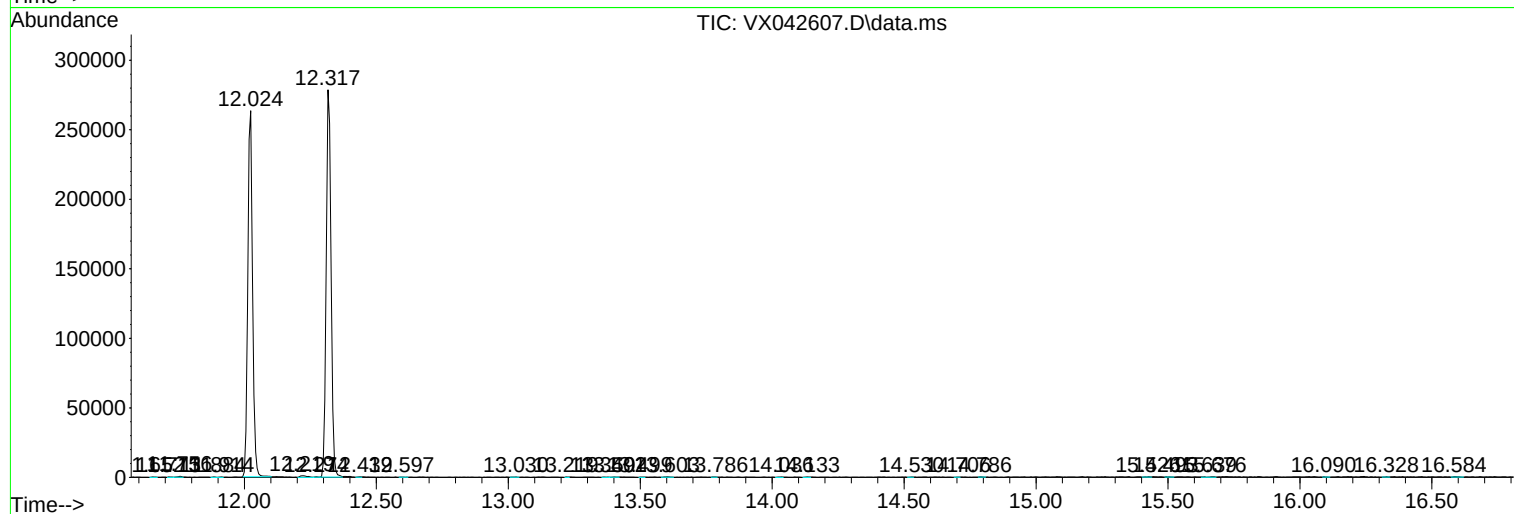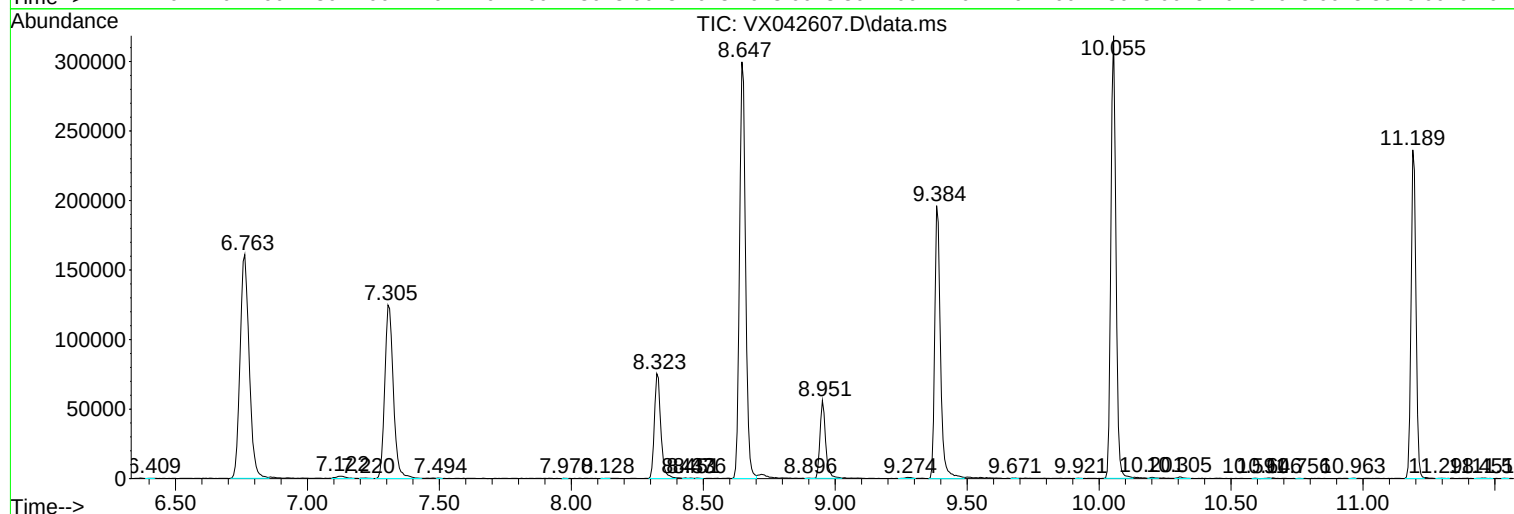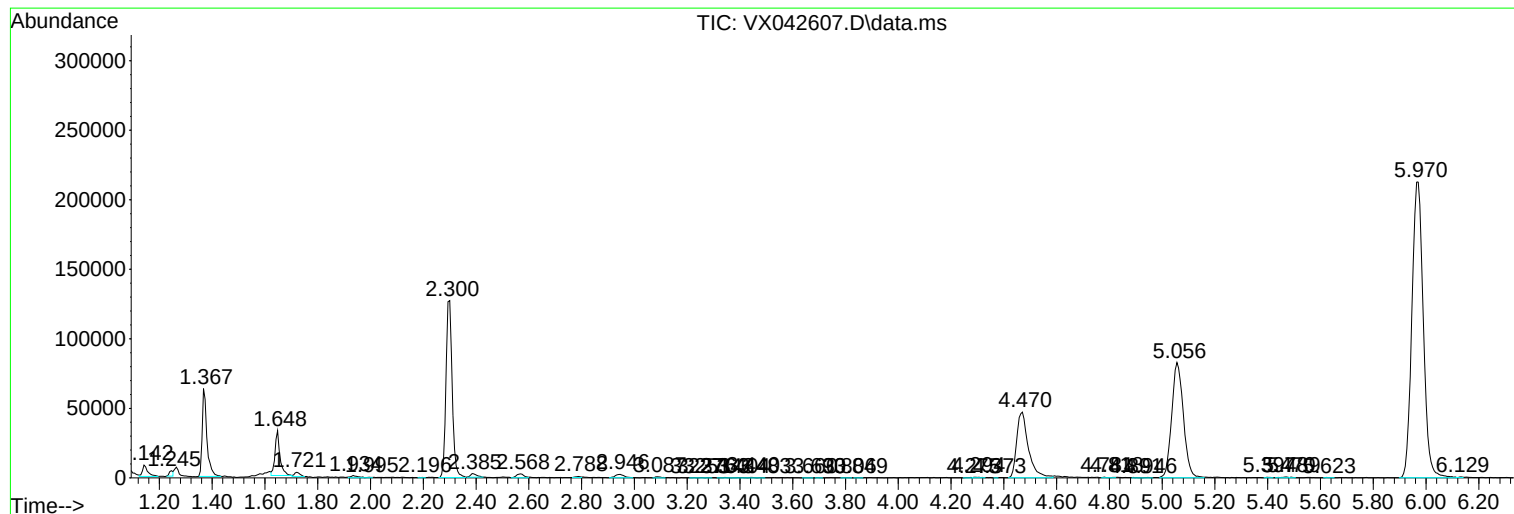

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042607.D
Acq On : 26 Jul 2024 18:52
Operator : JC/MD
Sample : P3334-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042607.D
Acq On : 26 Jul 2024 18:52
Operator : JC/MD
Sample : P3334-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc