

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042616.D
 Acq On : 26 Jul 2024 22:21
 Operator : JC/MD
 Sample : P3334-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	13	rVB2	2951	2638	0.46%	0.060%
2	1.264	23	29	39	rVB4	5007	10606	1.87%	0.239%
3	1.374	43	47	57	rBV2	71300	96220	16.95%	2.171%
4	1.557	72	77	78	rBV3	1678	2324	0.41%	0.052%
5	1.648	88	92	101	rVB	30083	40339	7.10%	0.910%
6	1.721	101	104	110	rVB4	2458	3807	0.67%	0.086%
7	1.935	137	139	144	rVB3	997	1286	0.23%	0.029%
8	1.983	144	147	148	rVB	298	245	0.04%	0.006%
9	2.014	148	152	154	rBV2	387	374	0.07%	0.008%
10	2.300	192	199	210	rBV	108629	176199	31.03%	3.976%
11	2.386	210	213	221	rVV	3392	6154	1.08%	0.139%
12	2.569	236	243	250	rVB	5374	10216	1.80%	0.231%
13	2.630	250	253	255	rBV2	251	352	0.06%	0.008%
14	2.721	265	268	269	rBV2	291	320	0.06%	0.007%
15	2.782	274	278	280	rBV3	803	1080	0.19%	0.024%
16	2.941	296	304	313	rBV	5524	12702	2.24%	0.287%
17	3.087	323	328	338	rBB2	7592	14220	2.50%	0.321%
18	3.178	338	343	345	rBV	233	328	0.06%	0.007%
19	3.227	349	351	354	rVB	232	263	0.05%	0.006%
20	3.331	364	368	369	rBV2	437	535	0.09%	0.012%
21	3.440	381	386	391	rBB2	395	680	0.12%	0.015%
22	3.825	446	449	451	rBV	189	246	0.04%	0.006%
23	3.959	468	471	474	rBV2	253	327	0.06%	0.007%
24	4.032	482	483	488	rVB	276	273	0.05%	0.006%
25	4.081	488	491	492	rBV	283	249	0.04%	0.006%
26	4.251	516	519	522	rBV2	171	262	0.05%	0.006%
27	4.288	522	525	526	rBV2	368	320	0.06%	0.007%
28	4.483	546	557	573	rBV2	127486	400257	70.50%	9.031%
29	4.696	591	592	595	rBV2	318	339	0.06%	0.008%
30	5.056	638	651	668	rBV	72489	231825	40.83%	5.231%
31	5.349	696	699	703	rVB2	280	257	0.05%	0.006%
32	5.391	703	706	708	rBV2	202	263	0.05%	0.006%
33	5.452	713	716	719	rVV2	301	401	0.07%	0.009%
34	5.525	727	728	731	rBV2	286	294	0.05%	0.007%
35	5.623	741	744	746	rBV2	289	261	0.05%	0.006%
36	5.660	748	750	756	rVB2	269	302	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042616.D
 Acq On : 26 Jul 2024 22:21
 Operator : JC/MD
 Sample : P3334-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.964	786	800	816	rBV3	191789	567761	100.00%	12.811%
38	6.556	891	897	898	rBV2	296	427	0.08%	0.010%
39	6.690	916	919	921	rBV2	229	243	0.04%	0.005%
40	6.763	921	931	945	rBV	147030	358293	63.11%	8.085%
41	7.129	985	991	1002	rBV4	11339	25703	4.53%	0.580%
42	7.306	1012	1020	1041	rBV	114873	256590	45.19%	5.790%
43	7.476	1046	1048	1050	rBV	326	400	0.07%	0.009%
44	8.232	1170	1172	1175	rVB2	246	305	0.05%	0.007%
45	8.324	1182	1187	1199	rVV	68321	113977	20.07%	2.572%
46	8.434	1203	1205	1209	rVV	293	351	0.06%	0.008%
47	8.604	1228	1233	1234	rBV	281	240	0.04%	0.005%
48	8.647	1234	1240	1249	rBV	265708	422849	74.48%	9.541%
49	8.866	1273	1276	1278	rVB3	323	299	0.05%	0.007%
50	8.897	1278	1281	1284	rBV3	270	352	0.06%	0.008%
51	8.952	1285	1290	1305	rVB	47214	71708	12.63%	1.618%
52	9.202	1328	1331	1332	rBV	198	236	0.04%	0.005%
53	9.275	1341	1343	1347	rVB3	587	448	0.08%	0.010%
54	9.385	1356	1361	1374	rBV	177904	262502	46.23%	5.923%
55	9.817	1429	1432	1433	rBV	341	331	0.06%	0.007%
56	9.897	1442	1445	1447	rBV	242	264	0.05%	0.006%
57	10.055	1465	1471	1482	rBV	291335	401951	70.80%	9.070%
58	10.201	1492	1495	1499	rBV4	865	1281	0.23%	0.029%
59	10.305	1509	1512	1518	rVV	1376	1557	0.27%	0.035%
60	10.494	1541	1543	1548	rBV2	226	376	0.07%	0.008%
61	10.543	1548	1551	1554	rVV2	226	349	0.06%	0.008%
62	10.653	1565	1569	1572	rVB2	444	612	0.11%	0.014%
63	10.707	1574	1578	1579	rBV	288	395	0.07%	0.009%
64	10.921	1610	1613	1616	rBV	212	365	0.06%	0.008%
65	10.957	1616	1619	1623	rVB2	268	430	0.08%	0.010%
66	11.031	1628	1631	1634	rVB	226	282	0.05%	0.006%
67	11.189	1652	1657	1667	rBV	210392	283002	49.85%	6.386%
68	11.512	1708	1710	1713	rBV2	243	293	0.05%	0.007%
69	11.610	1721	1726	1728	rBV	160	307	0.05%	0.007%
70	11.628	1728	1729	1734	rBV2	168	277	0.05%	0.006%
71	11.756	1747	1750	1755	rVB	785	979	0.17%	0.022%
72	11.793	1755	1756	1760	rBV2	307	364	0.06%	0.008%
73	11.902	1770	1774	1775	rBV2	265	371	0.07%	0.008%
74	12.024	1789	1794	1801	rBV	233510	303984	53.54%	6.859%
75	12.140	1811	1813	1816	rBV2	378	260	0.05%	0.006%
76	12.183	1819	1820	1823	rBV2	221	297	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042616.D
 Acq On : 26 Jul 2024 22:21
 Operator : JC/MD
 Sample : P3334-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.219	1823	1826	1834	rVB3	2597	4064	0.72%	0.092%
78	12.317	1837	1842	1853	rBV	244863	321865	56.69%	7.263%
79	12.439	1859	1862	1864	rVB2	194	246	0.04%	0.006%
80	12.908	1936	1939	1940	rBV	243	269	0.05%	0.006%
81	13.798	2082	2085	2087	rBV2	489	538	0.09%	0.012%
82	13.914	2100	2104	2106	rBV2	211	326	0.06%	0.007%
83	13.987	2113	2116	2118	rBV	301	391	0.07%	0.009%
84	14.170	2143	2146	2151	rVB	194	263	0.05%	0.006%
85	14.250	2158	2159	2163	rBV	389	319	0.06%	0.007%
86	14.615	2217	2219	2223	rBV3	523	633	0.11%	0.014%
87	14.670	2225	2228	2230	rBV2	269	361	0.06%	0.008%
88	14.725	2235	2237	2243	rVB3	255	460	0.08%	0.010%
89	14.792	2246	2248	2250	rBV	322	270	0.05%	0.006%
90	14.926	2267	2270	2275	rBV2	369	743	0.13%	0.017%
91	15.530	2365	2369	2370	rBV2	269	289	0.05%	0.007%
92	15.566	2374	2375	2378	rVV2	266	254	0.04%	0.006%
93	15.627	2383	2385	2388	rVB	401	281	0.05%	0.006%
94	15.664	2388	2391	2393	rBV2	237	247	0.04%	0.006%
95	15.786	2409	2411	2416	rVB2	306	323	0.06%	0.007%
96	15.829	2416	2418	2421	rBV2	231	294	0.05%	0.007%
97	16.103	2461	2463	2467	rBV3	341	373	0.07%	0.008%
98	16.188	2473	2477	2478	rBV3	244	322	0.06%	0.007%
99	16.298	2493	2495	2497	rBV2	464	381	0.07%	0.009%
100	16.676	2554	2557	2561	rVV3	310	525	0.09%	0.012%


Sum of corrected areas: 4431812

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042616.D
Acq On : 26 Jul 2024 22:21
Operator : JC/MD
Sample : P3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

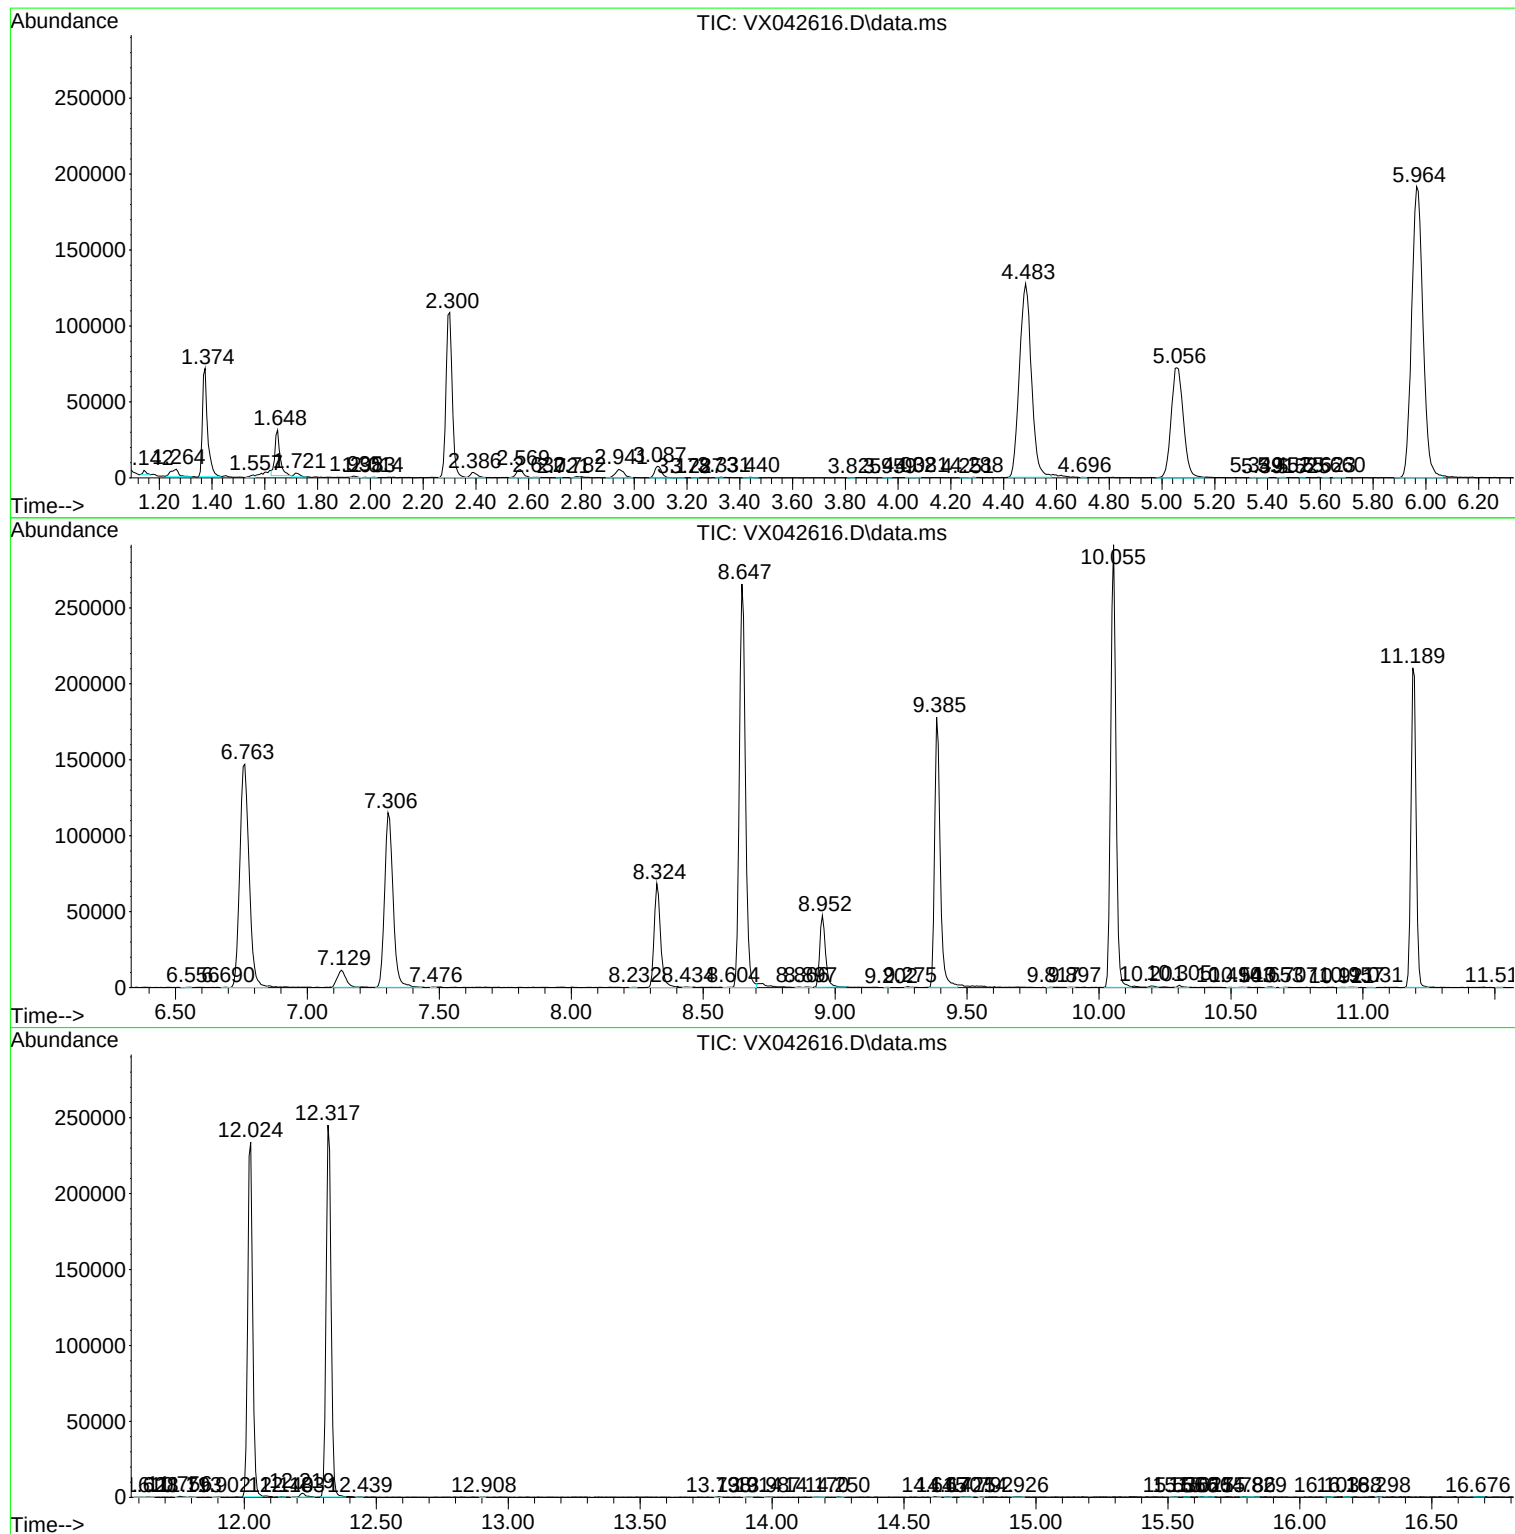

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042616.D
Acq On : 26 Jul 2024 22:21
Operator : JC/MD
Sample : P3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042616.D
Acq On : 26 Jul 2024 22:21
Operator : JC/MD
Sample : P3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc