

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042618.D
 Acq On : 26 Jul 2024 23:08
 Operator : JC/MD
 Sample : P3335-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV	3149	3194	0.55%	0.076%
2	1.368	43	46	59	rVB	52321	64338	11.10%	1.540%
3	1.514	69	70	71	rBV	543	245	0.04%	0.006%
4	1.648	89	92	101	rVB	31962	40598	7.00%	0.972%
5	1.904	133	134	137	rBV2	306	277	0.05%	0.007%
6	2.093	164	165	167	rVB	457	205	0.04%	0.005%
7	2.300	192	199	209	rBV	122583	195759	33.76%	4.685%
8	2.392	209	214	221	rVB	1710	3583	0.62%	0.086%
9	2.471	225	227	229	rBV	323	171	0.03%	0.004%
10	2.624	250	252	254	rBV	217	197	0.03%	0.005%
11	2.794	274	280	283	rVV2	592	989	0.17%	0.024%
12	3.002	312	314	316	rBV	172	157	0.03%	0.004%
13	3.099	324	330	332	rBV2	202	399	0.07%	0.010%
14	3.166	337	341	344	rBB2	226	309	0.05%	0.007%
15	3.197	344	346	350	rBB	170	240	0.04%	0.006%
16	3.343	367	370	372	rBV	116	158	0.03%	0.004%
17	3.398	374	379	380	rBV2	186	274	0.05%	0.007%
18	3.477	391	392	397	rVB2	250	277	0.05%	0.007%
19	3.520	397	399	401	rBB	177	161	0.03%	0.004%
20	3.538	401	402	406	rBB	188	181	0.03%	0.004%
21	3.617	409	415	418	rBB2	204	418	0.07%	0.010%
22	3.788	440	443	444	rBB2	199	184	0.03%	0.004%
23	3.825	447	449	452	rBB	170	176	0.03%	0.004%
24	3.904	459	462	464	rBB	190	167	0.03%	0.004%
25	3.965	467	472	475	rBV2	233	426	0.07%	0.010%
26	4.044	482	485	488	rBB	199	204	0.04%	0.005%
27	4.087	488	492	496	rBV2	328	473	0.08%	0.011%
28	4.367	534	538	539	rBV	165	191	0.03%	0.005%
29	4.459	546	553	569	rBV	38917	117288	20.23%	2.807%
30	4.898	623	625	626	rBV	299	193	0.03%	0.005%
31	4.928	629	630	633	rBV	255	228	0.04%	0.005%
32	4.952	633	634	636	rBV	207	191	0.03%	0.005%
33	5.056	642	651	669	rVB3	75185	231696	39.96%	5.545%
34	5.257	683	684	688	rVB3	307	203	0.04%	0.005%
35	5.288	688	689	691	rVB3	318	165	0.03%	0.004%
36	5.312	691	693	695	rBV3	201	209	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042618.D
 Acq On : 26 Jul 2024 23:08
 Operator : JC/MD
 Sample : P3335-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.477	718	720	723	rBV2	240	323	0.06%	0.008%
38	5.647	745	748	749	rVB	240	244	0.04%	0.006%
39	5.739	760	763	765	rBV	273	383	0.07%	0.009%
40	5.971	789	801	816	rBV2	194936	579826	100.00%	13.876%
41	6.221	840	842	845	rBV2	434	364	0.06%	0.009%
42	6.281	848	852	853	rBV	164	185	0.03%	0.004%
43	6.422	874	875	879	rVB	205	178	0.03%	0.004%
44	6.641	907	911	912	rBV2	239	291	0.05%	0.007%
45	6.696	918	920	922	rBV	213	248	0.04%	0.006%
46	6.763	922	931	946	rVV	148684	361502	62.35%	8.651%
47	7.037	974	976	977	rBV	189	162	0.03%	0.004%
48	7.306	1012	1020	1034	rBV	115403	260085	44.86%	6.224%
49	7.580	1060	1065	1066	rVB	239	285	0.05%	0.007%
50	7.854	1109	1110	1113	rBV2	190	160	0.03%	0.004%
51	8.043	1138	1141	1143	rBV	179	253	0.04%	0.006%
52	8.153	1157	1159	1161	rBV	222	204	0.04%	0.005%
53	8.214	1165	1169	1172	rBV	253	353	0.06%	0.008%
54	8.324	1181	1187	1197	rBV2	65203	112094	19.33%	2.682%
55	8.647	1234	1240	1252	rBV	294081	457648	78.93%	10.952%
56	8.952	1285	1290	1302	rBV	49291	74133	12.79%	1.774%
57	9.275	1340	1343	1348	rBV3	847	1193	0.21%	0.029%
58	9.385	1356	1361	1373	rBV	166307	255937	44.14%	6.125%
59	9.750	1418	1421	1422	rBV	294	243	0.04%	0.006%
60	10.055	1465	1471	1480	rBV	291974	409520	70.63%	9.800%
61	10.293	1508	1510	1513	rBV	315	436	0.08%	0.010%
62	10.720	1578	1580	1581	rBV	179	177	0.03%	0.004%
63	10.878	1604	1606	1607	rBV	232	192	0.03%	0.005%
64	11.043	1631	1633	1637	rBB	226	323	0.06%	0.008%
65	11.085	1637	1640	1642	rBV	316	410	0.07%	0.010%
66	11.189	1652	1657	1664	rBV	214981	283875	48.96%	6.793%
67	11.305	1673	1676	1677	rBV	512	436	0.08%	0.010%
68	11.451	1699	1700	1703	rBV	174	162	0.03%	0.004%
69	11.506	1708	1709	1715	rVB2	269	308	0.05%	0.007%
70	11.646	1730	1732	1733	rBV	250	162	0.03%	0.004%
71	11.768	1751	1752	1755	rBV	264	287	0.05%	0.007%
72	11.817	1758	1760	1764	rVB2	272	263	0.05%	0.006%
73	11.860	1764	1767	1768	rBV2	176	172	0.03%	0.004%
74	12.018	1788	1793	1807	rBV	251717	334172	57.63%	7.997%
75	12.195	1820	1822	1823	rBV	274	192	0.03%	0.005%
76	12.219	1823	1826	1833	rVB2	4258	5929	1.02%	0.142%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042618.D
 Acq On : 26 Jul 2024 23:08
 Operator : JC/MD
 Sample : P3335-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1857	rVV	285716	365117	62.97%	8.738%
78	12.451	1862	1864	1866	rBV	210	189	0.03%	0.005%
79	12.488	1868	1870	1874	rBV2	216	269	0.05%	0.006%
80	12.652	1896	1897	1899	rBV2	272	240	0.04%	0.006%
81	12.762	1912	1915	1917	rBV2	267	316	0.05%	0.008%
82	12.799	1919	1921	1924	rVV	187	187	0.03%	0.004%
83	12.866	1929	1932	1935	rBV2	458	641	0.11%	0.015%
84	13.256	1995	1996	2003	rVB	253	278	0.05%	0.007%
85	13.555	2044	2045	2048	rVV	239	260	0.04%	0.006%
86	13.841	2089	2092	2095	rBV2	185	216	0.04%	0.005%
87	13.896	2100	2101	2105	rBV2	221	288	0.05%	0.007%
88	14.085	2130	2132	2135	rVB	262	248	0.04%	0.006%
89	14.225	2153	2155	2157	rBV2	191	222	0.04%	0.005%
90	14.384	2179	2181	2186	rVB2	256	289	0.05%	0.007%
91	14.457	2192	2193	2196	rBV	145	166	0.03%	0.004%
92	14.567	2209	2211	2213	rVB	295	198	0.03%	0.005%
93	14.585	2213	2214	2216	rBV	289	203	0.04%	0.005%
94	14.652	2223	2225	2227	rVB	276	246	0.04%	0.006%
95	14.676	2227	2229	2230	rBV	316	241	0.04%	0.006%
96	14.762	2242	2243	2245	rBV	277	236	0.04%	0.006%
97	14.951	2272	2274	2276	rBV	421	404	0.07%	0.010%
98	15.341	2337	2338	2340	rBV	428	392	0.07%	0.009%
99	15.560	2373	2374	2375	rBV	403	209	0.04%	0.005%
100	16.463	2520	2522	2523	rBV2	298	245	0.04%	0.006%




Sum of corrected areas: 4178734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042618.D
Acq On : 26 Jul 2024 23:08
Operator : JC/MD
Sample : P3335-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

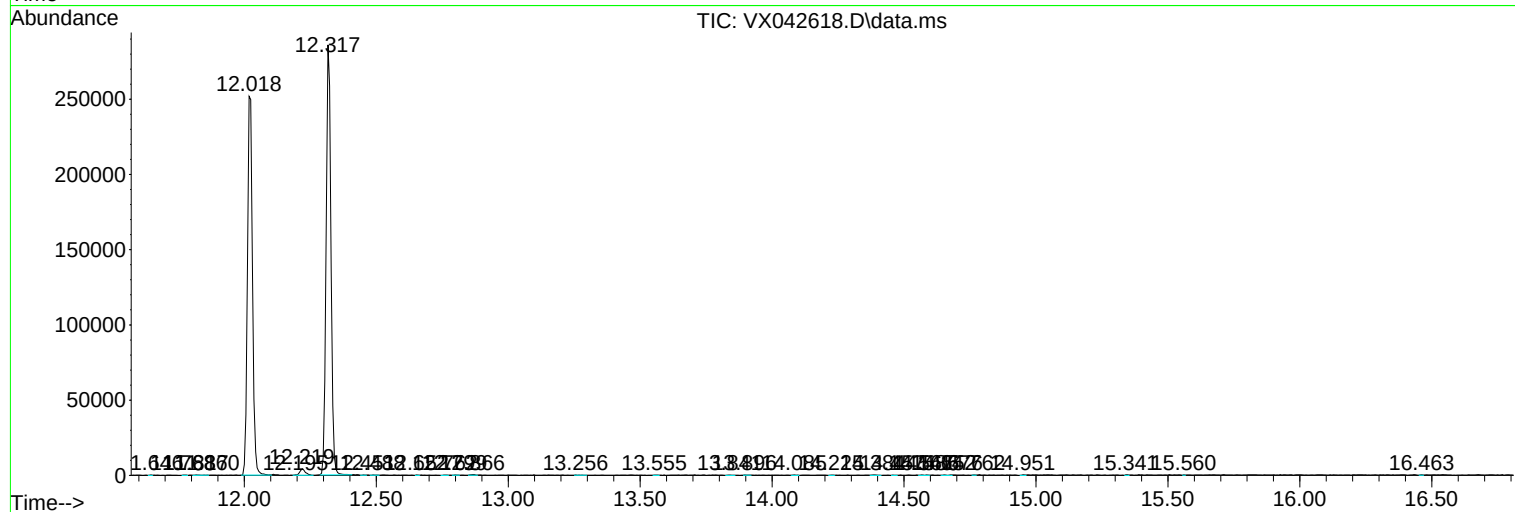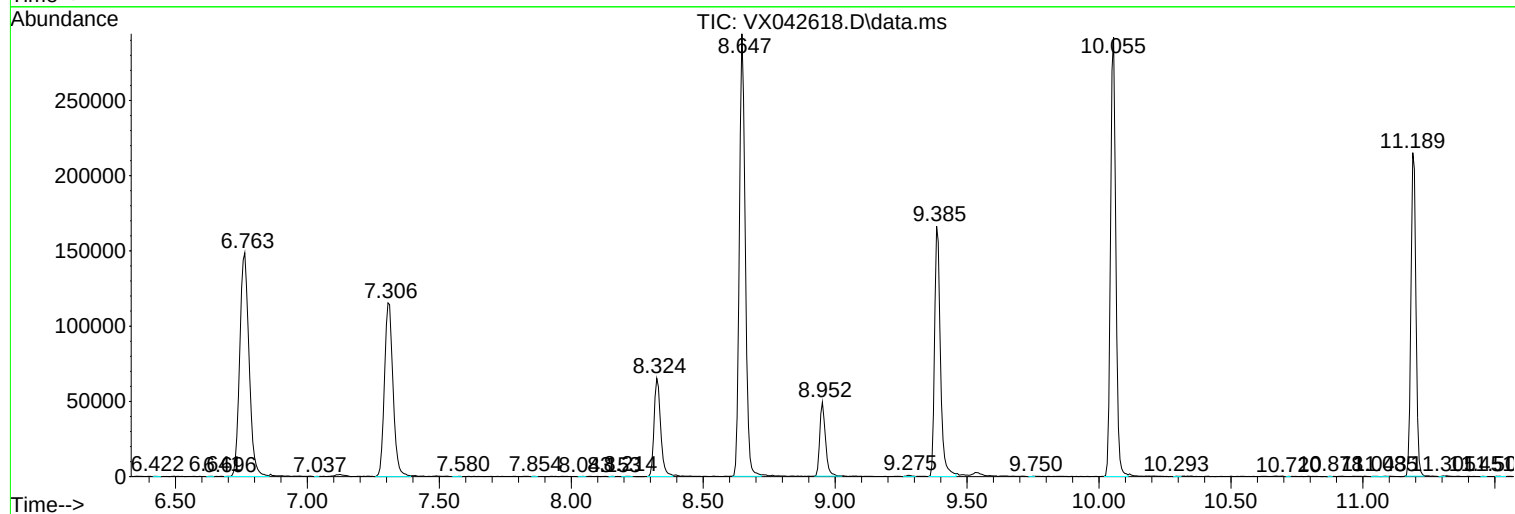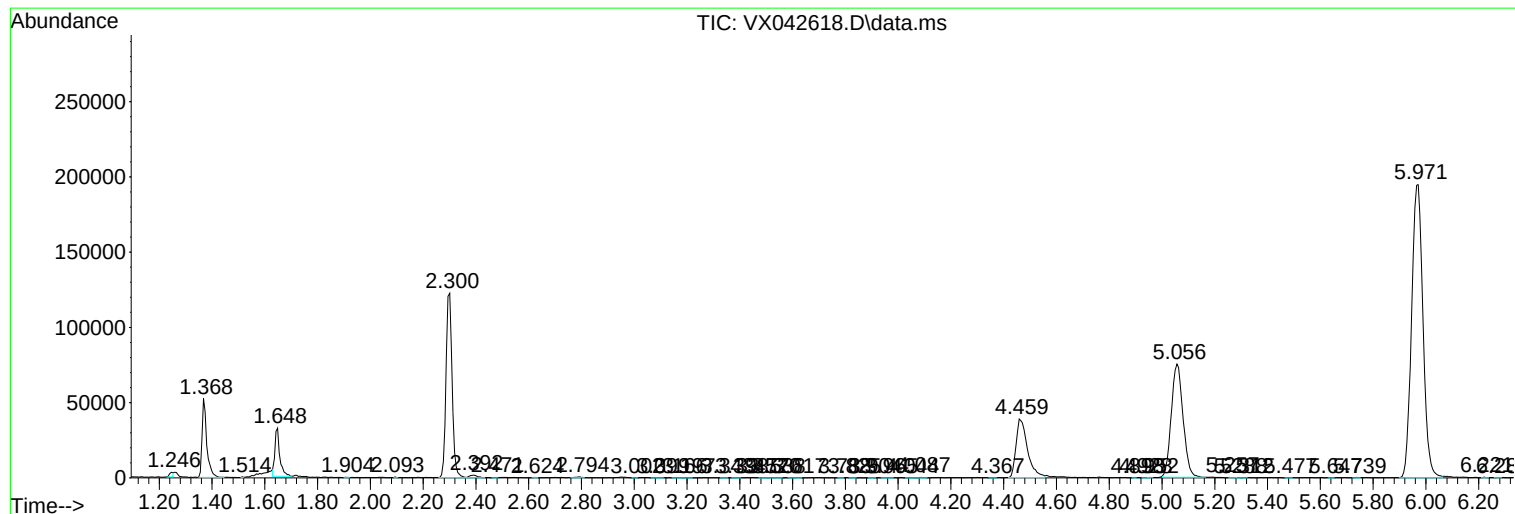

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042618.D
Acq On : 26 Jul 2024 23:08
Operator : JC/MD
Sample : P3335-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042618.D
Acq On : 26 Jul 2024 23:08
Operator : JC/MD
Sample : P3335-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc