

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042623.D
 Acq On : 27 Jul 2024 01:03
 Operator : JC/MD
 Sample : P3335-07 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rBV	45701	60985	10.59%	1.480%
2	1.648	89	92	102	rVB	31636	40421	7.02%	0.981%
3	2.099	164	166	170	rBV2	299	368	0.06%	0.009%
4	2.215	183	185	186	rBV	289	182	0.03%	0.004%
5	2.239	186	189	191	rBV2	187	257	0.04%	0.006%
6	2.300	192	199	209	rVV	121632	190728	33.10%	4.628%
7	2.447	221	223	227	rBV2	219	319	0.06%	0.008%
8	2.508	230	233	237	rVB	274	385	0.07%	0.009%
9	2.569	242	243	246	rVB	367	238	0.04%	0.006%
10	2.678	258	261	263	rBV	165	203	0.04%	0.005%
11	2.697	263	264	267	rVV2	130	121	0.02%	0.003%
12	2.782	274	278	282	rBV	1184	1983	0.34%	0.048%
13	2.892	294	296	297	rVV	178	105	0.02%	0.003%
14	2.947	297	305	317	rVB2	5741	14167	2.46%	0.344%
15	3.129	333	335	337	rBV	212	144	0.02%	0.003%
16	3.337	367	369	371	rBB	165	120	0.02%	0.003%
17	3.367	371	374	375	rBV	131	137	0.02%	0.003%
18	3.501	393	396	397	rBV	163	147	0.03%	0.004%
19	3.520	397	399	402	rVB	206	205	0.04%	0.005%
20	3.648	418	420	423	rBV	167	217	0.04%	0.005%
21	3.739	433	435	438	rBB	149	143	0.02%	0.003%
22	3.867	452	456	457	rBB	335	240	0.04%	0.006%
23	3.898	458	461	465	rBB2	257	247	0.04%	0.006%
24	3.940	466	468	471	rBB	95	111	0.02%	0.003%
25	3.971	471	473	475	rBV	203	215	0.04%	0.005%
26	4.062	486	488	489	rVV	209	154	0.03%	0.004%
27	4.208	511	512	516	rBV2	196	219	0.04%	0.005%
28	4.465	546	554	571	rBV2	38161	115855	20.11%	2.811%
29	4.952	633	634	637	rBV	152	154	0.03%	0.004%
30	4.983	637	639	640	rVV	178	143	0.02%	0.003%
31	5.056	640	651	669	rVV	75786	232008	40.27%	5.629%
32	5.318	691	694	695	rBV2	162	208	0.04%	0.005%
33	5.763	764	767	768	rBV2	178	169	0.03%	0.004%
34	5.964	789	800	818	rBV2	196241	576131	100.00%	13.979%
35	6.354	863	864	866	rBV2	142	121	0.02%	0.003%
36	6.415	873	874	876	rBB2	225	145	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042623.D
 Acq On : 27 Jul 2024 01:03
 Operator : JC/MD
 Sample : P3335-07 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.647	910	912	913	rBV	261	206	0.04%	0.005%
38	6.763	921	931	946	rBV	149993	355002	61.62%	8.614%
39	7.037	975	976	979	rBV	141	145	0.03%	0.004%
40	7.129	985	991	999	rVB5	3410	7277	1.26%	0.177%
41	7.305	1011	1020	1036	rBV	116891	256953	44.60%	6.235%
42	7.488	1049	1050	1053	rVB2	305	241	0.04%	0.006%
43	7.641	1073	1075	1078	rBV	247	273	0.05%	0.007%
44	7.793	1095	1100	1101	rBV	253	333	0.06%	0.008%
45	7.915	1119	1120	1123	rVB	207	141	0.02%	0.003%
46	7.952	1123	1126	1129	rBB	244	302	0.05%	0.007%
47	7.994	1129	1133	1135	rBV2	290	457	0.08%	0.011%
48	8.043	1139	1141	1143	rVB	138	115	0.02%	0.003%
49	8.263	1176	1177	1180	rBB	198	198	0.03%	0.005%
50	8.324	1180	1187	1199	rBV	65421	110522	19.18%	2.682%
51	8.531	1220	1221	1223	rVB	297	150	0.03%	0.004%
52	8.561	1223	1226	1227	rBV2	216	265	0.05%	0.006%
53	8.647	1234	1240	1256	rBV	288246	452446	78.53%	10.978%
54	8.952	1285	1290	1298	rBV	48836	71569	12.42%	1.737%
55	9.159	1323	1324	1325	rBV	196	125	0.02%	0.003%
56	9.384	1356	1361	1377	rBV	169768	249062	43.23%	6.043%
57	9.701	1410	1413	1419	rVB2	717	944	0.16%	0.023%
58	9.805	1428	1430	1432	rBV	272	270	0.05%	0.007%
59	9.884	1441	1443	1446	rBV	235	168	0.03%	0.004%
60	9.994	1456	1461	1462	rBV	175	201	0.03%	0.005%
61	10.055	1465	1471	1489	rVV	289773	408369	70.88%	9.908%
62	10.226	1497	1499	1502	rVB	322	221	0.04%	0.005%
63	10.262	1502	1505	1506	rBV	144	111	0.02%	0.003%
64	10.317	1512	1514	1515	rBV	243	172	0.03%	0.004%
65	10.896	1607	1609	1611	rBV	213	192	0.03%	0.005%
66	11.189	1652	1657	1668	rBV	207622	278762	48.39%	6.764%
67	11.439	1697	1698	1701	rVB	236	172	0.03%	0.004%
68	11.469	1701	1703	1704	rBB	226	122	0.02%	0.003%
69	11.488	1704	1706	1708	rBB	283	181	0.03%	0.004%
70	11.518	1708	1711	1714	rBB	303	304	0.05%	0.007%
71	11.561	1714	1718	1720	rBV	278	337	0.06%	0.008%
72	11.853	1764	1766	1767	rBV	212	206	0.04%	0.005%
73	11.890	1771	1772	1773	rBV	218	105	0.02%	0.003%
74	12.024	1788	1794	1807	rBV	244653	327169	56.79%	7.938%
75	12.231	1826	1828	1830	rBV	296	267	0.05%	0.006%
76	12.317	1837	1842	1850	rBV	274800	354257	61.49%	8.596%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042623.D
 Acq On : 27 Jul 2024 01:03
 Operator : JC/MD
 Sample : P3335-07 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.603	1888	1889	1891	rBV	167	156	0.03%	0.004%
78	12.719	1907	1908	1911	rBV	356	369	0.06%	0.009%
79	12.798	1918	1921	1923	rBB	251	206	0.04%	0.005%
80	12.817	1923	1924	1927	rBB	150	121	0.02%	0.003%
81	12.847	1927	1929	1930	rBV	179	139	0.02%	0.003%
82	12.939	1941	1944	1947	rBV	163	277	0.05%	0.007%
83	13.073	1964	1966	1967	rVB	238	140	0.02%	0.003%
84	13.091	1968	1969	1972	rBB	257	231	0.04%	0.006%
85	13.122	1972	1974	1975	rBB	214	108	0.02%	0.003%
86	13.152	1975	1979	1980	rBV2	204	252	0.04%	0.006%
87	13.347	2009	2011	2013	rBV	161	146	0.03%	0.004%
88	13.384	2013	2017	2019	rVV2	210	265	0.05%	0.006%
89	13.500	2032	2036	2038	rBV2	205	266	0.05%	0.006%
90	13.969	2111	2113	2116	rVB	178	177	0.03%	0.004%
91	13.999	2116	2118	2120	rBV	267	240	0.04%	0.006%
92	14.146	2139	2142	2143	rBV	209	230	0.04%	0.006%
93	14.231	2152	2156	2158	rBV2	259	454	0.08%	0.011%
94	14.359	2176	2177	2179	rBV2	141	140	0.02%	0.003%
95	14.597	2213	2216	2218	rBV	264	363	0.06%	0.009%
96	14.652	2223	2225	2227	rVB	233	205	0.04%	0.005%
97	14.786	2245	2247	2249	rVB	212	129	0.02%	0.003%
98	14.804	2249	2250	2251	rBV	193	135	0.02%	0.003%
99	14.853	2256	2258	2262	rBV2	328	405	0.07%	0.010%
100	14.902	2265	2266	2269	rBV2	296	257	0.04%	0.006%

Sum of corrected areas: 4121418




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042623.D
Acq On : 27 Jul 2024 01:03
Operator : JC/MD
Sample : P3335-07 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

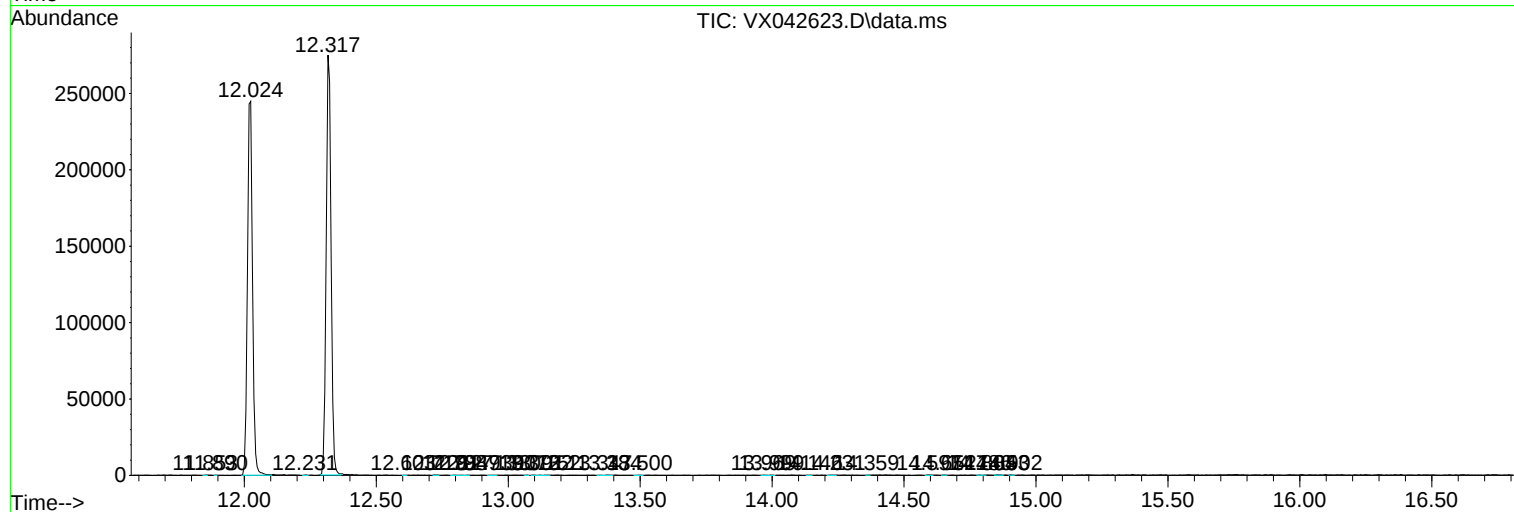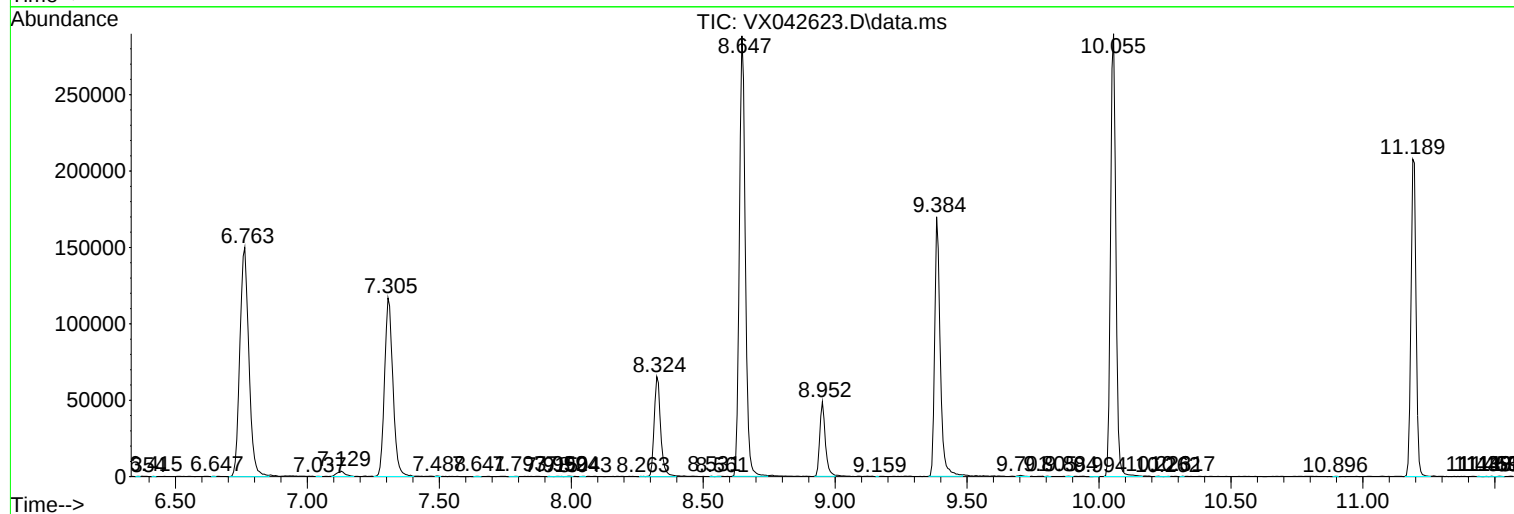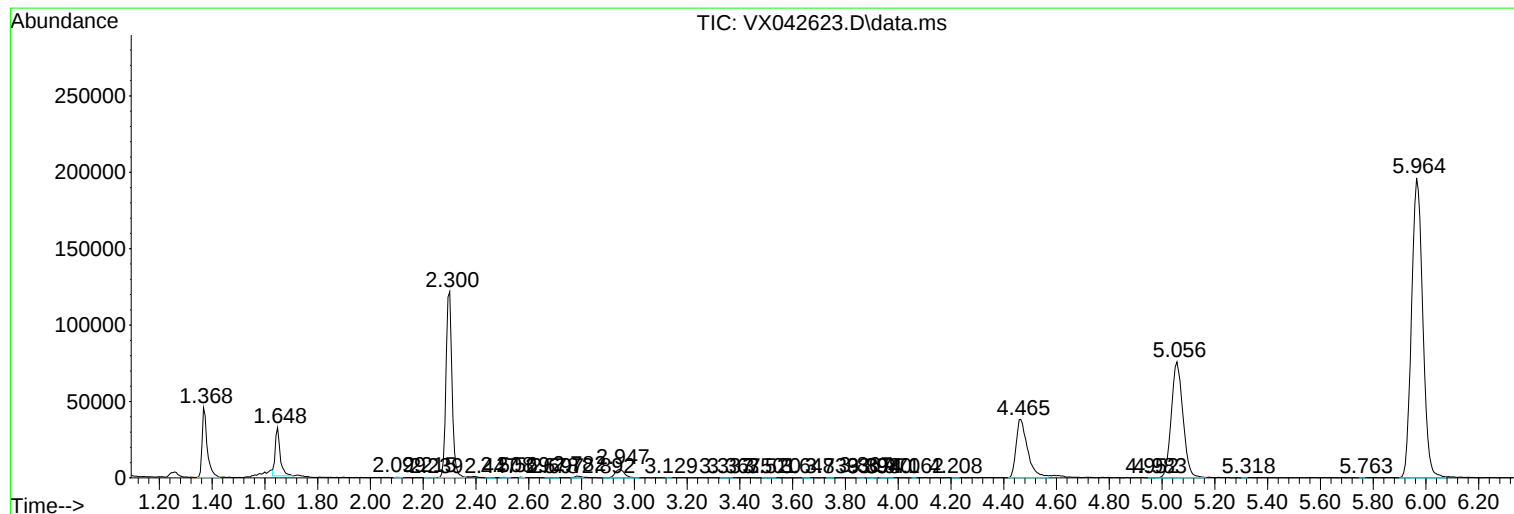

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042623.D
Acq On : 27 Jul 2024 01:03
Operator : JC/MD
Sample : P3335-07 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042623.D
Acq On : 27 Jul 2024 01:03
Operator : JC/MD
Sample : P3335-07 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc