

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042641.D
 Acq On : 27 Jul 2024 07:58
 Operator : JC/MD
 Sample : P3276-23ME 10X
 Misc : 9.94g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20L1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	61	rBV	34367	52190	3.45%	0.997%
2	1.648	89	92	102	rVB	25370	39641	2.62%	0.758%
3	2.197	181	182	183	rBV	196	107	0.01%	0.002%
4	2.215	183	185	187	rVV	254	174	0.01%	0.003%
5	2.294	192	198	211	rVV	96389	154566	10.21%	2.954%
6	2.459	224	225	227	rBV	175	125	0.01%	0.002%
7	2.684	261	262	266	rBV	166	160	0.01%	0.003%
8	2.788	274	279	283	rBV4	1098	1876	0.12%	0.036%
9	2.892	294	296	297	rBV	214	144	0.01%	0.003%
10	2.940	298	304	318	rVB2	6886	16100	1.06%	0.308%
11	3.099	328	330	332	rBB	133	117	0.01%	0.002%
12	3.123	332	334	335	rBV	277	210	0.01%	0.004%
13	3.276	357	359	361	rBV	235	218	0.01%	0.004%
14	3.416	379	382	385	rBV	156	189	0.01%	0.004%
15	3.587	407	410	411	rBV	196	213	0.01%	0.004%
16	3.684	423	426	431	rBV	247	358	0.02%	0.007%
17	3.751	435	437	438	rBB	184	122	0.01%	0.002%
18	3.782	439	442	443	rBV	144	156	0.01%	0.003%
19	3.843	450	452	455	rBV	114	114	0.01%	0.002%
20	3.940	466	468	471	rBV2	241	366	0.02%	0.007%
21	4.032	478	483	484	rBV2	298	381	0.03%	0.007%
22	4.087	491	492	495	rVB	229	123	0.01%	0.002%
23	4.111	495	496	498	rBV	130	132	0.01%	0.003%
24	4.330	530	532	535	rBB	249	220	0.01%	0.004%
25	4.373	535	539	541	rBV	209	360	0.02%	0.007%
26	4.471	546	555	570	rBV	31190	97393	6.43%	1.861%
27	4.800	607	609	612	rVB2	518	360	0.02%	0.007%
28	4.836	612	615	616	rBV2	286	260	0.02%	0.005%
29	4.958	631	635	636	rBV	145	193	0.01%	0.004%
30	5.056	640	651	664	rBV2	60554	185152	12.23%	3.539%
31	5.257	682	684	689	rBV2	310	384	0.03%	0.007%
32	5.330	691	696	697	rBV2	208	341	0.02%	0.007%
33	5.361	700	701	703	rBV	155	139	0.01%	0.003%
34	5.672	750	752	755	rVB2	231	151	0.01%	0.003%
35	5.775	766	769	770	rBV2	292	327	0.02%	0.006%
36	5.842	777	780	783	rBV	246	286	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042641.D
 Acq On : 27 Jul 2024 07:58
 Operator : JC/MD
 Sample : P3276-23ME 10X
 Misc : 9.94g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20L1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.964	789	800	816	rBV3	161308	474390	31.33%	9.066%
38	6.245	845	846	852	rBV2	311	544	0.04%	0.010%
39	6.300	853	855	857	rVB2	371	266	0.02%	0.005%
40	6.361	858	865	868	rBV2	357	680	0.04%	0.013%
41	6.672	914	916	918	rBB2	219	167	0.01%	0.003%
42	6.757	922	930	945	rVV	156867	381321	25.18%	7.288%
43	7.123	981	990	1002	rBV	694325	1514311	100.00%	28.941%
44	7.306	1013	1020	1034	rVB	94396	212668	14.04%	4.064%
45	7.738	1089	1091	1092	rBV	237	201	0.01%	0.004%
46	7.897	1113	1117	1121	rVB	273	412	0.03%	0.008%
47	7.927	1121	1122	1125	rBV	178	191	0.01%	0.004%
48	7.958	1125	1127	1129	rBV	163	128	0.01%	0.002%
49	8.049	1138	1142	1144	rBV	194	299	0.02%	0.006%
50	8.214	1167	1169	1172	rBV2	215	171	0.01%	0.003%
51	8.287	1179	1181	1182	rBV	291	238	0.02%	0.005%
52	8.324	1182	1187	1200	rVB	48321	84251	5.56%	1.610%
53	8.543	1221	1223	1226	rBV	256	286	0.02%	0.005%
54	8.647	1234	1240	1254	rBV	231260	370594	24.47%	7.083%
55	8.952	1282	1290	1304	rBV	35662	55826	3.69%	1.067%
56	9.275	1338	1343	1350	rBV	19246	28460	1.88%	0.544%
57	9.391	1356	1362	1383	rBV	126511	206370	13.63%	3.944%
58	9.708	1410	1414	1417	rVB2	854	1206	0.08%	0.023%
59	9.836	1433	1435	1441	rBV2	312	458	0.03%	0.009%
60	9.958	1453	1455	1456	rBV	157	139	0.01%	0.003%
61	9.994	1459	1461	1465	rBV2	218	124	0.01%	0.002%
62	10.055	1465	1471	1481	rBV	312959	442056	29.19%	8.448%
63	10.409	1527	1529	1532	rVB	121	125	0.01%	0.002%
64	10.646	1567	1568	1571	rBV	154	139	0.01%	0.003%
65	10.713	1577	1579	1580	rBV	351	290	0.02%	0.006%
66	10.799	1590	1593	1596	rBV	192	287	0.02%	0.005%
67	10.915	1609	1612	1613	rBV	194	173	0.01%	0.003%
68	10.927	1613	1614	1616	rBV	229	167	0.01%	0.003%
69	11.079	1637	1639	1645	rBB2	295	419	0.03%	0.008%
70	11.140	1645	1649	1652	rBV	222	355	0.02%	0.007%
71	11.189	1652	1657	1668	rBV	171428	232057	15.32%	4.435%
72	11.396	1689	1691	1694	rBB	219	224	0.01%	0.004%
73	11.427	1694	1696	1699	rBV	220	251	0.02%	0.005%
74	11.591	1720	1723	1728	rBV2	316	415	0.03%	0.008%
75	11.634	1728	1730	1731	rVV2	196	124	0.01%	0.002%
76	11.665	1731	1735	1736	rBV2	160	155	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042641.D
 Acq On : 27 Jul 2024 07:58
 Operator : JC/MD
 Sample : P3276-23ME 10X
 Misc : 9.94g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20L1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.817	1759	1760	1762	rBV2	218	208	0.01%	0.004%
78	11.896	1770	1773	1775	rBB	260	215	0.01%	0.004%
79	11.914	1775	1776	1779	rBV	170	184	0.01%	0.004%
80	12.024	1788	1794	1803	rBV	281280	363033	23.97%	6.938%
81	12.183	1819	1820	1822	rBV2	220	142	0.01%	0.003%
82	12.317	1837	1842	1854	rBV	229568	300401	19.84%	5.741%
83	12.488	1867	1870	1873	rBV	198	325	0.02%	0.006%
84	12.609	1888	1890	1891	rBV	204	166	0.01%	0.003%
85	12.713	1906	1907	1909	rVB	194	109	0.01%	0.002%
86	12.792	1918	1920	1923	rVB2	165	112	0.01%	0.002%
87	13.097	1968	1970	1972	rBB	286	190	0.01%	0.004%
88	13.128	1972	1975	1979	rBV	238	455	0.03%	0.009%
89	13.323	2005	2007	2009	rBV	256	245	0.02%	0.005%
90	13.506	2034	2037	2038	rBV	212	175	0.01%	0.003%
91	13.524	2038	2040	2041	rBV	219	118	0.01%	0.002%
92	13.847	2089	2093	2096	rBV	218	275	0.02%	0.005%
93	13.957	2109	2111	2112	rVB	219	112	0.01%	0.002%
94	14.091	2128	2133	2135	rBV2	275	343	0.02%	0.007%
95	14.292	2165	2166	2169	rBV	169	227	0.01%	0.004%
96	14.469	2194	2195	2197	rVB	238	111	0.01%	0.002%
97	14.487	2197	2198	2199	rBV	197	141	0.01%	0.003%
98	14.682	2228	2230	2234	rBV2	299	327	0.02%	0.006%
99	15.249	2322	2323	2325	rBV2	292	222	0.01%	0.004%
100	16.725	2563	2565	2566	rBV	431	265	0.02%	0.005%




Sum of corrected areas: 5232387

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042641.D
Acq On : 27 Jul 2024 07:58
Operator : JC/MD
Sample : P3276-23ME 10X
Misc : 9.94g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20L1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

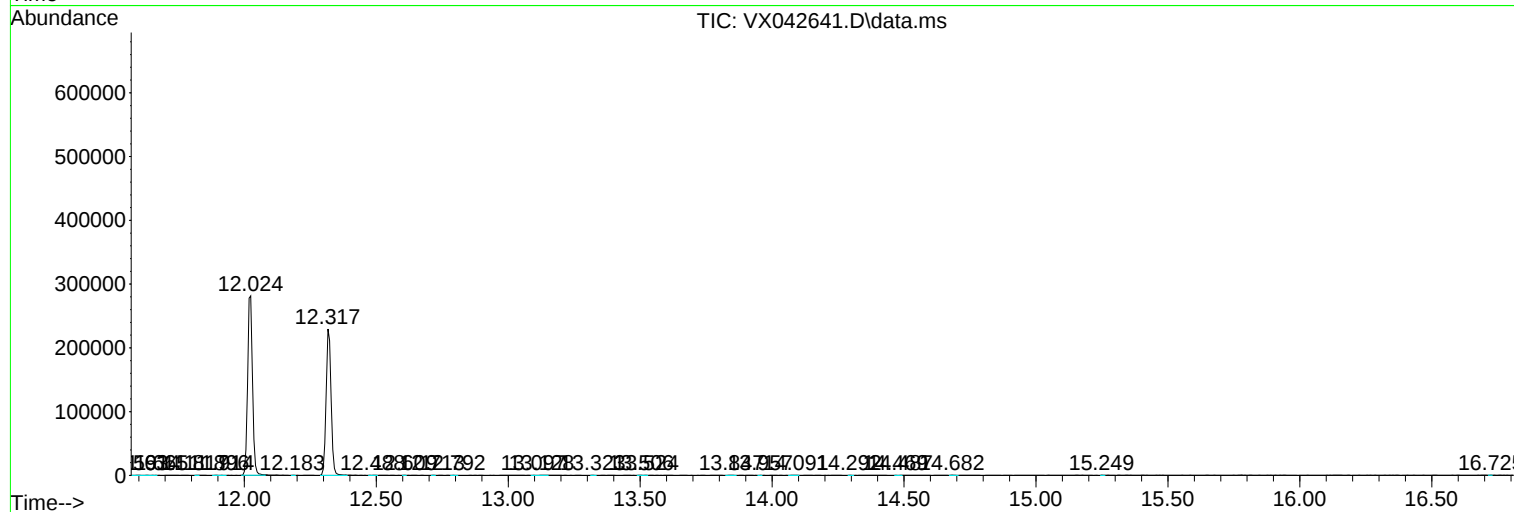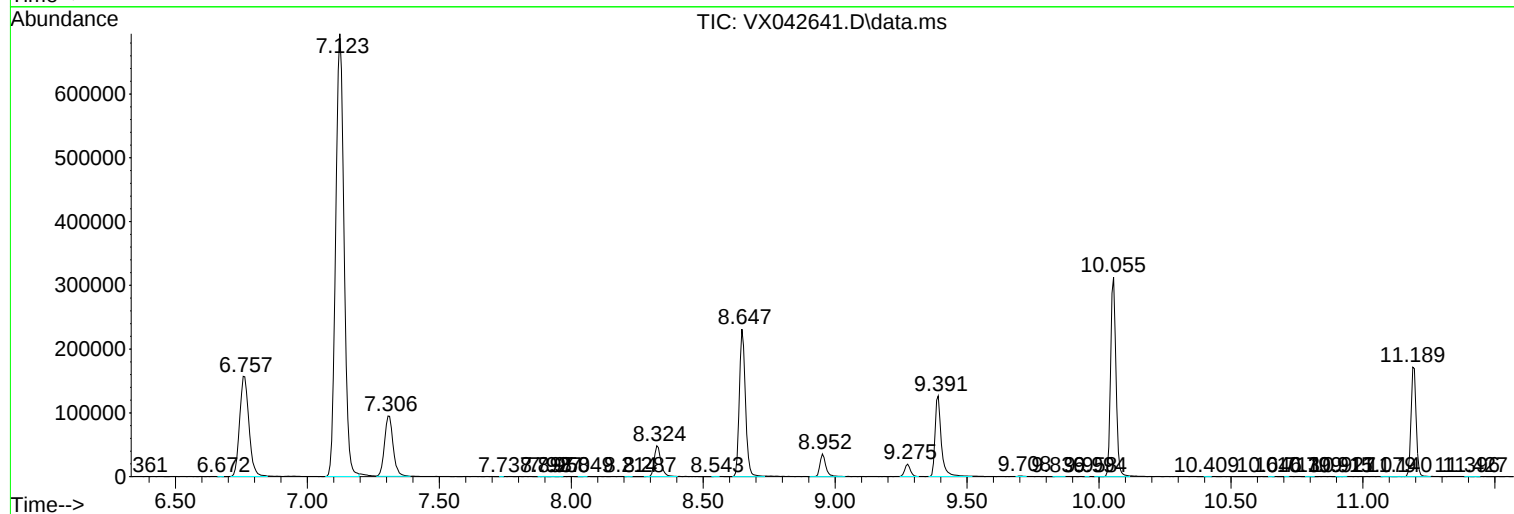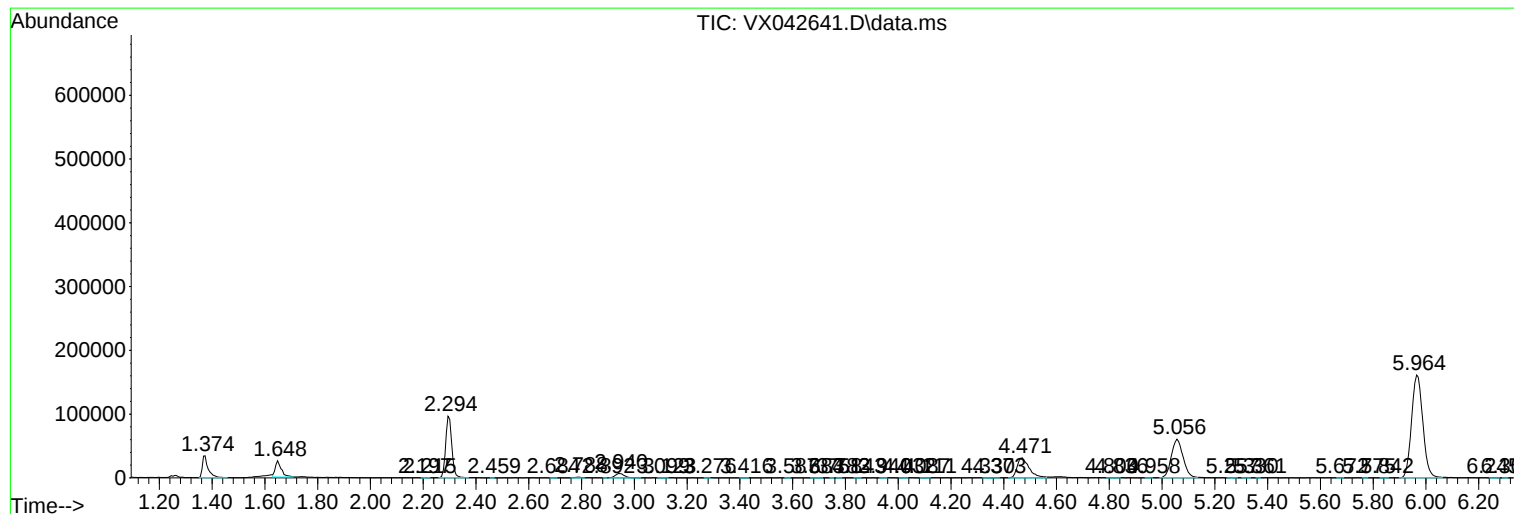

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042641.D
Acq On : 27 Jul 2024 07:58
Operator : JC/MD
Sample : P3276-23ME 10X
Misc : 9.94g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20L1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042641.D
Acq On : 27 Jul 2024 07:58
Operator : JC/MD
Sample : P3276-23ME 10X
Misc : 9.94g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20L1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------