

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042643.D
 Acq On : 27 Jul 2024 17:40
 Operator : JC/MD
 Sample : VX0728WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK702

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	59	rVB	56905	68595	11.05%	1.487%
2	1.660	89	94	99	rBV	37272	52022	8.38%	1.128%
3	1.831	121	122	124	rBV	326	146	0.02%	0.003%
4	2.014	150	152	153	rBV	333	214	0.03%	0.005%
5	2.300	193	199	210	rBV	132586	213886	34.44%	4.637%
6	2.514	228	234	238	rBB	617	940	0.15%	0.020%
7	2.672	254	260	263	rBV2	208	409	0.07%	0.009%
8	2.757	272	274	275	rBV	199	161	0.03%	0.003%
9	2.788	275	279	282	rVV4	935	1430	0.23%	0.031%
10	2.873	289	293	295	rBB	170	186	0.03%	0.004%
11	2.946	300	305	308	rBB2	458	620	0.10%	0.013%
12	3.026	315	318	320	rBV	119	170	0.03%	0.004%
13	3.081	324	327	330	rBV	258	318	0.05%	0.007%
14	3.282	359	360	363	rVB	290	177	0.03%	0.004%
15	3.337	366	369	371	rBB	201	157	0.03%	0.003%
16	3.520	396	399	400	rBB	162	137	0.02%	0.003%
17	3.574	405	408	410	rBV	206	190	0.03%	0.004%
18	3.611	413	414	417	rBB	226	157	0.03%	0.003%
19	3.648	417	420	422	rBV	212	188	0.03%	0.004%
20	3.788	441	443	449	rBV	143	272	0.04%	0.006%
21	3.891	454	460	462	rBB2	192	316	0.05%	0.007%
22	3.995	476	477	482	rBB	166	227	0.04%	0.005%
23	4.044	482	485	486	rBV	241	219	0.04%	0.005%
24	4.093	490	493	494	rBV	171	191	0.03%	0.004%
25	4.318	528	530	533	rVB	165	127	0.02%	0.003%
26	4.452	544	552	571	rBV	45488	132096	21.27%	2.864%
27	4.818	610	612	614	rVB	278	185	0.03%	0.004%
28	4.970	636	637	638	rBV	257	151	0.02%	0.003%
29	5.050	638	650	669	rVV2	85449	257762	41.51%	5.588%
30	5.275	685	687	690	rBB2	178	177	0.03%	0.004%
31	5.300	690	691	693	rBV	177	133	0.02%	0.003%
32	5.385	698	705	709	rBV2	1128	2368	0.38%	0.051%
33	5.501	722	724	725	rBV2	243	143	0.02%	0.003%
34	5.653	746	749	753	rBV	236	297	0.05%	0.006%
35	5.775	764	769	772	rBV2	219	405	0.07%	0.009%
36	5.964	789	800	814	rBV2	208655	621022	100.00%	13.462%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042643.D
 Acq On : 27 Jul 2024 17:40
 Operator : JC/MD
 Sample : VX0728WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK702

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.245	844	846	848	rBV	207	174	0.03%	0.004%
38	6.306	853	856	859	rBV2	290	396	0.06%	0.009%
39	6.415	873	874	878	rBV	169	230	0.04%	0.005%
40	6.531	890	893	895	rVB2	271	251	0.04%	0.005%
41	6.549	895	896	898	rBV2	174	124	0.02%	0.003%
42	6.580	898	901	903	rVB	289	236	0.04%	0.005%
43	6.598	903	904	908	rBB	203	211	0.03%	0.005%
44	6.653	908	913	916	rBV2	203	379	0.06%	0.008%
45	6.757	920	930	943	rBV	165907	404582	65.15%	8.770%
46	7.305	1009	1020	1038	rVV	122450	277534	44.69%	6.016%
47	7.488	1048	1050	1052	rBV2	364	207	0.03%	0.004%
48	7.574	1061	1064	1066	rBV2	155	167	0.03%	0.004%
49	7.598	1066	1068	1073	rVV	246	217	0.03%	0.005%
50	7.635	1073	1074	1077	rVB	223	184	0.03%	0.004%
51	7.659	1077	1078	1081	rBB	151	138	0.02%	0.003%
52	7.927	1120	1122	1123	rBV	212	144	0.02%	0.003%
53	7.946	1123	1125	1130	rVB	153	203	0.03%	0.004%
54	8.183	1162	1164	1166	rVV	233	189	0.03%	0.004%
55	8.324	1175	1187	1203	rBV	79516	134018	21.58%	2.905%
56	8.494	1212	1215	1216	rBV2	128	123	0.02%	0.003%
57	8.586	1227	1230	1231	rBV	196	209	0.03%	0.005%
58	8.647	1233	1240	1257	rVV	312993	492022	79.23%	10.666%
59	8.945	1285	1289	1301	rBV	54886	87632	14.11%	1.900%
60	9.165	1323	1325	1327	rVB	182	133	0.02%	0.003%
61	9.268	1337	1342	1348	rBB3	824	1174	0.19%	0.025%
62	9.323	1348	1351	1353	rBV2	285	326	0.05%	0.007%
63	9.384	1355	1361	1377	rBV	185163	279858	45.06%	6.067%
64	9.683	1408	1410	1416	rBV3	267	424	0.07%	0.009%
65	9.726	1416	1417	1419	rVB3	194	129	0.02%	0.003%
66	9.890	1441	1444	1445	rBV	203	250	0.04%	0.005%
67	9.994	1459	1461	1465	rBV	240	362	0.06%	0.008%
68	10.049	1465	1470	1487	rVV	335133	468573	75.45%	10.158%
69	10.945	1616	1617	1619	rBV	161	145	0.02%	0.003%
70	11.073	1637	1638	1642	rBB	162	129	0.02%	0.003%
71	11.189	1652	1657	1668	rBV	238112	307056	49.44%	6.656%
72	11.341	1680	1682	1684	rVB	371	247	0.04%	0.005%
73	11.360	1684	1685	1688	rVB	245	132	0.02%	0.003%
74	11.390	1688	1690	1692	rBV	208	196	0.03%	0.004%
75	11.481	1703	1705	1707	rBV	167	175	0.03%	0.004%
76	11.579	1718	1721	1723	rBV2	204	252	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042643.D
 Acq On : 27 Jul 2024 17:40
 Operator : JC/MD
 Sample : VX0728WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK702

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.847	1762	1765	1767	rBV	254	291	0.05%	0.006%
78	11.969	1783	1785	1788	rBV	129	151	0.02%	0.003%
79	12.018	1788	1793	1805	rBV	313219	388365	62.54%	8.419%
80	12.213	1821	1825	1827	rVB2	248	308	0.05%	0.007%
81	12.317	1837	1842	1853	rBV	329447	403000	64.89%	8.736%
82	12.573	1878	1884	1885	rBV	260	409	0.07%	0.009%
83	12.670	1898	1900	1901	rBV	221	171	0.03%	0.004%
84	12.750	1911	1913	1916	rVV2	234	262	0.04%	0.006%
85	12.871	1931	1933	1934	rVB2	232	157	0.03%	0.003%
86	12.975	1948	1950	1952	rBV2	165	184	0.03%	0.004%
87	13.189	1983	1985	1989	rVB2	111	191	0.03%	0.004%
88	13.225	1989	1991	1995	rVB	225	296	0.05%	0.006%
89	13.274	1995	1999	2001	rBV	323	339	0.05%	0.007%
90	13.408	2019	2021	2025	rBV	343	431	0.07%	0.009%
91	13.670	2061	2064	2068	rBV2	321	498	0.08%	0.011%
92	13.853	2092	2094	2099	rBV2	319	414	0.07%	0.009%
93	14.121	2137	2138	2142	rBV	331	366	0.06%	0.008%
94	14.383	2180	2181	2182	rBV	185	127	0.02%	0.003%
95	14.487	2196	2198	2201	rBV	131	123	0.02%	0.003%
96	15.115	2300	2301	2302	rBV	392	219	0.04%	0.005%
97	15.206	2314	2316	2318	rBV	313	245	0.04%	0.005%
98	15.261	2323	2325	2329	rVB2	356	389	0.06%	0.008%
99	15.944	2434	2437	2441	rBV2	273	579	0.09%	0.013%
100	16.017	2447	2449	2450	rBV2	290	188	0.03%	0.004%




Sum of corrected areas: 4613028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042643.D
Acq On : 27 Jul 2024 17:40
Operator : JC/MD
Sample : VX0728WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK702

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

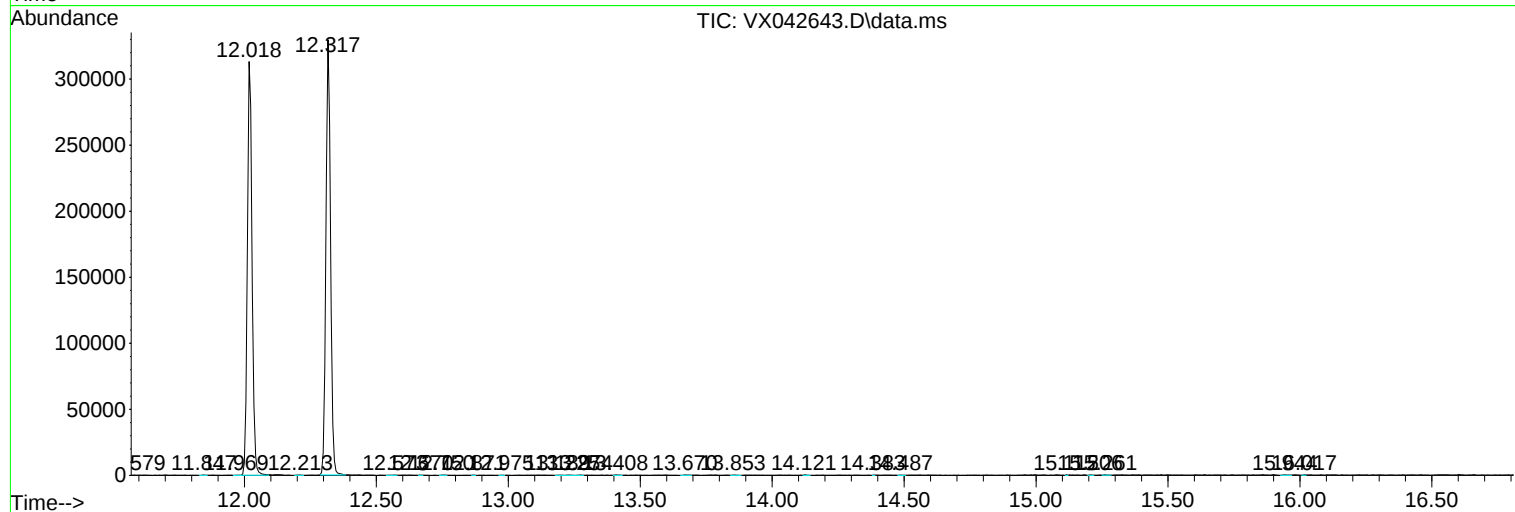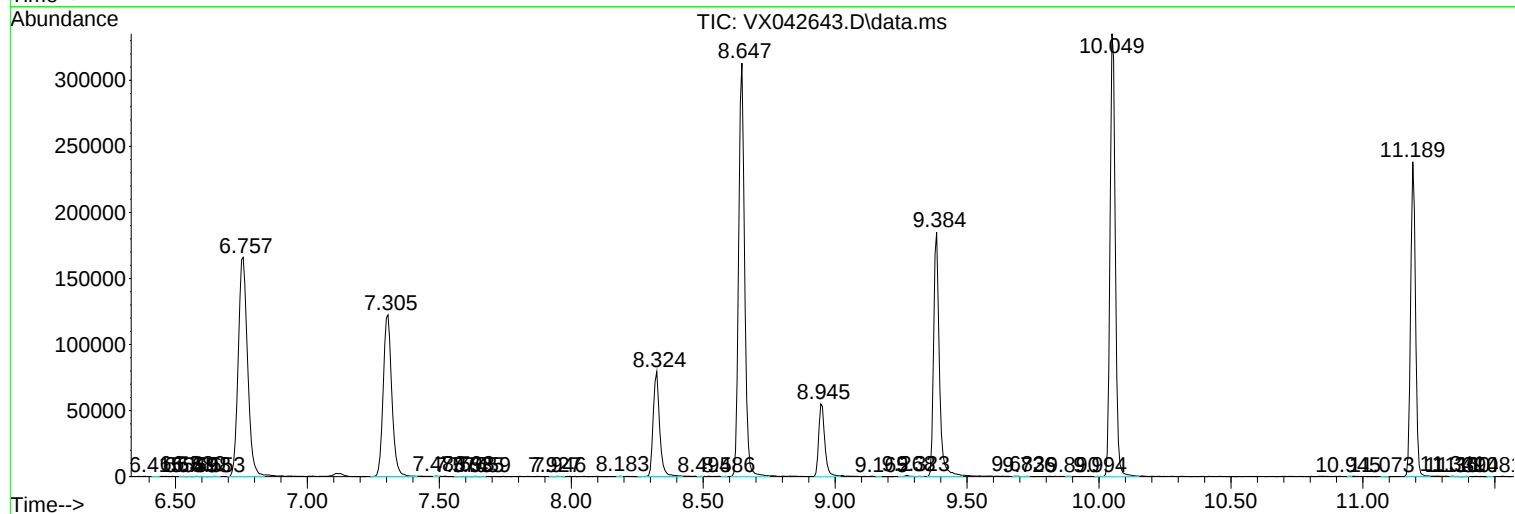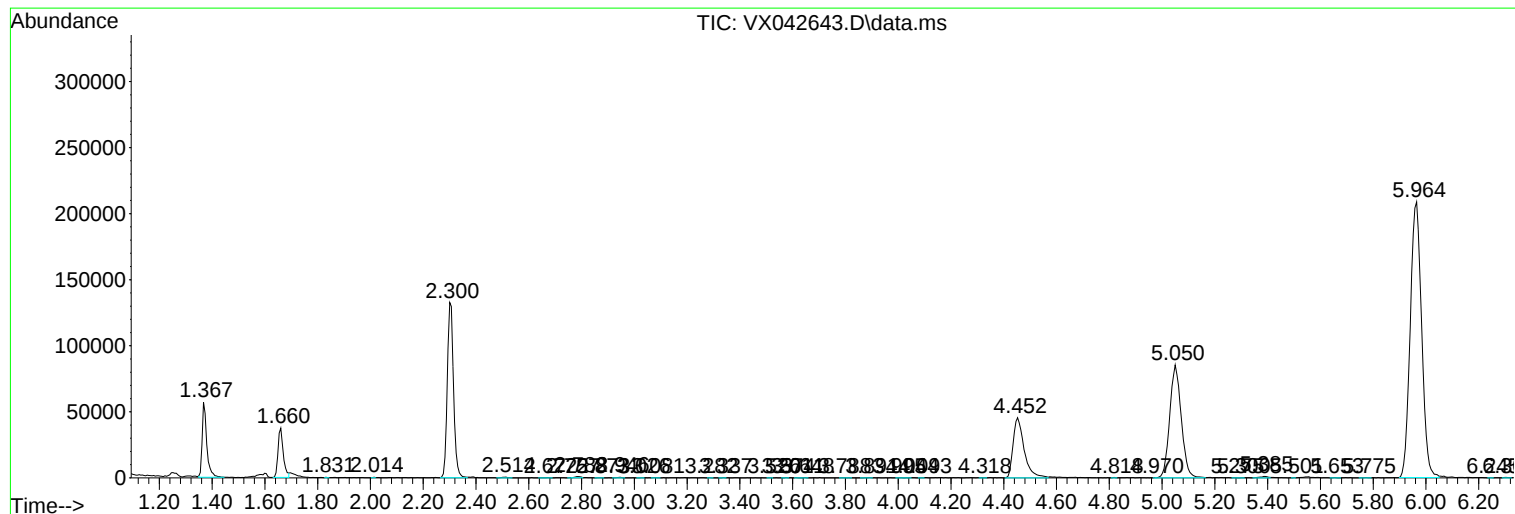

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042643.D
Acq On : 27 Jul 2024 17:40
Operator : JC/MD
Sample : VX0728WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK702

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042643.D
Acq On : 27 Jul 2024 17:40
Operator : JC/MD
Sample : VX0728WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK702

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc