

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042644.D
 Acq On : 27 Jul 2024 18:06
 Operator : JC/MD
 Sample : P3373-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	28	rBV2	3772	5165	0.87%	0.116%
2	1.368	43	46	58	rVB	49560	64172	10.78%	1.440%
3	1.648	89	92	101	rVB	29012	40081	6.73%	0.899%
4	2.191	177	181	182	rBV	311	364	0.06%	0.008%
5	2.300	192	199	209	rBV	124334	196246	32.97%	4.403%
6	2.502	229	232	233	rBV	357	328	0.06%	0.007%
7	2.678	258	261	264	rBB	236	278	0.05%	0.006%
8	2.825	284	285	288	rBV	170	198	0.03%	0.004%
9	2.940	298	304	310	rBV3	1830	4144	0.70%	0.093%
10	3.056	320	323	324	rBV2	221	233	0.04%	0.005%
11	3.099	327	330	334	rVV3	513	764	0.13%	0.017%
12	3.154	338	339	341	rBV3	136	131	0.02%	0.003%
13	3.203	345	347	349	rVB	216	142	0.02%	0.003%
14	3.221	349	350	353	rBV	127	154	0.03%	0.003%
15	3.318	364	366	371	rBV	225	327	0.05%	0.007%
16	3.489	392	394	399	rBB	169	220	0.04%	0.005%
17	3.544	400	403	405	rBV	203	247	0.04%	0.006%
18	3.623	413	416	417	rBV	151	173	0.03%	0.004%
19	3.678	424	425	429	rBV	216	227	0.04%	0.005%
20	3.977	472	474	478	rBV	251	387	0.07%	0.009%
21	4.032	481	483	485	rBV	205	256	0.04%	0.006%
22	4.068	488	489	492	rBV	236	257	0.04%	0.006%
23	4.129	495	499	501	rBB	224	302	0.05%	0.007%
24	4.391	540	542	544	rBV	188	134	0.02%	0.003%
25	4.458	545	553	568	rBV	39645	119323	20.05%	2.677%
26	4.733	597	598	601	rBV2	382	365	0.06%	0.008%
27	4.879	619	622	624	rVB	245	203	0.03%	0.005%
28	4.934	629	631	632	rBV	197	157	0.03%	0.004%
29	4.971	636	637	639	rBV	250	146	0.02%	0.003%
30	5.056	639	651	667	rBV	80927	247873	41.64%	5.561%
31	5.257	682	684	686	rVB	385	276	0.05%	0.006%
32	5.281	686	688	691	rBV2	235	263	0.04%	0.006%
33	5.641	745	747	750	rBV	161	157	0.03%	0.004%
34	5.727	759	761	763	rBV2	266	226	0.04%	0.005%
35	5.806	773	774	776	rBV	133	121	0.02%	0.003%
36	5.964	789	800	820	rBV2	200988	595228	100.00%	13.354%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042644.D
 Acq On : 27 Jul 2024 18:06
 Operator : JC/MD
 Sample : P3373-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.568	896	899	903	rBV	262	310	0.05%	0.007%
38	6.757	920	930	947	rBV	176600	429098	72.09%	9.627%
39	7.037	974	976	977	rBV	325	269	0.05%	0.006%
40	7.306	1012	1020	1034	rBV	121382	264852	44.50%	5.942%
41	7.665	1077	1079	1081	rVB	300	197	0.03%	0.004%
42	7.690	1081	1083	1084	rBV	163	132	0.02%	0.003%
43	7.818	1101	1104	1106	rBV2	380	403	0.07%	0.009%
44	7.982	1129	1131	1134	rBV	224	270	0.05%	0.006%
45	8.110	1149	1152	1156	rBV	229	367	0.06%	0.008%
46	8.153	1156	1159	1160	rVV	187	147	0.02%	0.003%
47	8.202	1164	1167	1169	rVB	146	159	0.03%	0.004%
48	8.324	1181	1187	1198	rBV2	73505	122666	20.61%	2.752%
49	8.482	1211	1213	1215	rBV2	377	297	0.05%	0.007%
50	8.647	1234	1240	1249	rBV	300316	471965	79.29%	10.588%
51	8.952	1284	1290	1299	rBV	52783	80926	13.60%	1.816%
52	9.086	1310	1312	1316	rVB	267	267	0.04%	0.006%
53	9.116	1316	1317	1319	rBV	243	179	0.03%	0.004%
54	9.275	1338	1343	1349	rVB2	2151	3163	0.53%	0.071%
55	9.348	1352	1355	1356	rBV	158	188	0.03%	0.004%
56	9.384	1356	1361	1377	rBV	173252	255587	42.94%	5.734%
57	9.598	1394	1396	1397	rBV	350	264	0.04%	0.006%
58	9.701	1411	1413	1415	rBV	272	282	0.05%	0.006%
59	9.726	1415	1417	1419	rBV	265	165	0.03%	0.004%
60	9.939	1450	1452	1456	rBV2	174	205	0.03%	0.005%
61	10.049	1465	1470	1481	rBV	331161	484590	81.41%	10.872%
62	10.305	1509	1512	1520	rVB3	1090	1893	0.32%	0.042%
63	10.470	1537	1539	1541	rBV2	269	263	0.04%	0.006%
64	10.561	1551	1554	1556	rBV	231	300	0.05%	0.007%
65	10.701	1575	1577	1579	rBV2	236	253	0.04%	0.006%
66	10.750	1582	1585	1588	rVV2	216	383	0.06%	0.009%
67	10.805	1591	1594	1595	rBV	373	275	0.05%	0.006%
68	11.012	1627	1628	1630	rBB	184	127	0.02%	0.003%
69	11.189	1652	1657	1666	rBV	220862	283437	47.62%	6.359%
70	11.311	1675	1677	1683	rVB	2455	2391	0.40%	0.054%
71	11.372	1686	1687	1688	rBV	187	116	0.02%	0.003%
72	11.451	1698	1700	1703	rVB	202	204	0.03%	0.005%
73	11.506	1708	1709	1713	rVB	313	267	0.04%	0.006%
74	11.536	1713	1714	1717	rBB	154	147	0.02%	0.003%
75	11.695	1737	1740	1743	rBV	248	360	0.06%	0.008%
76	11.823	1758	1761	1763	rBV	240	193	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042644.D
 Acq On : 27 Jul 2024 18:06
 Operator : JC/MD
 Sample : P3373-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.860	1766	1767	1769	rBV	312	182	0.03%	0.004%
78	12.018	1788	1793	1804	rBV	308264	396638	66.64%	8.898%
79	12.219	1824	1826	1832	rVB3	568	778	0.13%	0.017%
80	12.268	1832	1834	1837	rBV2	351	273	0.05%	0.006%
81	12.317	1837	1842	1850	rBV	297876	368471	61.90%	8.266%
82	12.524	1875	1876	1879	rVB	166	140	0.02%	0.003%
83	12.658	1896	1898	1900	rBV2	219	217	0.04%	0.005%
84	12.713	1904	1907	1909	rBV2	175	254	0.04%	0.006%
85	12.744	1911	1912	1913	rBV	294	213	0.04%	0.005%
86	12.902	1937	1938	1940	rBV	155	129	0.02%	0.003%
87	13.024	1956	1958	1961	rBV	165	147	0.02%	0.003%
88	13.097	1968	1970	1972	rBV2	226	198	0.03%	0.004%
89	13.189	1984	1985	1988	rBV	189	253	0.04%	0.006%
90	13.323	2005	2007	2009	rBV	173	146	0.02%	0.003%
91	13.457	2027	2029	2032	rBB2	271	292	0.05%	0.007%
92	13.487	2032	2034	2036	rBV	257	202	0.03%	0.005%
93	13.591	2049	2051	2053	rBV2	270	273	0.05%	0.006%
94	13.646	2058	2060	2063	rBV2	192	175	0.03%	0.004%
95	13.890	2098	2100	2102	rBV2	137	156	0.03%	0.003%
96	14.121	2136	2138	2142	rBV2	411	584	0.10%	0.013%
97	14.725	2235	2237	2239	rBV	224	242	0.04%	0.005%
98	14.926	2268	2270	2273	rBV	163	226	0.04%	0.005%
99	15.048	2289	2290	2292	rBV2	250	166	0.03%	0.004%
100	16.048	2453	2454	2456	rBV2	232	225	0.04%	0.005%


Sum of corrected areas: 4457405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042644.D
Acq On : 27 Jul 2024 18:06
Operator : JC/MD
Sample : P3373-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

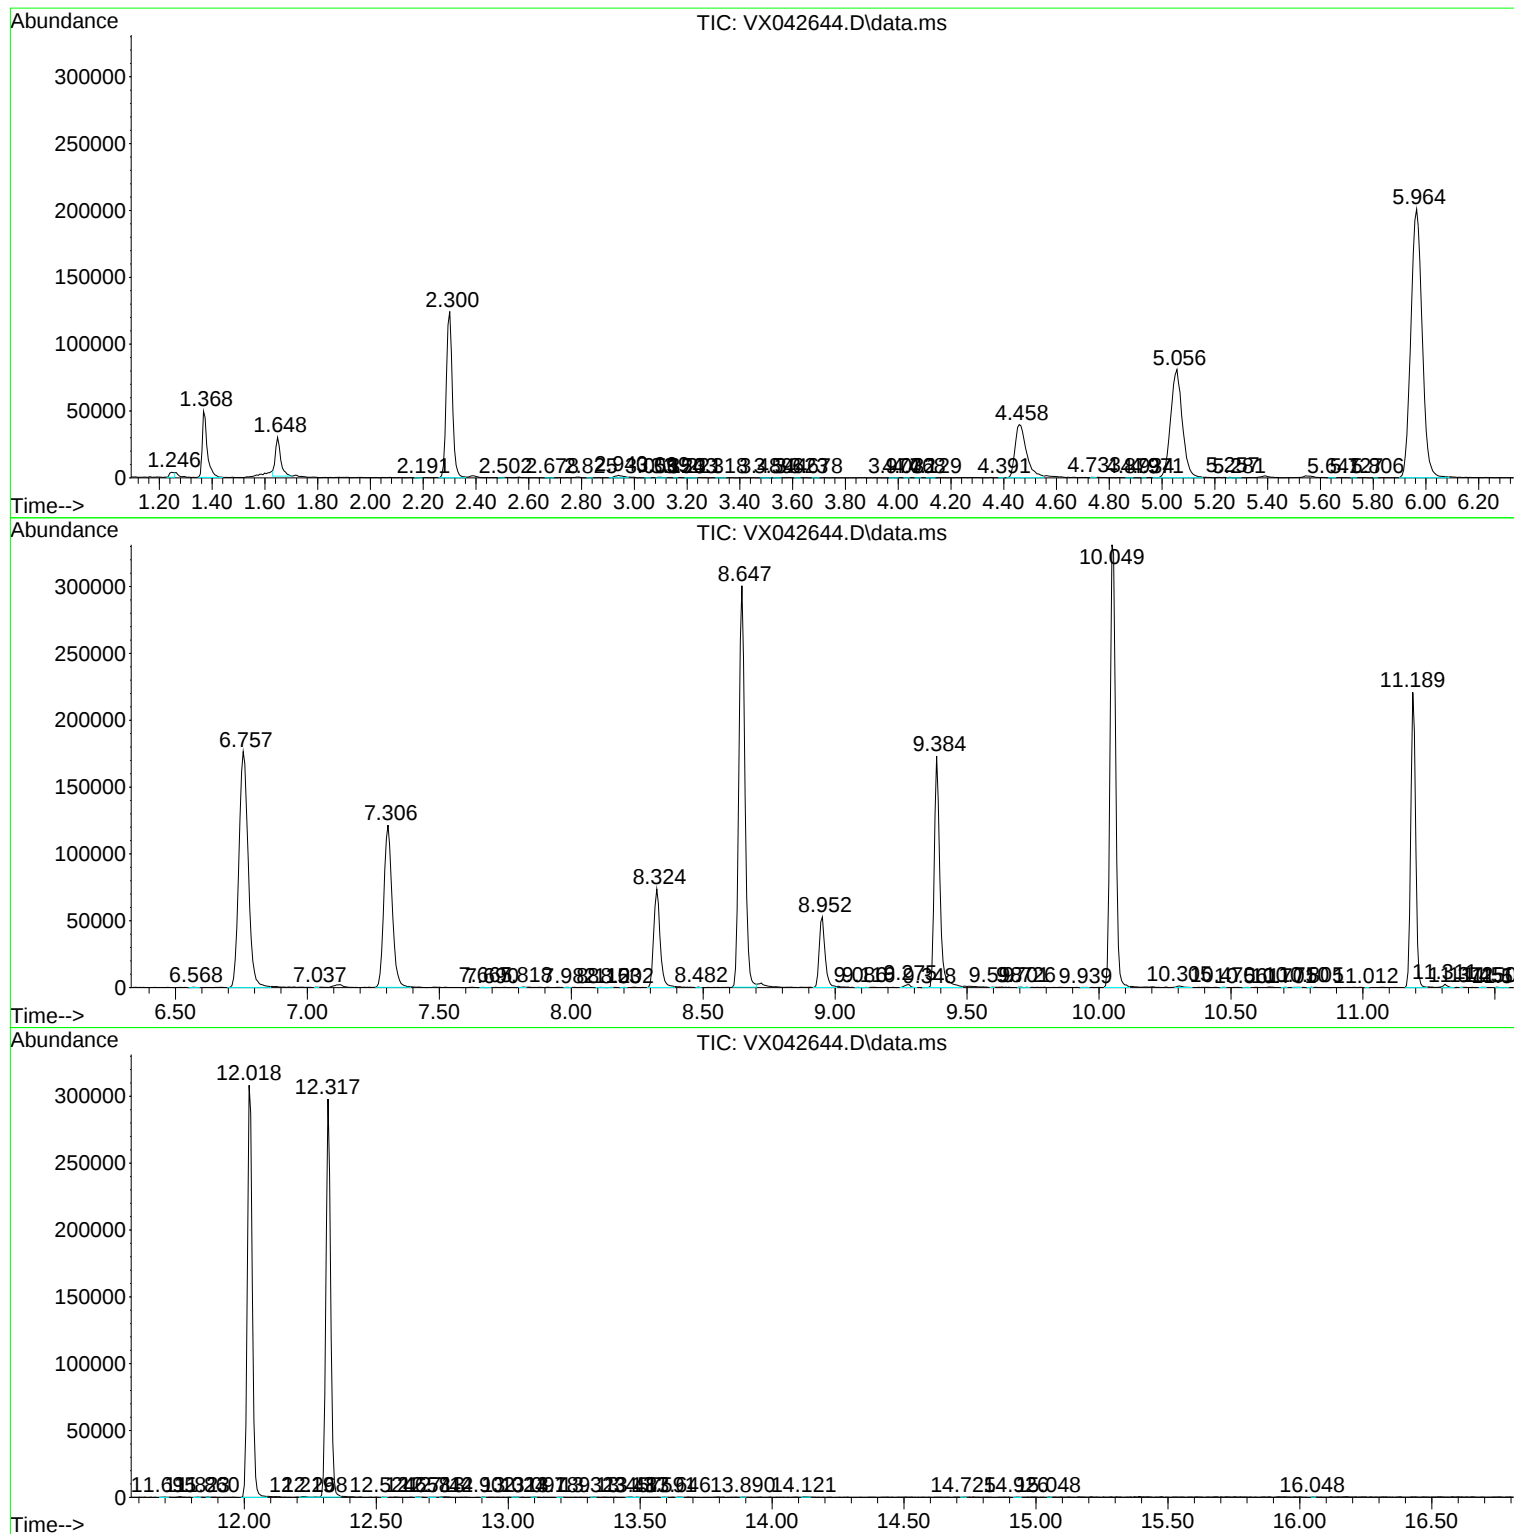

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042644.D
Acq On : 27 Jul 2024 18:06
Operator : JC/MD
Sample : P3373-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042644.D
Acq On : 27 Jul 2024 18:06
Operator : JC/MD
Sample : P3373-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc