

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042646.D
 Acq On : 27 Jul 2024 18:49
 Operator : JC/MD
 Sample : P3373-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	23	26	32	rBV2	4046	7562	1.34%	0.177%
2	1.367	43	46	58	rVB	51554	58965	10.42%	1.381%
3	1.648	89	92	101	rVB	34145	39647	7.00%	0.929%
4	2.300	193	199	210	rVV	114469	184023	32.51%	4.310%
5	2.501	228	232	238	rVB2	427	901	0.16%	0.021%
6	2.562	238	242	243	rBV	363	433	0.08%	0.010%
7	2.739	268	271	274	rBV	159	217	0.04%	0.005%
8	2.782	274	278	281	rBV4	721	1081	0.19%	0.025%
9	2.855	289	290	292	rBV	184	124	0.02%	0.003%
10	3.215	346	349	351	rBV2	205	250	0.04%	0.006%
11	3.269	356	358	359	rBV	146	151	0.03%	0.004%
12	3.367	373	374	377	rVB	205	177	0.03%	0.004%
13	3.416	378	382	383	rBV	119	123	0.02%	0.003%
14	3.568	404	407	409	rBB	303	266	0.05%	0.006%
15	3.605	411	413	416	rBV	262	314	0.06%	0.007%
16	3.714	428	431	432	rBV	133	166	0.03%	0.004%
17	3.769	438	440	442	rBV	240	299	0.05%	0.007%
18	3.910	460	463	464	rBB	132	113	0.02%	0.003%
19	4.025	477	482	484	rBV	250	404	0.07%	0.009%
20	4.178	504	507	508	rBV	91	107	0.02%	0.003%
21	4.269	521	522	528	rVV2	193	273	0.05%	0.006%
22	4.318	528	530	534	rVB	205	214	0.04%	0.005%
23	4.397	541	543	544	rBV	150	118	0.02%	0.003%
24	4.464	547	554	573	rBV	39293	118754	20.98%	2.781%
25	4.934	629	631	638	rBV2	248	342	0.06%	0.008%
26	5.062	639	652	668	rBV	74734	233443	41.25%	5.467%
27	5.220	675	678	679	rBV2	326	261	0.05%	0.006%
28	5.360	697	701	702	rVB	181	220	0.04%	0.005%
29	5.397	702	707	712	rBV3	577	1181	0.21%	0.028%
30	5.434	712	713	714	rBV3	216	107	0.02%	0.003%
31	5.617	742	743	747	rBV2	133	177	0.03%	0.004%
32	5.653	747	749	752	rVB2	234	198	0.03%	0.005%
33	5.684	752	754	760	rBV2	297	330	0.06%	0.008%
34	5.812	773	775	778	rVB2	164	126	0.02%	0.003%
35	5.964	790	800	820	rBV2	191113	565986	100.00%	13.255%
36	6.324	857	859	862	rVB	196	234	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042646.D
 Acq On : 27 Jul 2024 18:49
 Operator : JC/MD
 Sample : P3373-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.372	866	867	869	rBV	434	233	0.04%	0.005%
38	6.470	882	883	887	rBV	185	201	0.04%	0.005%
39	6.507	887	889	891	rBV	206	141	0.02%	0.003%
40	6.549	894	896	899	rBV2	241	298	0.05%	0.007%
41	6.665	913	915	916	rBV	383	297	0.05%	0.007%
42	6.763	921	931	948	rBV2	165584	402750	71.16%	9.432%
43	7.122	984	990	997	rVB6	2179	5354	0.95%	0.125%
44	7.214	1001	1005	1009	rBV	280	474	0.08%	0.011%
45	7.305	1011	1020	1037	rBV	113910	254487	44.96%	5.960%
46	7.592	1064	1067	1068	rBV	279	251	0.04%	0.006%
47	7.830	1102	1106	1109	rBV2	571	829	0.15%	0.019%
48	7.897	1115	1117	1119	rBV2	217	263	0.05%	0.006%
49	8.043	1139	1141	1144	rBV	191	234	0.04%	0.005%
50	8.244	1171	1174	1176	rBV2	214	292	0.05%	0.007%
51	8.323	1181	1187	1202	rBV	67179	117876	20.83%	2.761%
52	8.646	1234	1240	1249	rBV	272724	440039	77.75%	10.306%
53	8.903	1281	1282	1285	rBV2	291	201	0.04%	0.005%
54	8.951	1285	1290	1300	rBV	49301	75971	13.42%	1.779%
55	9.281	1340	1344	1348	rVB2	1585	2297	0.41%	0.054%
56	9.384	1356	1361	1373	rBV	163734	254137	44.90%	5.952%
57	9.750	1420	1421	1424	rBV2	252	223	0.04%	0.005%
58	9.890	1442	1444	1445	rBV	202	192	0.03%	0.004%
59	9.976	1455	1458	1459	rBV	138	139	0.02%	0.003%
60	10.055	1465	1471	1488	rBV	340933	457120	80.77%	10.706%
61	10.317	1509	1514	1518	rBV4	1139	2240	0.40%	0.052%
62	10.427	1531	1532	1534	rBV	140	153	0.03%	0.004%
63	10.579	1555	1557	1559	rBV	293	218	0.04%	0.005%
64	10.652	1564	1569	1574	rBV3	1062	2050	0.36%	0.048%
65	10.750	1583	1585	1587	rBV3	282	288	0.05%	0.007%
66	10.792	1591	1592	1593	rVB	329	126	0.02%	0.003%
67	10.969	1617	1621	1625	rBV3	543	672	0.12%	0.016%
68	11.097	1639	1642	1643	rBV	296	259	0.05%	0.006%
69	11.189	1652	1657	1665	rBV	212302	283178	50.03%	6.632%
70	11.311	1674	1677	1682	rVB	701	950	0.17%	0.022%
71	11.451	1698	1700	1702	rBV2	349	279	0.05%	0.007%
72	11.689	1738	1739	1742	rBV	239	207	0.04%	0.005%
73	12.024	1788	1794	1803	rBV	293598	376183	66.47%	8.810%
74	12.225	1824	1827	1830	rBV	1026	1150	0.20%	0.027%
75	12.317	1837	1842	1853	rBV	276250	363051	64.14%	8.503%
76	12.463	1865	1866	1869	rVB	357	256	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042646.D
 Acq On : 27 Jul 2024 18:49
 Operator : JC/MD
 Sample : P3373-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08K2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.634	1891	1894	1897	rVB	295	299	0.05%	0.007%
78	12.658	1897	1898	1901	rBV	231	151	0.03%	0.004%
79	13.310	2002	2005	2007	rBV2	140	217	0.04%	0.005%
80	13.579	2048	2049	2050	rBV	188	129	0.02%	0.003%
81	13.646	2059	2060	2063	rBV	238	263	0.05%	0.006%
82	13.780	2080	2082	2088	rVV2	439	562	0.10%	0.013%
83	13.938	2106	2108	2111	rBV	177	220	0.04%	0.005%
84	14.011	2118	2120	2121	rBV	201	154	0.03%	0.004%
85	14.158	2143	2144	2147	rBV	312	288	0.05%	0.007%
86	14.188	2147	2149	2150	rVV	217	115	0.02%	0.003%
87	14.274	2159	2163	2167	rBV2	402	679	0.12%	0.016%
88	14.554	2207	2209	2210	rBV2	227	135	0.02%	0.003%
89	14.615	2217	2219	2221	rBV	146	167	0.03%	0.004%
90	14.804	2248	2250	2252	rBV	332	266	0.05%	0.006%
91	14.859	2258	2259	2262	rVB	356	321	0.06%	0.008%
92	14.908	2262	2267	2268	rBV	269	473	0.08%	0.011%
93	14.920	2268	2269	2271	rBV2	329	289	0.05%	0.007%
94	14.987	2279	2280	2281	rBV2	346	191	0.03%	0.004%
95	15.029	2285	2287	2289	rBV	306	331	0.06%	0.008%
96	15.657	2389	2390	2394	rBV	249	265	0.05%	0.006%
97	16.066	2455	2457	2458	rBV2	378	340	0.06%	0.008%
98	16.261	2487	2489	2492	rBV	343	438	0.08%	0.010%
99	16.676	2555	2557	2558	rBV	295	214	0.04%	0.005%
100	16.730	2562	2566	2568	rBV2	295	477	0.08%	0.011%




Sum of corrected areas: 4269830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042646.D
Acq On : 27 Jul 2024 18:49
Operator : JC/MD
Sample : P3373-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

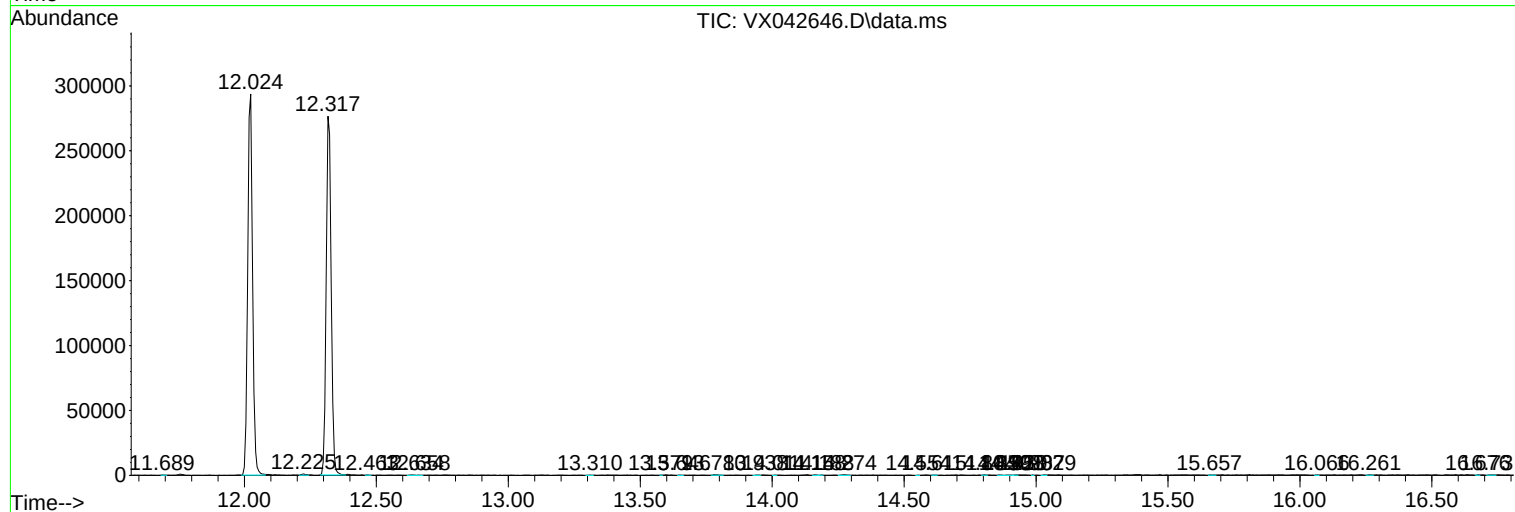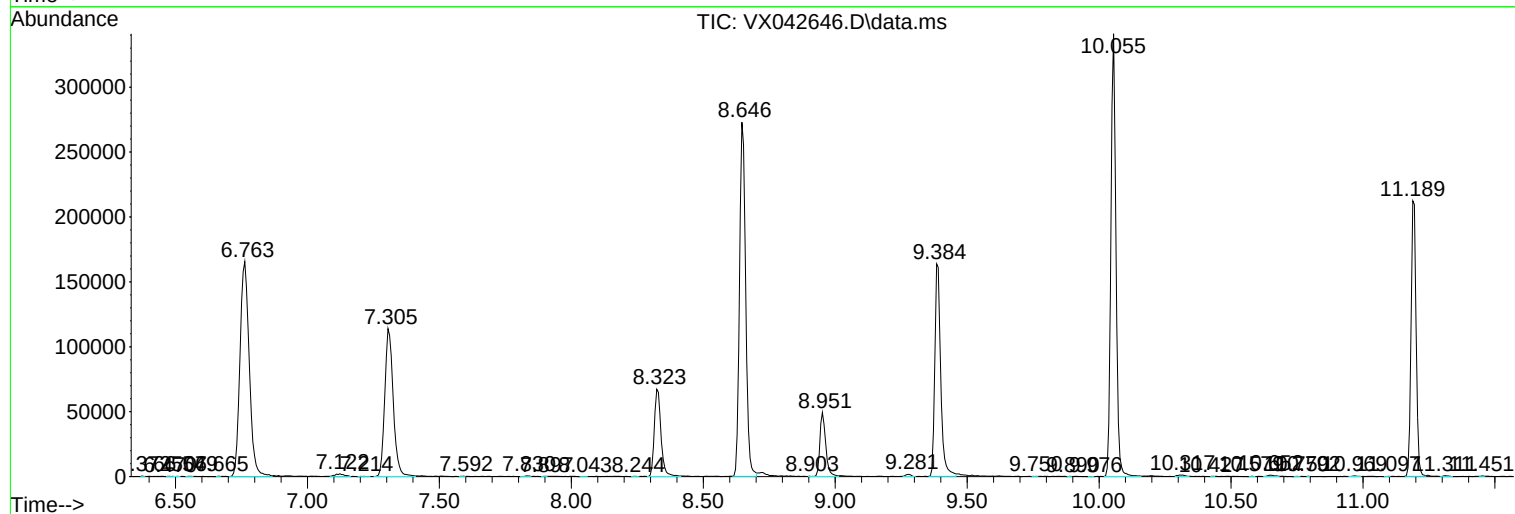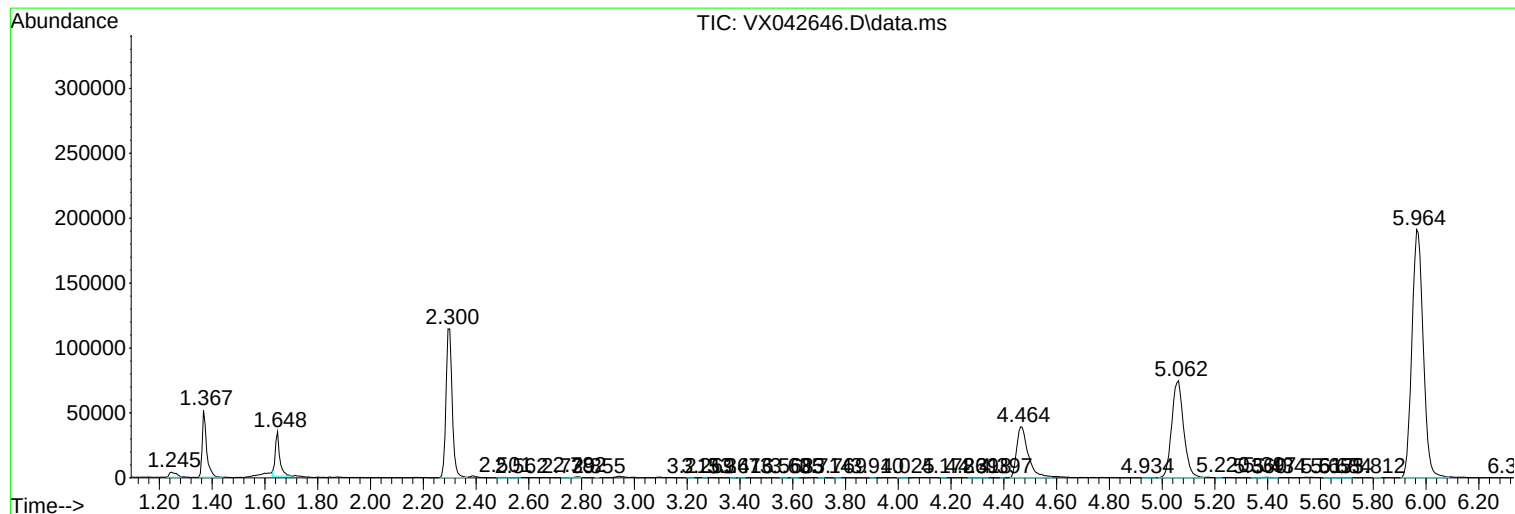

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042646.D
Acq On : 27 Jul 2024 18:49
Operator : JC/MD
Sample : P3373-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042646.D
Acq On : 27 Jul 2024 18:49
Operator : JC/MD
Sample : P3373-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08K2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc