

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042651.D
 Acq On : 27 Jul 2024 20:45
 Operator : JC/MD
 Sample : VX0728WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	36	rVB2	4036	8143	1.40%	0.193%
2	1.368	43	46	56	rVB	47218	61425	10.59%	1.456%
3	1.648	89	92	102	rVB	33054	44498	7.67%	1.055%
4	2.050	156	158	160	rBV	514	296	0.05%	0.007%
5	2.124	169	170	174	rBV	318	365	0.06%	0.009%
6	2.294	192	198	210	rBV	120885	187568	32.33%	4.445%
7	2.654	255	257	261	rVV2	205	271	0.05%	0.006%
8	2.934	301	303	305	rBV	592	802	0.14%	0.019%
9	3.026	314	318	320	rVB	237	342	0.06%	0.008%
10	3.056	321	323	324	rBV	189	167	0.03%	0.004%
11	3.172	338	342	343	rBV	152	179	0.03%	0.004%
12	3.184	343	344	346	rVV2	181	131	0.02%	0.003%
13	3.288	359	361	363	rBB2	232	179	0.03%	0.004%
14	3.325	363	367	368	rBV	169	200	0.03%	0.005%
15	3.373	373	375	376	rBV	180	134	0.02%	0.003%
16	3.428	382	384	387	rVB	238	144	0.02%	0.003%
17	3.581	406	409	411	rBB2	177	175	0.03%	0.004%
18	3.654	415	421	423	rBV	158	246	0.04%	0.006%
19	3.703	428	429	431	rBV	249	148	0.03%	0.004%
20	3.794	441	444	447	rBB	183	251	0.04%	0.006%
21	3.837	450	451	454	rBB	198	159	0.03%	0.004%
22	3.910	459	463	465	rBV	174	277	0.05%	0.007%
23	3.959	470	471	473	rBV	131	118	0.02%	0.003%
24	4.050	483	486	487	rBV	217	234	0.04%	0.006%
25	4.276	521	523	527	rBV2	245	369	0.06%	0.009%
26	4.355	533	536	537	rBV	293	210	0.04%	0.005%
27	4.471	546	555	569	rBV	40482	124419	21.45%	2.949%
28	4.891	622	624	625	rBV	219	124	0.02%	0.003%
29	4.946	631	633	635	rVB	305	223	0.04%	0.005%
30	5.056	639	651	667	rBV	77094	238170	41.06%	5.644%
31	5.318	692	694	695	rVV	213	114	0.02%	0.003%
32	5.385	701	705	706	rBV2	338	469	0.08%	0.011%
33	5.483	719	721	724	rBB	157	164	0.03%	0.004%
34	5.873	784	785	787	rBV	127	116	0.02%	0.003%
35	5.964	790	800	819	rBV2	196140	580120	100.00%	13.748%
36	6.330	858	860	863	rVB3	299	321	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042651.D
 Acq On : 27 Jul 2024 20:45
 Operator : JC/MD
 Sample : VX0728WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.440	876	878	881	rBV	171	185	0.03%	0.004%
38	6.537	892	894	896	rVB	235	199	0.03%	0.005%
39	6.592	899	903	905	rBV2	189	352	0.06%	0.008%
40	6.757	922	930	945	rBV	157532	378892	65.31%	8.979%
41	7.123	985	990	996	rVB5	1585	3843	0.66%	0.091%
42	7.190	999	1001	1002	rVB	381	178	0.03%	0.004%
43	7.220	1003	1006	1009	rBV3	419	627	0.11%	0.015%
44	7.306	1012	1020	1040	rBV	115941	262172	45.19%	6.213%
45	7.476	1045	1048	1050	rBV2	294	395	0.07%	0.009%
46	7.617	1069	1071	1072	rBV	201	169	0.03%	0.004%
47	7.915	1118	1120	1122	rBB	144	140	0.02%	0.003%
48	7.934	1122	1123	1125	rBV	245	201	0.03%	0.005%
49	8.196	1164	1166	1168	rBV2	220	125	0.02%	0.003%
50	8.275	1174	1179	1180	rBV2	210	322	0.06%	0.008%
51	8.330	1182	1188	1202	rVB	66642	116896	20.15%	2.770%
52	8.537	1220	1222	1224	rBV	427	321	0.06%	0.008%
53	8.592	1230	1231	1234	rBV2	205	210	0.04%	0.005%
54	8.647	1234	1240	1256	rVV	276752	444950	76.70%	10.545%
55	8.952	1285	1290	1302	rBV	49896	73743	12.71%	1.748%
56	9.135	1318	1320	1322	rVB	436	302	0.05%	0.007%
57	9.177	1325	1327	1328	rBV	200	133	0.02%	0.003%
58	9.214	1331	1333	1335	rBV	201	163	0.03%	0.004%
59	9.275	1341	1343	1350	rVB3	736	1036	0.18%	0.025%
60	9.385	1356	1361	1375	rBV	168978	262912	45.32%	6.231%
61	9.726	1416	1417	1418	rBV	209	116	0.02%	0.003%
62	10.006	1461	1463	1465	rBV	257	301	0.05%	0.007%
63	10.055	1465	1471	1487	rVV	312461	433280	74.69%	10.268%
64	10.275	1505	1507	1511	rVB	280	174	0.03%	0.004%
65	10.311	1511	1513	1517	rVB3	349	482	0.08%	0.011%
66	10.354	1517	1520	1523	rVB3	302	305	0.05%	0.007%
67	10.378	1523	1524	1526	rBB3	218	120	0.02%	0.003%
68	10.409	1528	1529	1531	rBV	180	187	0.03%	0.004%
69	10.512	1543	1546	1547	rBV	285	292	0.05%	0.007%
70	10.671	1571	1572	1574	rBV	215	153	0.03%	0.004%
71	10.811	1588	1595	1596	rBV	308	472	0.08%	0.011%
72	11.098	1639	1642	1643	rBV	163	121	0.02%	0.003%
73	11.189	1652	1657	1666	rBV	212339	286692	49.42%	6.794%
74	11.384	1686	1689	1690	rBB	251	178	0.03%	0.004%
75	11.457	1696	1701	1703	rBV2	357	483	0.08%	0.011%
76	11.634	1728	1730	1731	rBV	230	169	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042651.D
 Acq On : 27 Jul 2024 20:45
 Operator : JC/MD
 Sample : VX0728WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1803	rBV	260690	342283	59.00%	8.112%
78	12.189	1819	1821	1823	rBV2	238	161	0.03%	0.004%
79	12.238	1828	1829	1831	rBV	217	152	0.03%	0.004%
80	12.274	1834	1835	1837	rBV	206	122	0.02%	0.003%
81	12.317	1837	1842	1855	rVV	264370	349606	60.26%	8.285%
82	12.482	1866	1869	1871	rVB	224	219	0.04%	0.005%
83	12.536	1877	1878	1880	rBV	130	131	0.02%	0.003%
84	12.719	1906	1908	1909	rBV	264	168	0.03%	0.004%
85	12.756	1913	1914	1916	rVB	224	115	0.02%	0.003%
86	12.823	1924	1925	1929	rVB	269	169	0.03%	0.004%
87	13.030	1957	1959	1962	rVB	273	203	0.03%	0.005%
88	13.244	1992	1994	1996	rBV	278	305	0.05%	0.007%
89	13.347	2009	2011	2014	rBV2	149	198	0.03%	0.005%
90	13.597	2051	2052	2053	rVB2	461	168	0.03%	0.004%
91	13.847	2091	2093	2095	rBV	205	192	0.03%	0.005%
92	13.932	2106	2107	2109	rBV	313	206	0.04%	0.005%
93	14.073	2128	2130	2131	rVB	257	145	0.02%	0.003%
94	14.109	2131	2136	2137	rBV2	139	223	0.04%	0.005%
95	14.207	2150	2152	2153	rBV2	276	218	0.04%	0.005%
96	14.304	2163	2168	2171	rBV2	259	452	0.08%	0.011%
97	15.012	2283	2284	2288	rBV2	214	244	0.04%	0.006%
98	15.249	2322	2323	2324	rBV	298	158	0.03%	0.004%
99	15.700	2395	2397	2398	rBV	535	318	0.05%	0.008%
100	16.780	2572	2574	2575	rBV	311	193	0.03%	0.005%




Sum of corrected areas: 4219611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042651.D
Acq On : 27 Jul 2024 20:45
Operator : JC/MD
Sample : VX0728WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK704

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

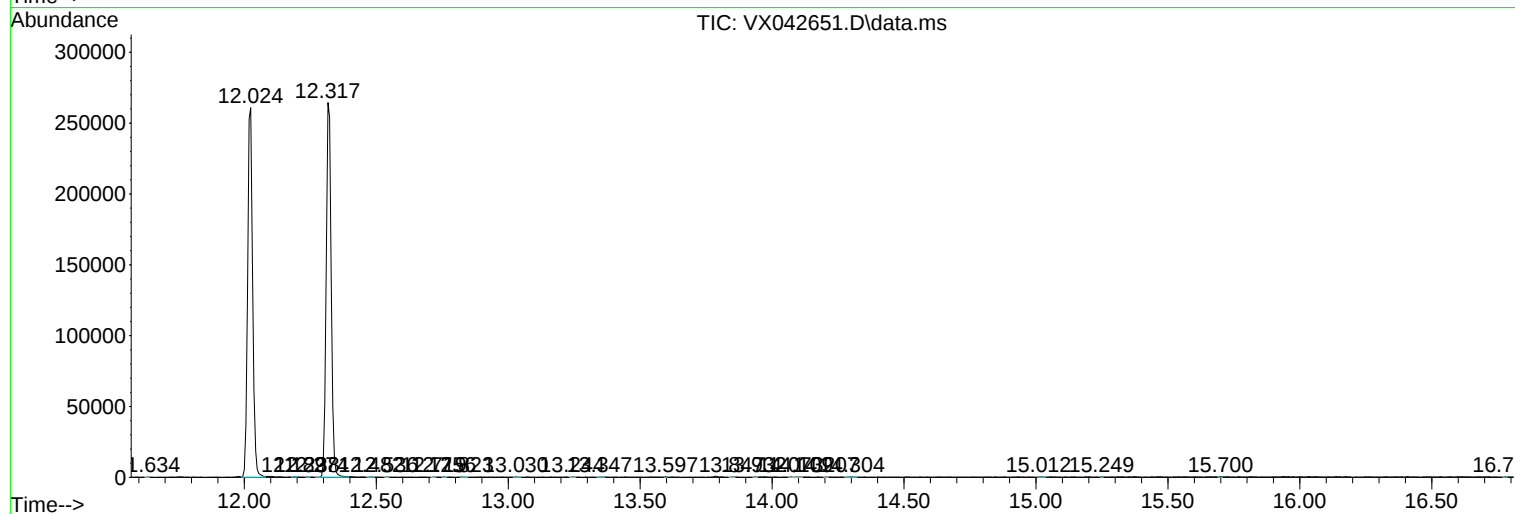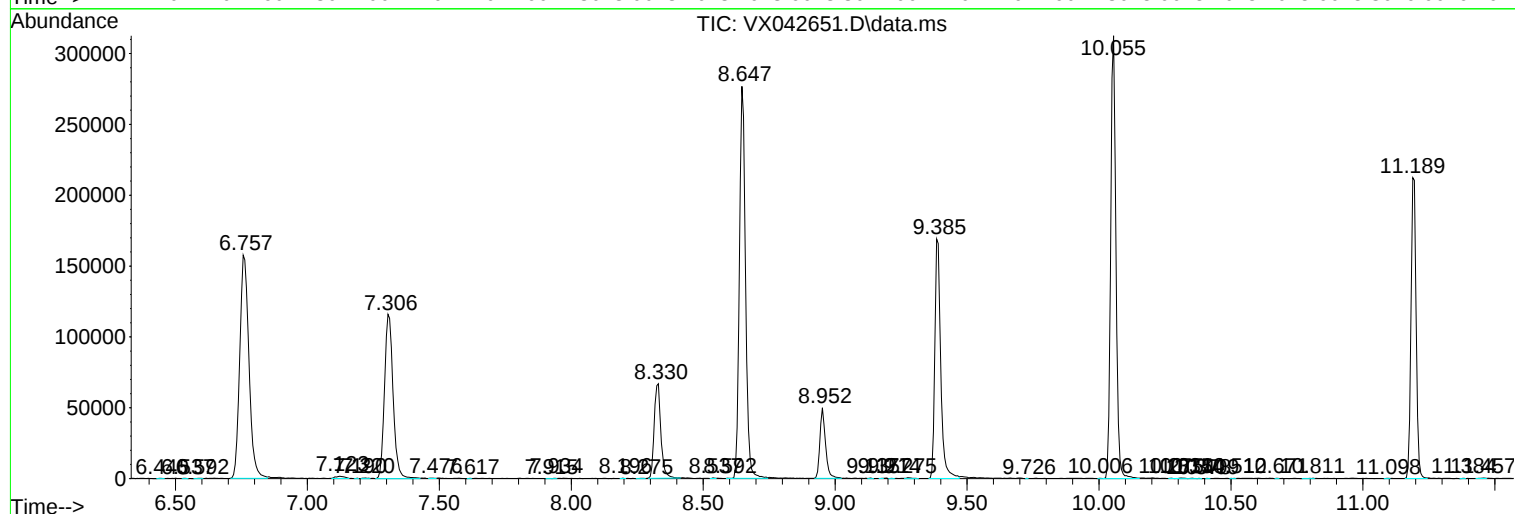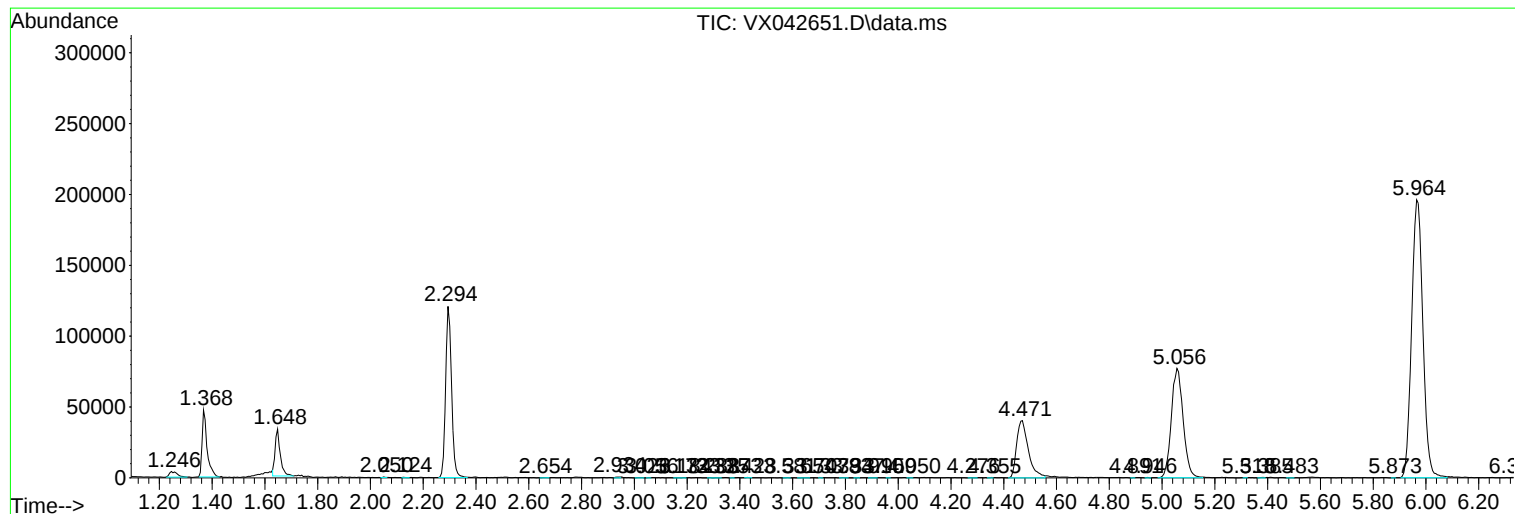

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042651.D
Acq On : 27 Jul 2024 20:45
Operator : JC/MD
Sample : VX0728WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK704

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042651.D
Acq On : 27 Jul 2024 20:45
Operator : JC/MD
Sample : VX0728WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK704

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
