

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042656.D
 Acq On : 27 Jul 2024 22:41
 Operator : JC/MD
 Sample : P3388-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	23	29	33	rVB3	3323	5829	1.03%	0.138%
2	1.343	40	42	43	rBV	444	350	0.06%	0.008%
3	1.368	43	46	58	rVV	48331	60729	10.73%	1.439%
4	1.575	72	80	81	rBV2	2538	4195	0.74%	0.099%
5	1.648	89	92	101	rVB	30148	40482	7.15%	0.960%
6	2.118	168	169	171	rBV	302	221	0.04%	0.005%
7	2.160	171	176	179	rBV2	373	646	0.11%	0.015%
8	2.294	192	198	212	rBV	111010	181503	32.07%	4.302%
9	2.496	228	231	233	rBV	420	344	0.06%	0.008%
10	2.739	267	271	275	rVB2	181	312	0.06%	0.007%
11	2.782	275	278	283	rBV3	601	900	0.16%	0.021%
12	2.934	300	303	304	rBV	564	520	0.09%	0.012%
13	3.136	332	336	339	rBV	169	241	0.04%	0.006%
14	3.343	367	370	372	rBB	229	232	0.04%	0.005%
15	3.550	402	404	408	rVB2	261	244	0.04%	0.006%
16	4.099	490	494	495	rVV	221	214	0.04%	0.005%
17	4.257	518	520	523	rVB	259	245	0.04%	0.006%
18	4.337	531	533	537	rVB	313	338	0.06%	0.008%
19	4.379	537	540	542	rBB	251	290	0.05%	0.007%
20	4.404	542	544	546	rBV	257	297	0.05%	0.007%
21	4.465	546	554	571	rBV	40521	121896	21.54%	2.889%
22	4.769	602	604	605	rBV	285	237	0.04%	0.006%
23	4.873	619	621	626	rVV2	165	236	0.04%	0.006%
24	5.056	639	651	670	rBV	81078	236653	41.81%	5.609%
25	5.215	675	677	679	rVV	350	294	0.05%	0.007%
26	5.257	682	684	687	rVB	236	225	0.04%	0.005%
27	5.294	687	690	692	rVB2	241	245	0.04%	0.006%
28	5.330	692	696	697	rBV	307	323	0.06%	0.008%
29	5.562	732	734	735	rBV2	256	227	0.04%	0.005%
30	5.964	789	800	816	rBV2	194112	565984	100.00%	13.416%
31	6.391	868	870	873	rBV	218	217	0.04%	0.005%
32	6.544	890	895	896	rBV2	198	289	0.05%	0.007%
33	6.635	907	910	913	rBV2	257	368	0.07%	0.009%
34	6.757	921	930	945	rBV	161087	393642	69.55%	9.331%
35	6.940	959	960	961	rBV	398	230	0.04%	0.005%
36	7.123	982	990	991	rBV3	2940	4771	0.84%	0.113%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042656.D
 Acq On : 27 Jul 2024 22:41
 Operator : JC/MD
 Sample : P3388-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.208	1002	1004	1007	rBV2	299	361	0.06%	0.009%
38	7.306	1012	1020	1036	rVV	114825	257339	45.47%	6.100%
39	7.440	1040	1042	1043	rVB	435	242	0.04%	0.006%
40	7.507	1049	1053	1058	rVB3	327	562	0.10%	0.013%
41	7.885	1112	1115	1117	rBV3	246	292	0.05%	0.007%
42	7.915	1119	1120	1125	rBV	171	223	0.04%	0.005%
43	8.123	1152	1154	1156	rBV	231	221	0.04%	0.005%
44	8.324	1181	1187	1201	rBV	69077	115665	20.44%	2.742%
45	8.647	1234	1240	1252	rBV	282750	438366	77.45%	10.391%
46	8.818	1266	1268	1270	rVB2	373	271	0.05%	0.006%
47	8.897	1279	1281	1283	rVB	441	364	0.06%	0.009%
48	8.952	1285	1290	1303	rVV	47777	73066	12.91%	1.732%
49	9.092	1312	1313	1316	rVB	291	238	0.04%	0.006%
50	9.147	1320	1322	1325	rVB	251	311	0.05%	0.007%
51	9.171	1325	1326	1329	rBV	258	282	0.05%	0.007%
52	9.385	1356	1361	1373	rBV	168146	257363	45.47%	6.100%
53	9.915	1445	1448	1451	rBB	237	314	0.06%	0.007%
54	9.939	1451	1452	1455	rBV	209	238	0.04%	0.006%
55	10.055	1465	1471	1483	rBV	328692	450537	79.60%	10.679%
56	10.201	1492	1495	1496	rBV	275	278	0.05%	0.007%
57	10.256	1502	1504	1507	rVB	340	380	0.07%	0.009%
58	10.293	1508	1510	1514	rBV2	281	479	0.08%	0.011%
59	10.354	1514	1520	1521	rVV2	395	541	0.10%	0.013%
60	10.573	1553	1556	1558	rBV2	201	243	0.04%	0.006%
61	10.689	1571	1575	1576	rBV2	227	298	0.05%	0.007%
62	10.726	1580	1581	1590	rVV2	253	583	0.10%	0.014%
63	10.799	1590	1593	1596	rVV2	142	215	0.04%	0.005%
64	10.860	1601	1603	1608	rVV2	263	322	0.06%	0.008%
65	11.189	1652	1657	1667	rBV	216870	277017	48.94%	6.566%
66	11.500	1706	1708	1711	rVB2	189	212	0.04%	0.005%
67	11.774	1750	1753	1756	rBV	297	347	0.06%	0.008%
68	11.811	1756	1759	1762	rBV2	215	266	0.05%	0.006%
69	12.024	1788	1794	1803	rBV	278173	358937	63.42%	8.508%
70	12.317	1837	1842	1850	rBV	269481	348007	61.49%	8.249%
71	12.768	1912	1916	1917	rBV	208	263	0.05%	0.006%
72	12.835	1924	1927	1929	rBV	353	376	0.07%	0.009%
73	12.920	1939	1941	1945	rVB2	210	249	0.04%	0.006%
74	13.055	1959	1963	1964	rBV2	203	233	0.04%	0.006%
75	13.286	1998	2001	2002	rBV2	236	288	0.05%	0.007%
76	13.372	2013	2015	2017	rBV2	185	221	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042656.D
 Acq On : 27 Jul 2024 22:41
 Operator : JC/MD
 Sample : P3388-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	13.634	2057	2058	2061	rBV	206	241	0.04%	0.006%
78	13.731	2072	2074	2075	rBV	247	215	0.04%	0.005%
79	13.823	2087	2089	2093	rVB2	250	300	0.05%	0.007%
80	13.908	2102	2103	2107	rVB	252	274	0.05%	0.006%
81	13.957	2107	2111	2115	rBB2	251	506	0.09%	0.012%
82	14.158	2142	2144	2151	rBV2	203	427	0.08%	0.010%
83	14.262	2160	2161	2163	rBV	315	253	0.04%	0.006%
84	14.286	2163	2165	2167	rVV	283	247	0.04%	0.006%
85	14.573	2210	2212	2216	rBV	229	325	0.06%	0.008%
86	14.719	2234	2236	2239	rVB3	231	266	0.05%	0.006%
87	14.835	2253	2255	2257	rBV2	234	292	0.05%	0.007%
88	15.085	2295	2296	2299	rBV	297	269	0.05%	0.006%
89	15.140	2302	2305	2306	rBV	307	336	0.06%	0.008%
90	15.237	2317	2321	2322	rBV2	456	455	0.08%	0.011%
91	15.390	2344	2346	2351	rVB	640	689	0.12%	0.016%
92	15.451	2353	2356	2359	rBV2	408	473	0.08%	0.011%
93	15.676	2389	2393	2395	rBV3	297	399	0.07%	0.009%
94	15.810	2414	2415	2419	rBV3	243	215	0.04%	0.005%
95	15.926	2432	2434	2438	rBV2	591	807	0.14%	0.019%
96	16.030	2449	2451	2454	rBV2	357	504	0.09%	0.012%
97	16.127	2466	2467	2471	rVB2	260	224	0.04%	0.005%
98	16.170	2471	2474	2476	rBV3	376	549	0.10%	0.013%
99	16.578	2539	2541	2543	rBV	258	246	0.04%	0.006%
100	16.676	2555	2557	2560	rBV4	256	318	0.06%	0.008%


Sum of corrected areas: 4218809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042656.D
Acq On : 27 Jul 2024 22:41
Operator : JC/MD
Sample : P3388-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

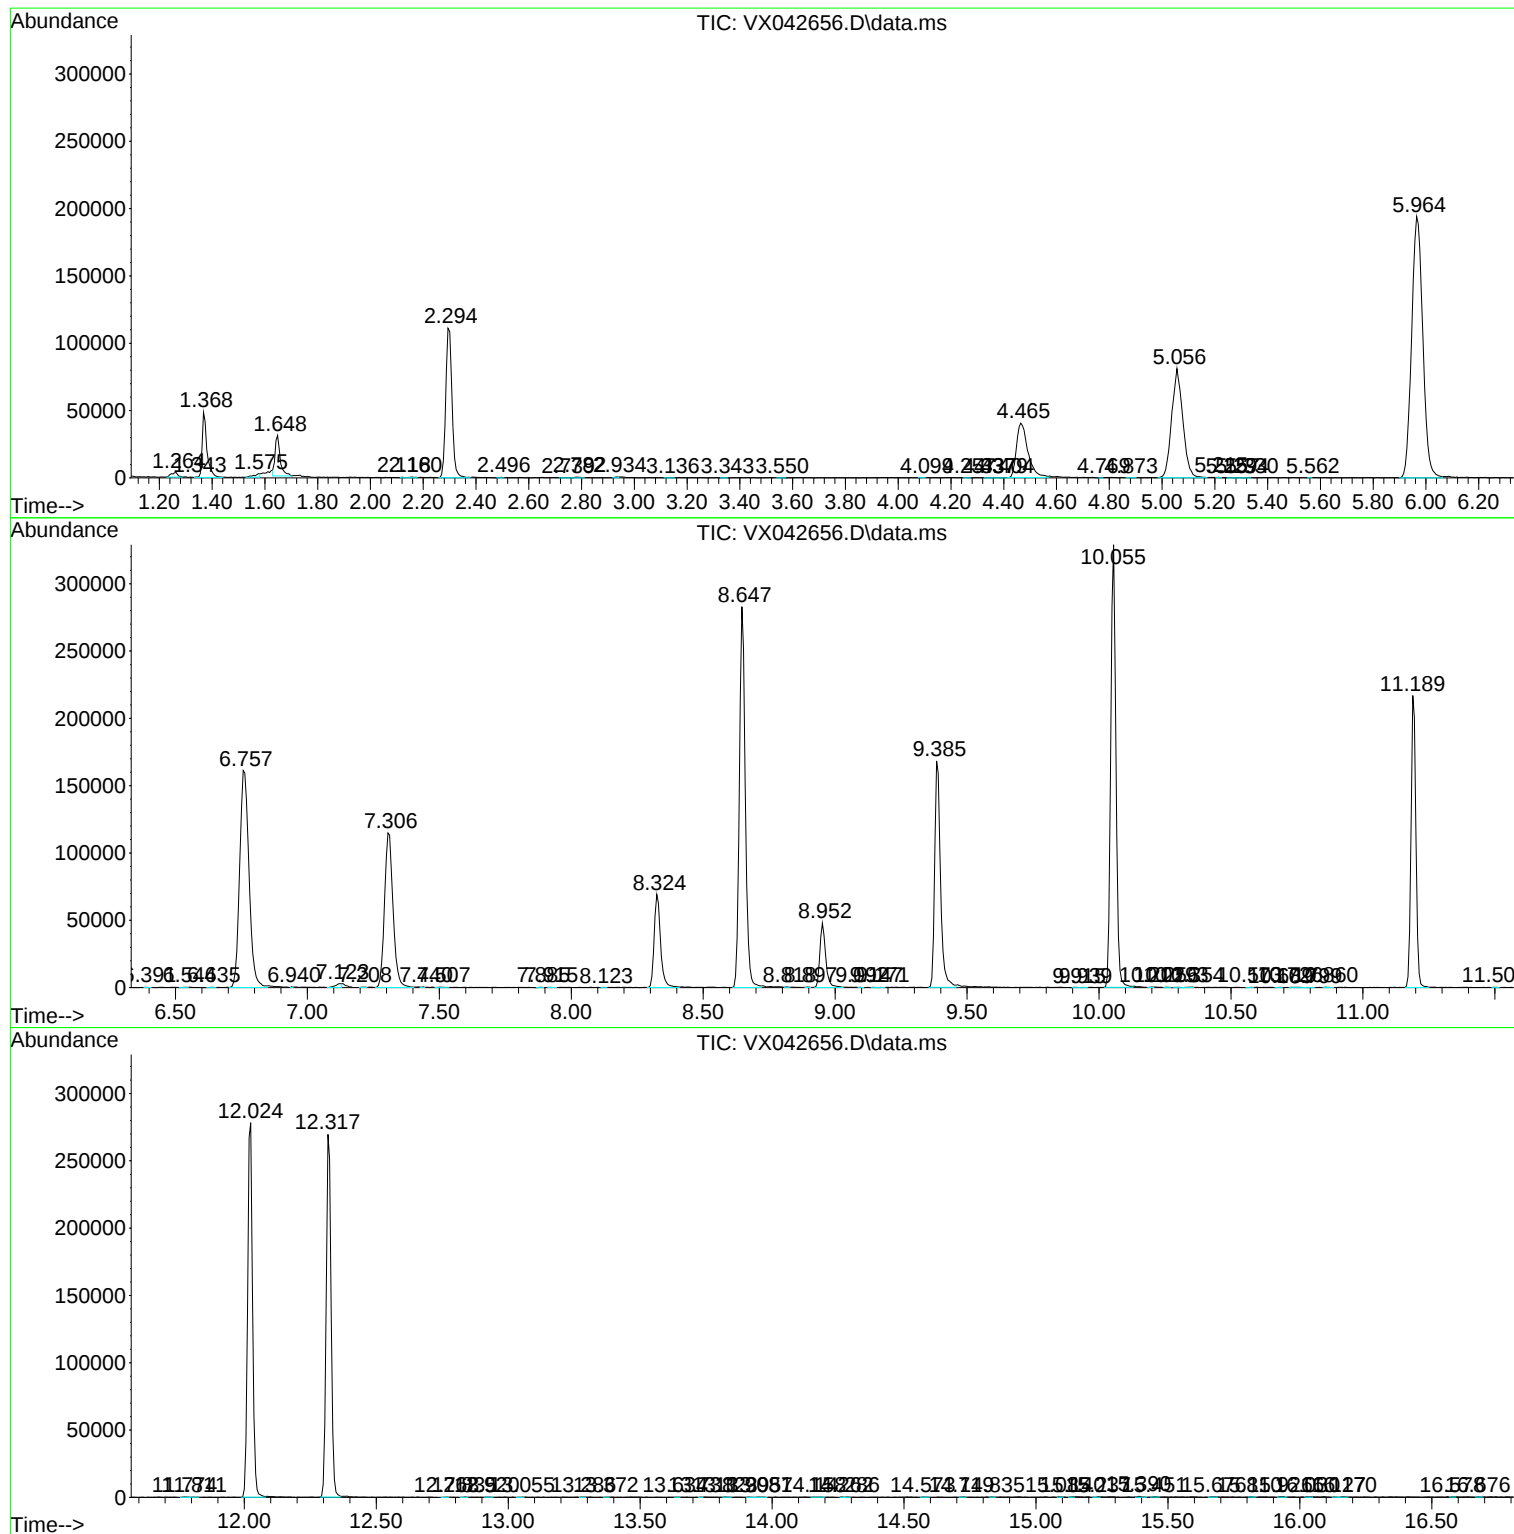

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042656.D
Acq On : 27 Jul 2024 22:41
Operator : JC/MD
Sample : P3388-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042656.D
Acq On : 27 Jul 2024 22:41
Operator : JC/MD
Sample : P3388-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc