

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042657.D
 Acq On : 27 Jul 2024 23:04
 Operator : JC/MD
 Sample : P3388-07 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	32	rBV3	3628	6255	1.08%	0.143%
2	1.368	43	46	56	rVB	48663	61115	10.55%	1.397%
3	1.648	71	92	102	rBV	34440	64544	11.14%	1.475%
4	2.002	149	150	152	rBV	309	218	0.04%	0.005%
5	2.026	152	154	156	rVB	356	274	0.05%	0.006%
6	2.130	168	171	174	rBV	205	372	0.06%	0.009%
7	2.172	176	178	180	rVB	391	341	0.06%	0.008%
8	2.197	180	182	185	rBV	251	218	0.04%	0.005%
9	2.227	185	187	190	rBV	321	366	0.06%	0.008%
10	2.294	192	198	209	rVB	116713	182125	31.44%	4.162%
11	2.508	231	233	236	rVB2	252	261	0.05%	0.006%
12	2.581	242	245	249	rVB	326	436	0.08%	0.010%
13	2.788	276	279	281	rBV	574	637	0.11%	0.015%
14	2.886	291	295	298	rBV	231	312	0.05%	0.007%
15	2.941	298	304	311	rVB2	1411	2473	0.43%	0.057%
16	3.087	326	328	330	rBV2	332	259	0.04%	0.006%
17	3.312	362	365	368	rVB2	252	353	0.06%	0.008%
18	3.538	399	402	404	rBV	215	288	0.05%	0.007%
19	3.575	404	408	409	rVB	253	265	0.05%	0.006%
20	3.642	417	419	425	rBB	260	395	0.07%	0.009%
21	3.770	438	440	445	rBB	136	245	0.04%	0.006%
22	3.819	445	448	451	rBB	202	232	0.04%	0.005%
23	3.867	452	456	457	rBV	284	224	0.04%	0.005%
24	4.465	546	554	569	rBV	43806	136920	23.63%	3.129%
25	4.727	595	597	599	rVB	385	332	0.06%	0.008%
26	4.763	599	603	605	rBV	407	518	0.09%	0.012%
27	4.879	621	622	627	rVV2	156	260	0.04%	0.006%
28	5.056	639	651	668	rBV2	78481	235535	40.66%	5.382%
29	5.276	684	687	689	rBV2	216	229	0.04%	0.005%
30	5.361	694	701	703	rBV2	232	450	0.08%	0.010%
31	5.385	703	705	708	rBV2	305	353	0.06%	0.008%
32	5.465	714	718	720	rBV	293	386	0.07%	0.009%
33	5.605	738	741	743	rBV	289	365	0.06%	0.008%
34	5.660	746	750	753	rVB2	253	440	0.08%	0.010%
35	5.702	753	757	759	rBV	235	330	0.06%	0.008%
36	5.739	761	763	766	rBV	232	236	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042657.D
 Acq On : 27 Jul 2024 23:04
 Operator : JC/MD
 Sample : P3388-07 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.964	788	800	817	rBV2	196549	579318	100.00%	13.238%
38	6.221	841	842	846	rBV	196	267	0.05%	0.006%
39	6.361	862	865	867	rVV	280	252	0.04%	0.006%
40	6.385	867	869	871	rVV	361	248	0.04%	0.006%
41	6.568	897	899	902	rVB	240	237	0.04%	0.005%
42	6.757	922	930	947	rBV	166305	403228	69.60%	9.214%
43	6.940	957	960	961	rBV2	358	333	0.06%	0.008%
44	6.983	965	967	970	rVB	466	356	0.06%	0.008%
45	7.044	974	977	978	rBV	215	258	0.04%	0.006%
46	7.129	983	991	1002	rVV4	25352	57396	9.91%	1.312%
47	7.208	1002	1004	1007	rVB2	519	615	0.11%	0.014%
48	7.306	1012	1020	1038	rBV	115044	261478	45.14%	5.975%
49	7.476	1046	1048	1049	rBV	421	351	0.06%	0.008%
50	7.751	1091	1093	1096	rBV	264	240	0.04%	0.005%
51	8.013	1135	1136	1141	rVB	253	332	0.06%	0.008%
52	8.056	1141	1143	1146	rBV2	225	334	0.06%	0.008%
53	8.135	1155	1156	1159	rBV	214	227	0.04%	0.005%
54	8.324	1182	1187	1200	rVV	65909	113372	19.57%	2.591%
55	8.519	1215	1219	1220	rBV2	220	266	0.05%	0.006%
56	8.647	1234	1240	1251	rBV	281079	445091	76.83%	10.171%
57	8.952	1284	1290	1301	rVV	46762	74396	12.84%	1.700%
58	9.147	1318	1322	1324	rBV	354	490	0.08%	0.011%
59	9.226	1333	1335	1336	rVV	355	225	0.04%	0.005%
60	9.287	1340	1345	1348	rVV3	484	822	0.14%	0.019%
61	9.385	1356	1361	1375	rBV	176313	265422	45.82%	6.065%
62	10.055	1465	1471	1482	rBV	322949	459912	79.39%	10.510%
63	10.390	1524	1526	1531	rVB2	240	272	0.05%	0.006%
64	10.701	1575	1577	1581	rVB2	240	217	0.04%	0.005%
65	10.866	1602	1604	1607	rVB	299	284	0.05%	0.006%
66	11.189	1652	1657	1665	rBV	219270	285763	49.33%	6.530%
67	11.396	1688	1691	1693	rVB	311	299	0.05%	0.007%
68	11.421	1693	1695	1697	rBV2	245	291	0.05%	0.007%
69	11.543	1714	1715	1719	rVV	268	233	0.04%	0.005%
70	11.744	1744	1748	1750	rVB	262	296	0.05%	0.007%
71	11.768	1750	1752	1754	rBV2	258	292	0.05%	0.007%
72	11.787	1754	1755	1758	rVB	302	248	0.04%	0.006%
73	12.024	1788	1794	1803	rBV	279269	364416	62.90%	8.327%
74	12.122	1808	1810	1811	rBV	343	313	0.05%	0.007%
75	12.244	1827	1830	1833	rBV	305	267	0.05%	0.006%
76	12.317	1837	1842	1853	rBV	269706	351528	60.68%	8.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042657.D
 Acq On : 27 Jul 2024 23:04
 Operator : JC/MD
 Sample : P3388-07 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.445	1861	1863	1865	rBV	375	351	0.06%	0.008%
78	12.610	1886	1890	1893	rBV2	236	414	0.07%	0.009%
79	12.640	1893	1895	1897	rVB2	372	257	0.04%	0.006%
80	12.671	1897	1900	1903	rBV	208	330	0.06%	0.008%
81	12.768	1913	1916	1918	rBV2	291	295	0.05%	0.007%
82	12.914	1938	1940	1942	rVB	274	230	0.04%	0.005%
83	12.939	1942	1944	1946	rBV	269	272	0.05%	0.006%
84	13.049	1959	1962	1964	rBV2	167	253	0.04%	0.006%
85	13.311	2002	2005	2007	rBV	171	260	0.04%	0.006%
86	13.707	2066	2070	2071	rBV	237	281	0.05%	0.006%
87	14.189	2147	2149	2152	rVB2	234	254	0.04%	0.006%
88	14.237	2152	2157	2158	rBV2	225	289	0.05%	0.007%
89	14.603	2214	2217	2219	rBV	281	302	0.05%	0.007%
90	14.658	2222	2226	2229	rBV2	368	555	0.10%	0.013%
91	14.780	2244	2246	2249	rVB	275	220	0.04%	0.005%
92	14.835	2252	2255	2256	rBV	296	304	0.05%	0.007%
93	14.914	2266	2268	2271	rVB2	252	240	0.04%	0.005%
94	15.323	2331	2335	2337	rBV2	477	349	0.06%	0.008%
95	15.341	2337	2338	2341	rBV2	337	391	0.07%	0.009%
96	15.591	2377	2379	2381	rBV	256	240	0.04%	0.005%
97	15.865	2422	2424	2427	rBV	340	375	0.06%	0.009%
98	16.097	2459	2462	2465	rBV2	257	379	0.07%	0.009%
99	16.328	2498	2500	2501	rBV	324	259	0.04%	0.006%
100	16.487	2524	2526	2528	rBV	262	217	0.04%	0.005%




Sum of corrected areas: 4376064

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042657.D
Acq On : 27 Jul 2024 23:04
Operator : JC/MD
Sample : P3388-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

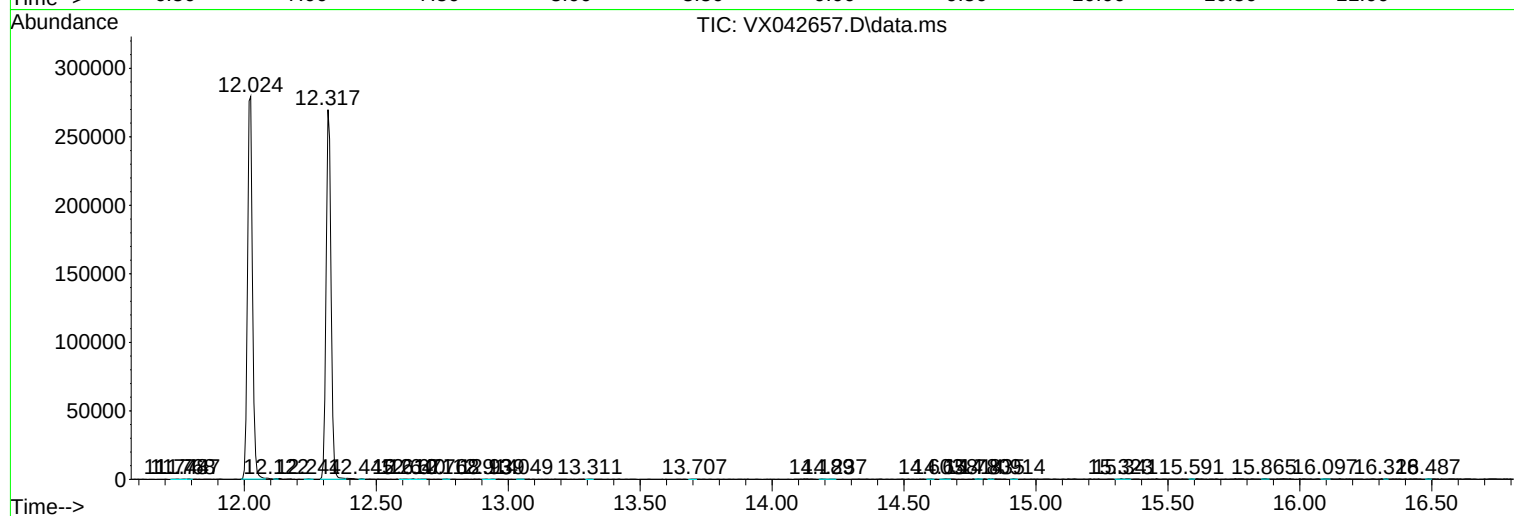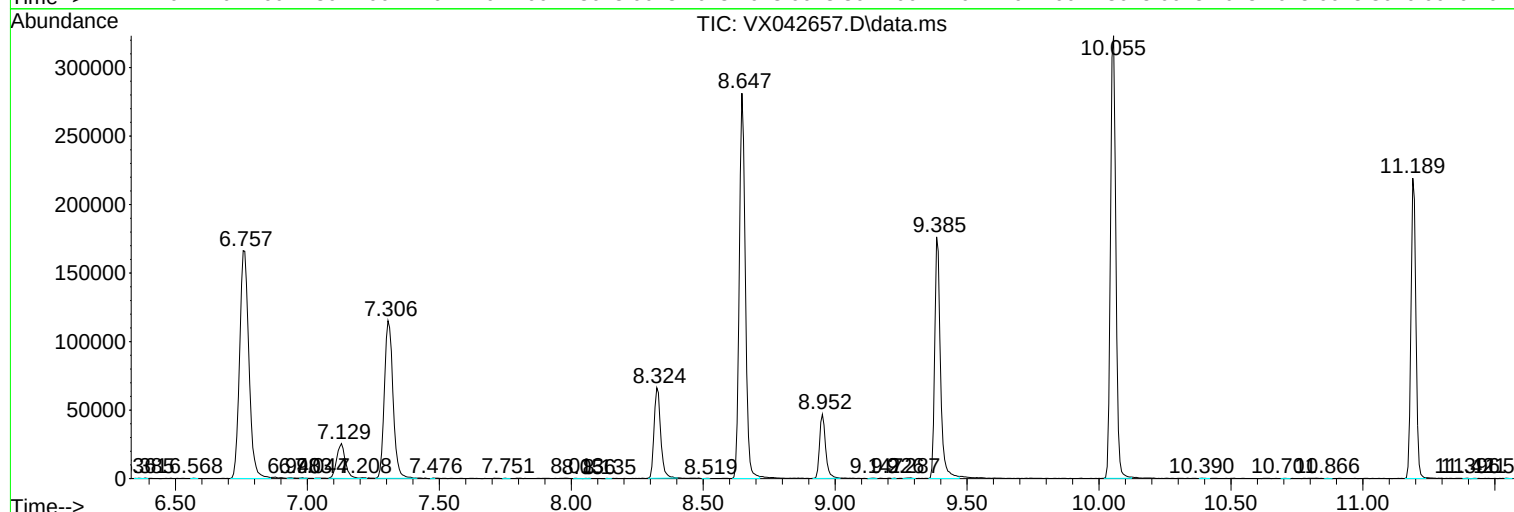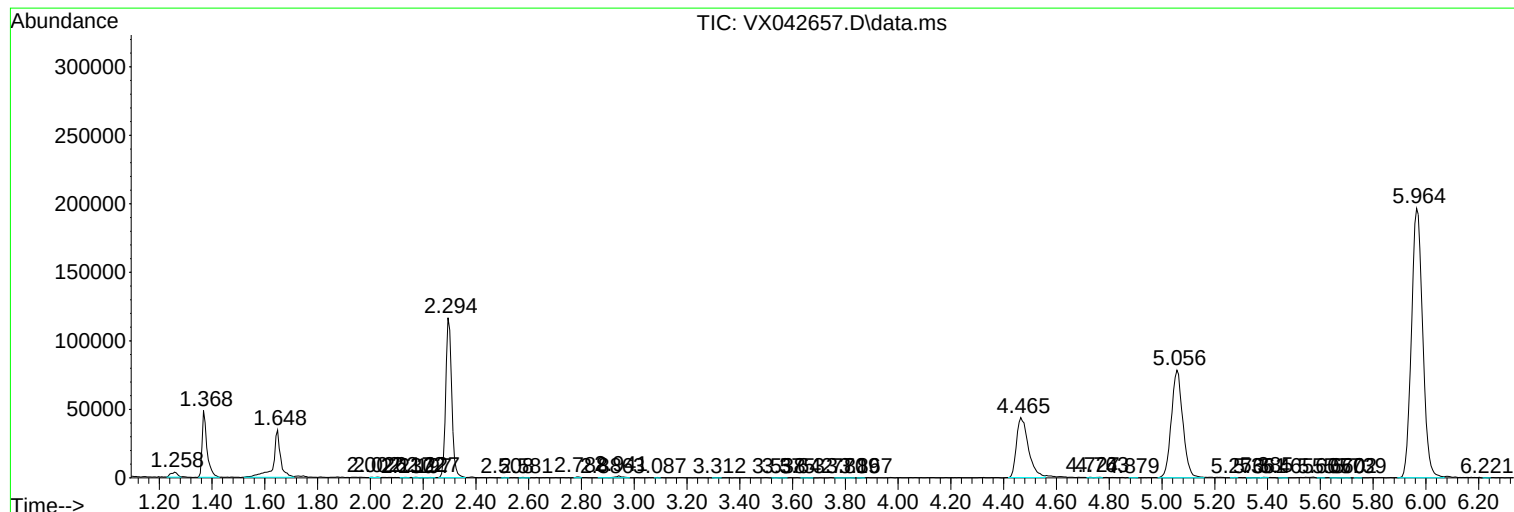

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042657.D
Acq On : 27 Jul 2024 23:04
Operator : JC/MD
Sample : P3388-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042657.D
Acq On : 27 Jul 2024 23:04
Operator : JC/MD
Sample : P3388-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc