

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042658.D
 Acq On : 27 Jul 2024 23:28
 Operator : JC/MD
 Sample : P3388-08 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	38	rVB2	3511	7253	1.25%	0.170%
2	1.368	42	46	58	rVB	49666	60924	10.50%	1.426%
3	1.520	69	71	72	rBV	389	206	0.04%	0.005%
4	1.648	88	92	100	rVB	32259	42299	7.29%	0.990%
5	1.831	120	122	126	rBV2	522	456	0.08%	0.011%
6	2.044	155	157	159	rVB	281	215	0.04%	0.005%
7	2.154	174	175	179	rBV	307	418	0.07%	0.010%
8	2.294	192	198	210	rVB	115899	182976	31.54%	4.282%
9	2.447	218	223	224	rBV	364	431	0.07%	0.010%
10	2.508	230	233	237	rVB2	326	424	0.07%	0.010%
11	2.569	242	243	248	rVV	347	364	0.06%	0.009%
12	2.788	275	279	285	rVB3	550	934	0.16%	0.022%
13	2.940	297	304	306	rBV3	695	1348	0.23%	0.032%
14	3.288	360	361	363	rBV3	213	207	0.04%	0.005%
15	3.392	375	378	381	rBB	207	209	0.04%	0.005%
16	3.422	381	383	386	rBB	219	221	0.04%	0.005%
17	3.459	387	389	393	rBB	189	240	0.04%	0.006%
18	4.001	474	478	479	rBV	251	303	0.05%	0.007%
19	4.074	486	490	493	rVB	202	255	0.04%	0.006%
20	4.148	498	502	503	rBV2	249	284	0.05%	0.007%
21	4.312	526	529	531	rBV2	220	255	0.04%	0.006%
22	4.465	545	554	573	rVV	41547	125231	21.59%	2.931%
23	4.910	624	627	630	rVB	236	243	0.04%	0.006%
24	4.958	630	635	636	rBV2	174	286	0.05%	0.007%
25	5.056	640	651	667	rBV	77697	237659	40.97%	5.562%
26	5.257	682	684	688	rVB	338	321	0.06%	0.008%
27	5.361	698	701	704	rBV2	214	282	0.05%	0.007%
28	5.397	704	707	708	rBV2	336	272	0.05%	0.006%
29	5.611	739	742	744	rBV2	219	271	0.05%	0.006%
30	5.690	751	755	760	rVB2	302	556	0.10%	0.013%
31	5.757	763	766	771	rVB2	169	308	0.05%	0.007%
32	5.806	773	774	778	rVB	225	227	0.04%	0.005%
33	5.849	778	781	785	rBB	235	305	0.05%	0.007%
34	5.964	789	800	820	rBV2	193859	580140	100.00%	13.577%
35	6.202	836	839	840	rBV2	188	221	0.04%	0.005%
36	6.275	847	851	853	rVB2	248	352	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042658.D
 Acq On : 27 Jul 2024 23:28
 Operator : JC/MD
 Sample : P3388-08 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.300	853	855	858	rBV	298	490	0.08%	0.011%
38	6.361	863	865	868	rVV2	238	293	0.05%	0.007%
39	6.757	921	930	948	rBV	160216	399290	68.83%	9.345%
40	7.110	984	988	997	rVB5	1866	4895	0.84%	0.115%
41	7.306	1009	1020	1037	rBV	119835	263376	45.40%	6.164%
42	7.415	1037	1038	1040	rVV	546	433	0.07%	0.010%
43	7.458	1043	1045	1046	rVV	352	245	0.04%	0.006%
44	7.507	1049	1053	1054	rVV2	335	369	0.06%	0.009%
45	7.525	1054	1056	1059	rVB2	301	236	0.04%	0.006%
46	7.562	1061	1062	1064	rBV2	288	217	0.04%	0.005%
47	7.720	1085	1088	1091	rBV2	174	225	0.04%	0.005%
48	7.781	1095	1098	1102	rBV	262	368	0.06%	0.009%
49	7.909	1115	1119	1121	rBV2	276	406	0.07%	0.010%
50	8.104	1148	1151	1154	rVB	175	237	0.04%	0.006%
51	8.147	1154	1158	1160	rBB2	216	258	0.04%	0.006%
52	8.183	1160	1164	1168	rBV2	167	332	0.06%	0.008%
53	8.324	1181	1187	1197	rBV	66880	113544	19.57%	2.657%
54	8.433	1203	1205	1210	rBV2	236	406	0.07%	0.010%
55	8.647	1234	1240	1256	rBV	284086	444964	76.70%	10.414%
56	8.952	1285	1290	1301	rVV	48393	73734	12.71%	1.726%
57	9.244	1335	1338	1340	rBV	175	235	0.04%	0.005%
58	9.281	1340	1344	1345	rBV2	364	411	0.07%	0.010%
59	9.348	1353	1355	1356	rBV	273	276	0.05%	0.006%
60	9.384	1356	1361	1380	rVV	172570	267653	46.14%	6.264%
61	9.543	1386	1387	1388	rBV	500	223	0.04%	0.005%
62	9.982	1455	1459	1462	rBV2	201	375	0.06%	0.009%
63	10.055	1465	1471	1482	rBV	330507	453473	78.17%	10.613%
64	10.604	1558	1561	1563	rBV	214	233	0.04%	0.005%
65	10.659	1567	1570	1571	rBV	379	277	0.05%	0.006%
66	11.049	1632	1634	1637	rVV2	207	216	0.04%	0.005%
67	11.104	1641	1643	1645	rBV2	201	237	0.04%	0.006%
68	11.189	1652	1657	1668	rBV	220958	284105	48.97%	6.649%
69	11.262	1668	1669	1671	rVB2	395	285	0.05%	0.007%
70	11.537	1712	1714	1718	rBV2	223	314	0.05%	0.007%
71	11.610	1723	1726	1727	rBV	221	262	0.05%	0.006%
72	11.793	1754	1756	1759	rVB2	223	225	0.04%	0.005%
73	12.018	1788	1793	1802	rBV	276393	358523	61.80%	8.391%
74	12.317	1837	1842	1849	rBV	266016	346642	59.75%	8.113%
75	12.756	1912	1914	1919	rBV2	395	499	0.09%	0.012%
76	12.890	1934	1936	1939	rVB	213	214	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042658.D
 Acq On : 27 Jul 2024 23:28
 Operator : JC/MD
 Sample : P3388-08 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	13.006	1954	1955	1959	rBV2	210	234	0.04%	0.005%
78	13.109	1969	1972	1973	rVV	180	224	0.04%	0.005%
79	13.225	1988	1991	1995	rVB	449	469	0.08%	0.011%
80	13.268	1995	1998	2000	rBV	232	266	0.05%	0.006%
81	13.292	2000	2002	2005	rVV2	179	241	0.04%	0.006%
82	13.500	2033	2036	2038	rBV	264	295	0.05%	0.007%
83	13.756	2074	2078	2082	rBV2	150	250	0.04%	0.006%
84	14.067	2127	2129	2131	rBV	205	235	0.04%	0.005%
85	14.359	2173	2177	2179	rVV2	196	207	0.04%	0.005%
86	14.469	2192	2195	2197	rVB2	385	264	0.05%	0.006%
87	14.627	2219	2221	2222	rBV	296	219	0.04%	0.005%
88	14.902	2264	2266	2269	rBV2	200	236	0.04%	0.006%
89	15.164	2306	2309	2311	rBV3	280	334	0.06%	0.008%
90	15.329	2334	2336	2337	rBV	296	259	0.04%	0.006%
91	15.420	2348	2351	2352	rVV2	265	214	0.04%	0.005%
92	15.469	2355	2359	2361	rBV2	478	577	0.10%	0.014%
93	15.633	2384	2386	2387	rBV2	365	297	0.05%	0.007%
94	15.871	2422	2425	2426	rBV2	312	287	0.05%	0.007%
95	15.938	2432	2436	2437	rBV	296	290	0.05%	0.007%
96	15.993	2442	2445	2446	rBV3	390	281	0.05%	0.007%
97	16.139	2468	2469	2472	rBV2	373	362	0.06%	0.008%
98	16.365	2505	2506	2508	rBV	364	310	0.05%	0.007%
99	16.676	2554	2557	2558	rBV	406	310	0.05%	0.007%
100	16.773	2571	2573	2575	rBV2	304	281	0.05%	0.007%




Sum of corrected areas: 4272834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042658.D
Acq On : 27 Jul 2024 23:28
Operator : JC/MD
Sample : P3388-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

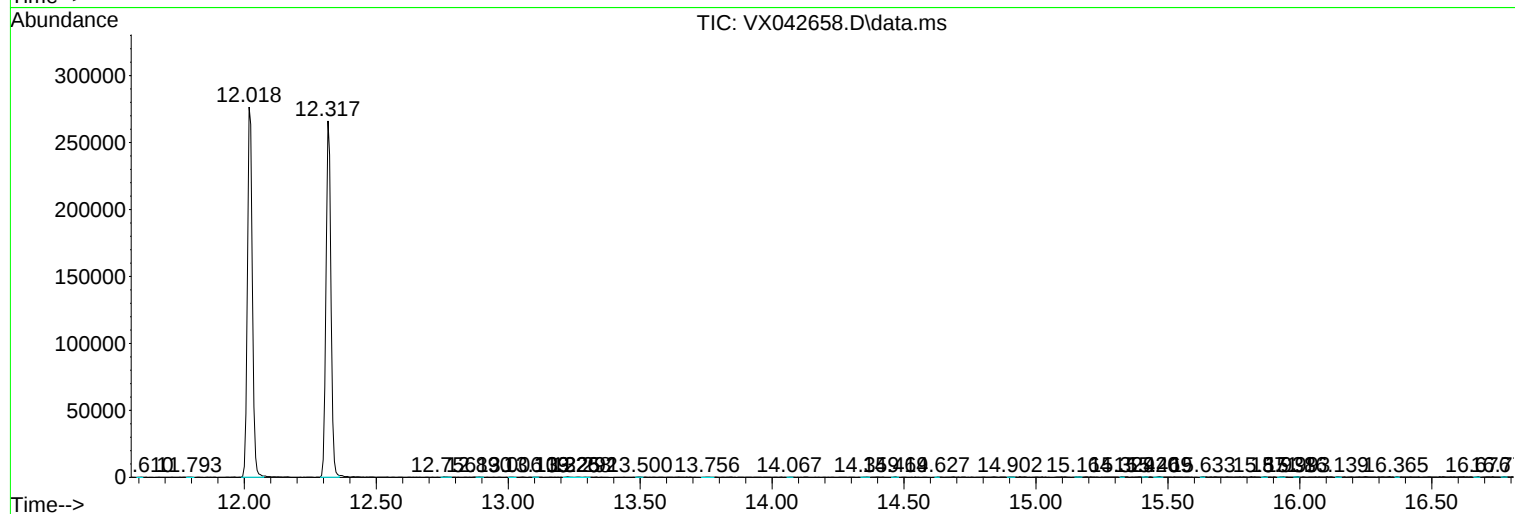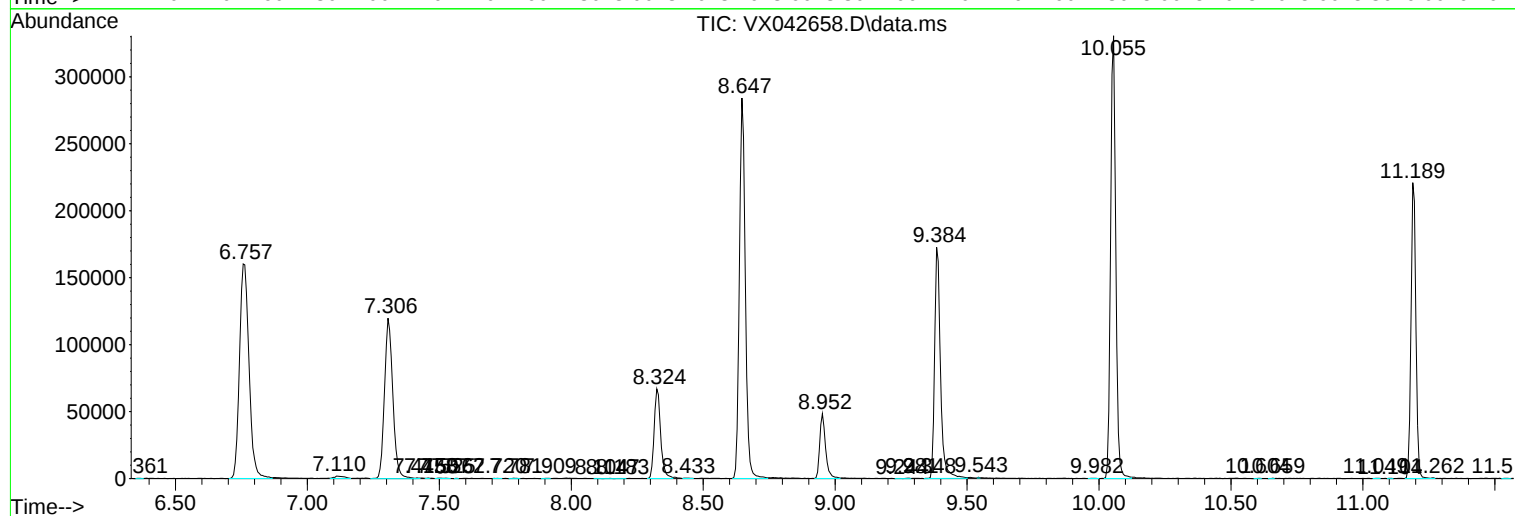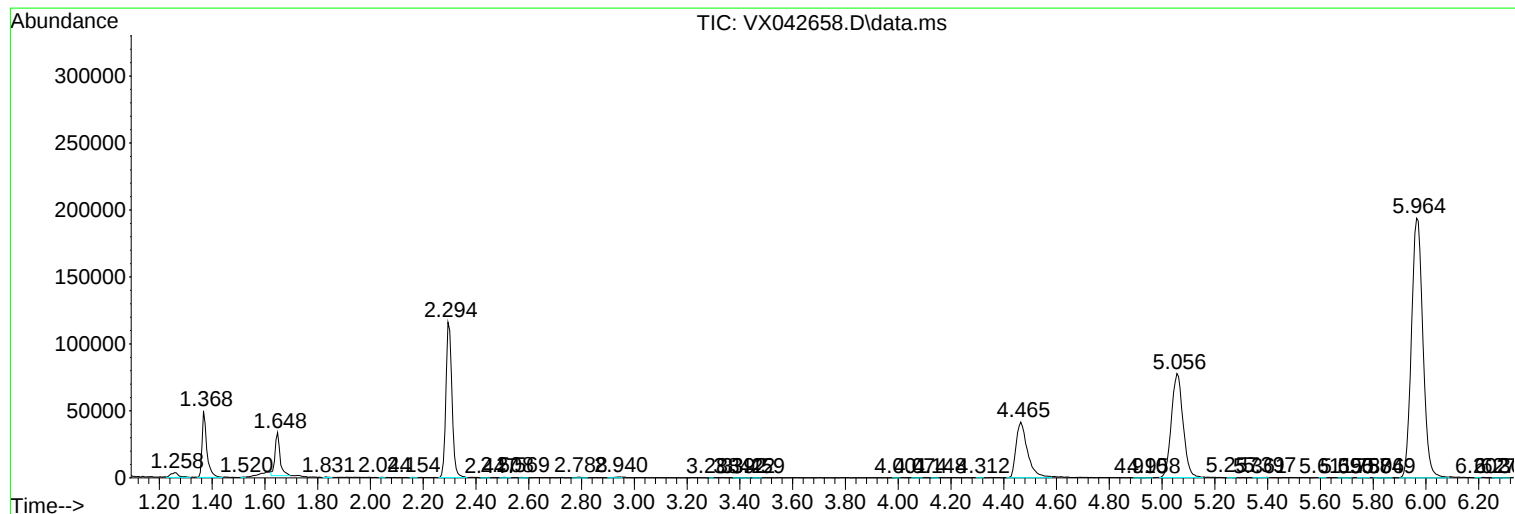

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042658.D
Acq On : 27 Jul 2024 23:28
Operator : JC/MD
Sample : P3388-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042658.D
Acq On : 27 Jul 2024 23:28
Operator : JC/MD
Sample : P3388-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc