

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042660.D
 Acq On : 28 Jul 2024 00:14
 Operator : JC/MD
 Sample : P3388-10 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	43616	59816	10.94%	1.452%
2	1.648	89	92	102	rVB	30309	39611	7.24%	0.962%
3	2.294	192	198	209	rBV	112961	174600	31.92%	4.239%
4	2.434	220	221	223	rVB	283	143	0.03%	0.003%
5	2.782	276	278	283	rVB3	568	670	0.12%	0.016%
6	3.050	320	322	323	rBV	177	74	0.01%	0.002%
7	3.129	333	335	338	rBV2	208	219	0.04%	0.005%
8	3.270	355	358	359	rBB2	218	206	0.04%	0.005%
9	3.288	359	361	362	rBV	257	202	0.04%	0.005%
10	3.355	370	372	375	rVB	264	218	0.04%	0.005%
11	3.392	375	378	382	rBB2	224	361	0.07%	0.009%
12	3.434	382	385	387	rBV	221	256	0.05%	0.006%
13	3.514	397	398	399	rBV	241	119	0.02%	0.003%
14	3.556	403	405	407	rBV	184	177	0.03%	0.004%
15	3.617	414	415	417	rBV	247	165	0.03%	0.004%
16	3.696	426	428	430	rBV	133	112	0.02%	0.003%
17	3.831	448	450	453	rBV2	151	154	0.03%	0.004%
18	3.922	462	465	466	rBV2	173	139	0.03%	0.003%
19	3.977	471	474	475	rVV2	227	224	0.04%	0.005%
20	4.013	478	480	482	rBV2	246	235	0.04%	0.006%
21	4.160	503	504	505	rBV2	265	165	0.03%	0.004%
22	4.221	512	514	515	rBV	244	147	0.03%	0.004%
23	4.282	521	524	526	rBV2	300	280	0.05%	0.007%
24	4.465	547	554	574	rBV2	38994	118631	21.69%	2.880%
25	4.782	603	606	607	rBV	303	250	0.05%	0.006%
26	4.879	621	622	623	rBV	173	77	0.01%	0.002%
27	5.062	641	652	666	rBV	72780	222134	40.62%	5.393%
28	5.428	711	712	714	rBV	241	226	0.04%	0.005%
29	5.544	729	731	732	rBV	297	200	0.04%	0.005%
30	5.629	743	745	747	rBV	217	217	0.04%	0.005%
31	5.690	752	755	757	rBV2	222	227	0.04%	0.006%
32	5.964	790	800	817	rBV2	184510	546921	100.00%	13.279%
33	6.379	866	868	870	rBV	267	271	0.05%	0.007%
34	6.440	874	878	879	rBV	244	274	0.05%	0.007%
35	6.586	897	902	904	rBV2	281	478	0.09%	0.012%
36	6.763	922	931	950	rBV	158650	384650	70.33%	9.339%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042660.D
 Acq On : 28 Jul 2024 00:14
 Operator : JC/MD
 Sample : P3388-10 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.098	984	986	987	rBV2	736	574	0.10%	0.014%
38	7.202	1000	1003	1004	rBV2	345	269	0.05%	0.007%
39	7.306	1012	1020	1031	rBV	109692	243438	44.51%	5.911%
40	7.495	1049	1051	1054	rBV	359	326	0.06%	0.008%
41	7.568	1062	1063	1064	rBV	166	82	0.01%	0.002%
42	7.616	1069	1071	1074	rBV	181	237	0.04%	0.006%
43	7.641	1074	1075	1076	rVB	281	103	0.02%	0.003%
44	7.690	1081	1083	1084	rBV	191	184	0.03%	0.004%
45	7.720	1086	1088	1090	rVB	259	177	0.03%	0.004%
46	7.745	1090	1092	1096	rBV	364	390	0.07%	0.009%
47	7.812	1101	1103	1104	rBV	137	117	0.02%	0.003%
48	8.251	1173	1175	1177	rBV	253	294	0.05%	0.007%
49	8.324	1182	1187	1198	rBV	64252	107305	19.62%	2.605%
50	8.647	1234	1240	1255	rBV	267432	421637	77.09%	10.237%
51	8.952	1285	1290	1301	rBV	44861	68840	12.59%	1.671%
52	9.110	1314	1316	1317	rVB	340	193	0.04%	0.005%
53	9.147	1317	1322	1326	rBV2	341	733	0.13%	0.018%
54	9.384	1356	1361	1371	rBV	171779	263249	48.13%	6.392%
55	9.634	1401	1402	1404	rBV	208	158	0.03%	0.004%
56	9.775	1423	1425	1427	rBV	136	125	0.02%	0.003%
57	9.903	1444	1446	1448	rVB	191	137	0.03%	0.003%
58	10.055	1465	1471	1483	rBV	319975	451827	82.61%	10.970%
59	10.220	1496	1498	1500	rVB	256	155	0.03%	0.004%
60	10.244	1500	1502	1505	rBV2	240	282	0.05%	0.007%
61	10.415	1529	1530	1532	rVB	310	185	0.03%	0.004%
62	10.439	1532	1534	1536	rBV	257	180	0.03%	0.004%
63	10.494	1541	1543	1544	rBV	273	162	0.03%	0.004%
64	10.567	1551	1555	1559	rBV2	243	507	0.09%	0.012%
65	10.646	1567	1568	1570	rBV2	203	142	0.03%	0.003%
66	10.720	1578	1580	1583	rBV2	304	377	0.07%	0.009%
67	10.945	1615	1617	1618	rVB2	179	85	0.02%	0.002%
68	11.104	1642	1643	1645	rBV2	254	170	0.03%	0.004%
69	11.189	1652	1657	1667	rBV	216170	284197	51.96%	6.900%
70	11.305	1674	1676	1678	rBV	218	125	0.02%	0.003%
71	11.354	1683	1684	1685	rBV	238	124	0.02%	0.003%
72	11.402	1691	1692	1696	rVB2	139	119	0.02%	0.003%
73	11.445	1698	1699	1701	rVB	210	153	0.03%	0.004%
74	11.469	1701	1703	1704	rBV	144	71	0.01%	0.002%
75	11.573	1718	1720	1721	rBV	214	128	0.02%	0.003%
76	11.750	1746	1749	1750	rBV	154	193	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042660.D
 Acq On : 28 Jul 2024 00:14
 Operator : JC/MD
 Sample : P3388-10 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.805	1756	1758	1761	rBV2	257	375	0.07%	0.009%
78	12.018	1788	1793	1802	rBV	282779	363793	66.52%	8.833%
79	12.317	1837	1842	1855	rBV	270337	348022	63.63%	8.450%
80	12.494	1868	1871	1872	rBV	391	276	0.05%	0.007%
81	12.835	1925	1927	1929	rVB	264	145	0.03%	0.004%
82	12.853	1929	1930	1932	rBV	200	146	0.03%	0.004%
83	13.036	1956	1960	1962	rBV	202	269	0.05%	0.007%
84	13.189	1983	1985	1987	rBV2	294	372	0.07%	0.009%
85	13.414	2019	2022	2023	rBV	173	214	0.04%	0.005%
86	13.475	2031	2032	2037	rVB	262	247	0.05%	0.006%
87	13.524	2037	2040	2044	rBV2	295	423	0.08%	0.010%
88	13.554	2044	2045	2047	rBV	155	90	0.02%	0.002%
89	13.628	2054	2057	2059	rBV2	355	379	0.07%	0.009%
90	13.695	2066	2068	2070	rBV2	143	191	0.03%	0.005%
91	13.804	2084	2086	2087	rBV	241	167	0.03%	0.004%
92	13.951	2109	2110	2116	rBV2	256	436	0.08%	0.011%
93	14.134	2136	2140	2142	rBV3	503	700	0.13%	0.017%
94	14.341	2172	2174	2175	rBV3	121	78	0.01%	0.002%
95	14.634	2221	2222	2224	rVB	421	217	0.04%	0.005%
96	14.664	2225	2227	2229	rBV	241	171	0.03%	0.004%
97	14.816	2250	2252	2253	rBV	356	325	0.06%	0.008%
98	15.268	2325	2326	2329	rBV	334	407	0.07%	0.010%
99	15.786	2409	2411	2412	rBV	216	149	0.03%	0.004%
100	16.444	2516	2519	2521	rBV2	535	472	0.09%	0.011%

Sum of corrected areas: 4118663




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042660.D
Acq On : 28 Jul 2024 00:14
Operator : JC/MD
Sample : P3388-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

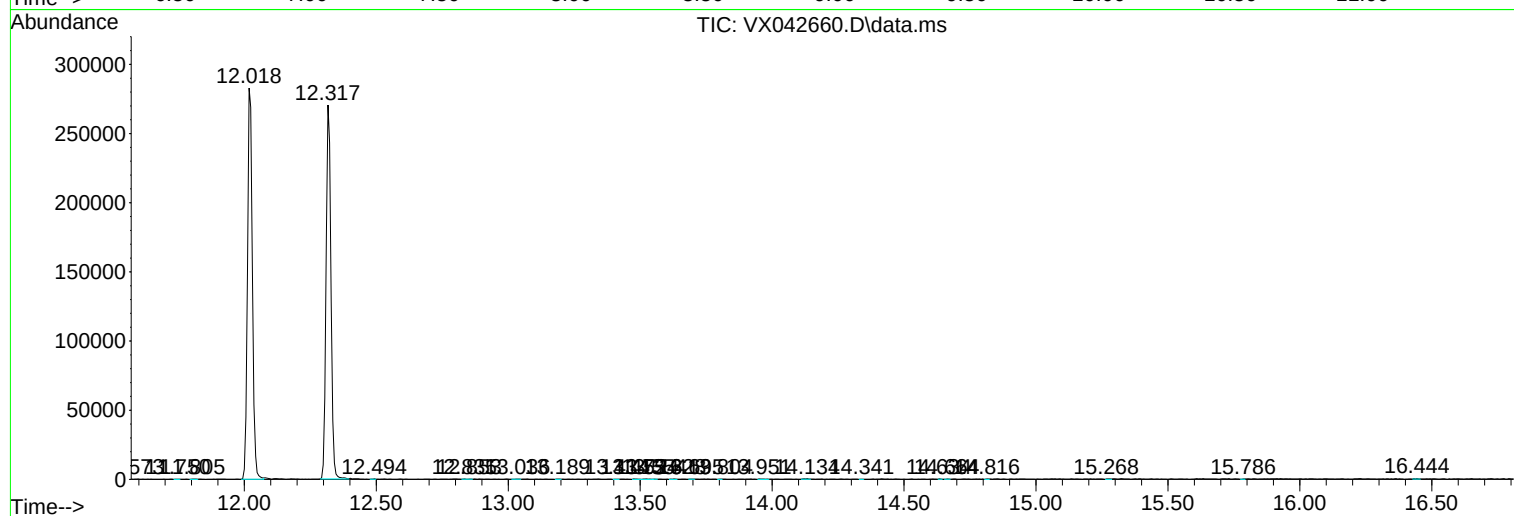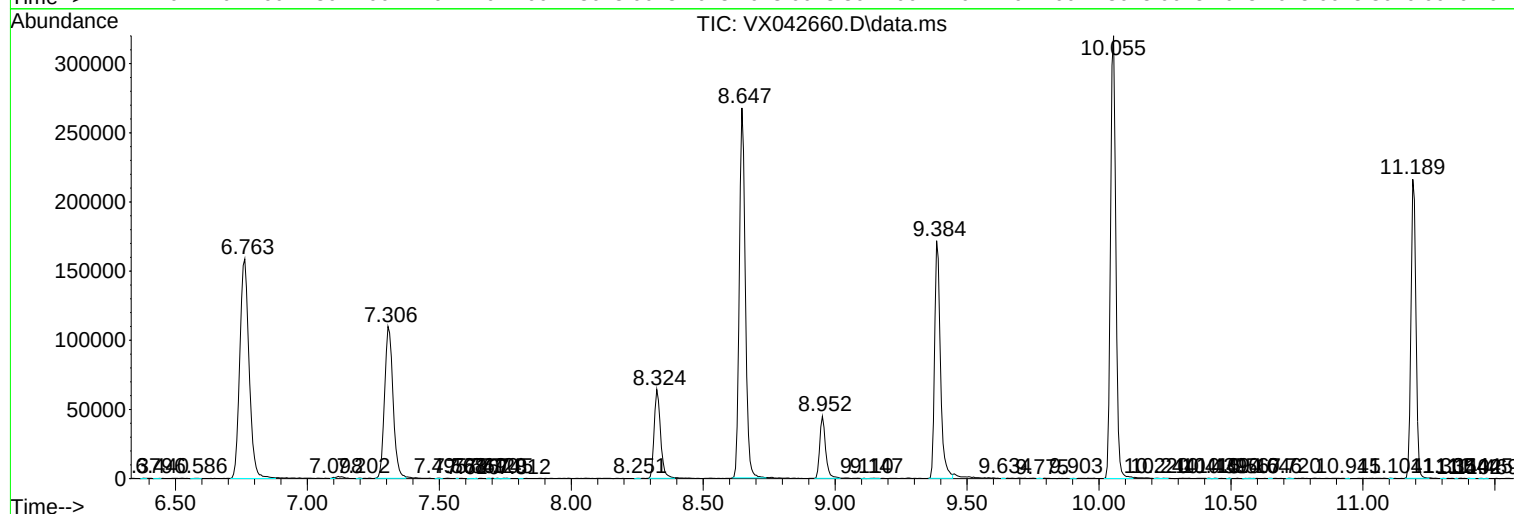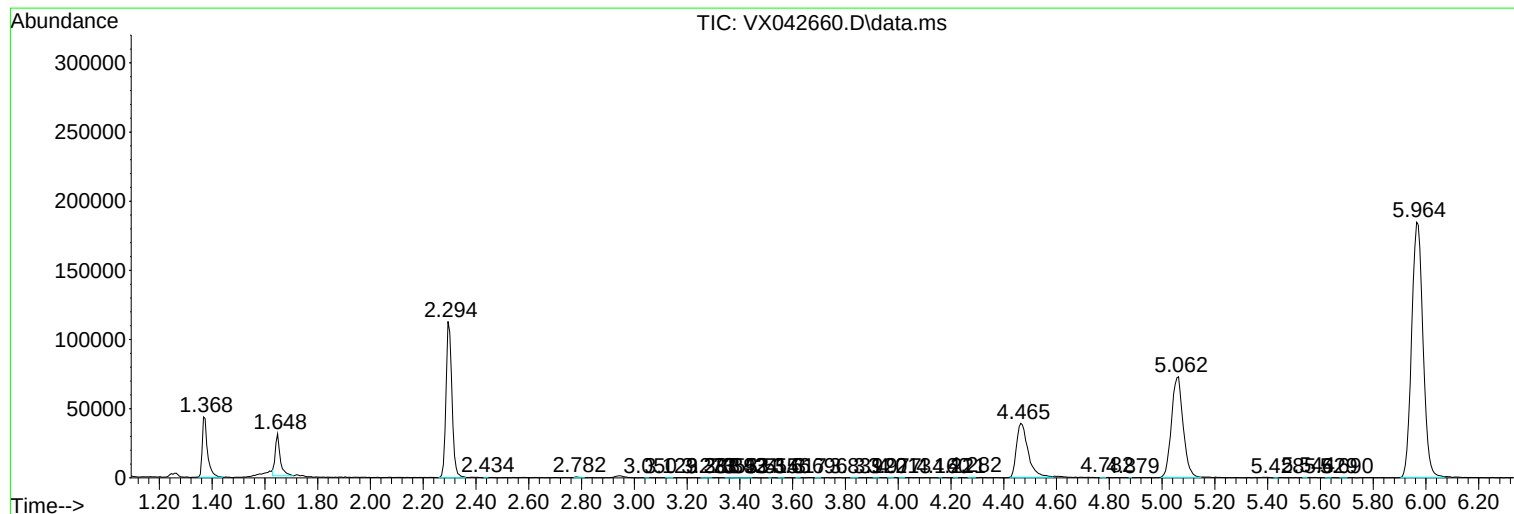

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042660.D
Acq On : 28 Jul 2024 00:14
Operator : JC/MD
Sample : P3388-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042660.D
Acq On : 28 Jul 2024 00:14
Operator : JC/MD
Sample : P3388-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc