

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042662.D
 Acq On : 28 Jul 2024 01:00
 Operator : JC/MD
 Sample : P3388-14 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	32	rBV3	2787	4948	0.88%	0.118%
2	1.368	43	46	57	rVB	43956	58021	10.36%	1.380%
3	1.526	70	72	73	rBV	714	528	0.09%	0.013%
4	1.551	73	76	77	rBV2	969	1030	0.18%	0.024%
5	1.648	88	92	100	rVB	29700	38216	6.82%	0.909%
6	2.069	159	161	164	rBV2	199	238	0.04%	0.006%
7	2.300	192	199	209	rBV	110080	177053	31.61%	4.211%
8	2.502	228	232	238	rVB	566	842	0.15%	0.020%
9	2.709	264	266	267	rBV	357	266	0.05%	0.006%
10	2.788	273	279	282	rBV4	1438	2515	0.45%	0.060%
11	2.867	288	292	293	rBV	227	319	0.06%	0.008%
12	2.947	298	305	313	rBV2	3822	8661	1.55%	0.206%
13	3.093	324	329	331	rBV3	950	1435	0.26%	0.034%
14	3.233	350	352	355	rBV	195	219	0.04%	0.005%
15	3.605	408	413	415	rBV2	356	656	0.12%	0.016%
16	3.745	434	436	438	rBV	203	244	0.04%	0.006%
17	3.977	470	474	476	rBV2	180	229	0.04%	0.005%
18	4.221	512	514	517	rBV2	193	277	0.05%	0.007%
19	4.465	546	554	571	rBV	40691	127384	22.74%	3.030%
20	4.922	625	629	632	rBV2	292	380	0.07%	0.009%
21	5.056	638	651	668	rBV	74748	226582	40.45%	5.389%
22	5.221	676	678	683	rBV3	401	438	0.08%	0.010%
23	5.355	697	700	701	rBV	364	397	0.07%	0.009%
24	5.556	730	733	734	rBV	340	344	0.06%	0.008%
25	5.647	744	748	749	rBV	298	256	0.05%	0.006%
26	5.769	766	768	770	rBV2	255	225	0.04%	0.005%
27	5.964	789	800	823	rBV2	187229	560126	100.00%	13.322%
28	6.348	861	863	865	rVV	348	332	0.06%	0.008%
29	6.385	867	869	871	rVV	281	290	0.05%	0.007%
30	6.446	876	879	881	rVV2	232	279	0.05%	0.007%
31	6.483	881	885	886	rVV	289	318	0.06%	0.008%
32	6.513	888	890	893	rVB2	204	277	0.05%	0.007%
33	6.757	922	930	944	rVV	159303	380407	67.91%	9.048%
34	7.129	983	991	1002	rVV6	11873	28411	5.07%	0.676%
35	7.306	1012	1020	1037	rBV	112148	251324	44.87%	5.978%
36	7.434	1039	1041	1046	rBV2	703	1019	0.18%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042662.D
 Acq On : 28 Jul 2024 01:00
 Operator : JC/MD
 Sample : P3388-14 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.824	1101	1105	1111	rVB2	564	951	0.17%	0.023%
38	8.324	1181	1187	1200	rBV	62217	108040	19.29%	2.570%
39	8.586	1223	1230	1234	rBV4	716	1528	0.27%	0.036%
40	8.647	1234	1240	1250	rBV	271524	425744	76.01%	10.126%
41	8.872	1273	1277	1279	rBV	279	303	0.05%	0.007%
42	8.952	1285	1290	1300	rBV	44979	70154	12.52%	1.669%
43	9.165	1321	1325	1330	rVB4	1076	1231	0.22%	0.029%
44	9.281	1340	1344	1347	rBV3	1247	1728	0.31%	0.041%
45	9.385	1356	1361	1378	rBV	159556	258011	46.06%	6.137%
46	9.616	1396	1399	1401	rBV2	454	518	0.09%	0.012%
47	9.951	1452	1454	1457	rBV2	247	240	0.04%	0.006%
48	10.055	1465	1471	1481	rBV	324582	447820	79.95%	10.651%
49	10.195	1491	1494	1500	rVB2	1374	2138	0.38%	0.051%
50	10.305	1508	1512	1518	rBV3	1533	2284	0.41%	0.054%
51	10.360	1518	1521	1523	rVB	204	231	0.04%	0.005%
52	10.482	1538	1541	1544	rBV2	257	343	0.06%	0.008%
53	10.646	1561	1568	1576	rBV5	1611	3764	0.67%	0.090%
54	10.768	1583	1588	1589	rBV	259	378	0.07%	0.009%
55	10.964	1618	1620	1623	rVV2	1289	1605	0.29%	0.038%
56	11.037	1630	1632	1636	rBV2	264	266	0.05%	0.006%
57	11.189	1652	1657	1664	rBV	212241	277876	49.61%	6.609%
58	11.451	1697	1700	1704	rVB2	1180	1404	0.25%	0.033%
59	11.646	1729	1732	1735	rBB	216	220	0.04%	0.005%
60	11.756	1747	1750	1755	rVB2	1471	1703	0.30%	0.041%
61	11.817	1758	1760	1762	rBV	277	280	0.05%	0.007%
62	11.969	1782	1785	1788	rBV2	1514	1779	0.32%	0.042%
63	12.018	1788	1793	1803	rVV	271058	358775	64.05%	8.533%
64	12.158	1813	1816	1821	rBV3	282	527	0.09%	0.013%
65	12.317	1837	1842	1857	rBV	267780	347857	62.10%	8.274%
66	12.451	1863	1864	1867	rVB	303	223	0.04%	0.005%
67	12.530	1874	1877	1880	rVV2	253	277	0.05%	0.007%
68	12.835	1926	1927	1931	rBV	198	213	0.04%	0.005%
69	12.920	1939	1941	1944	rVB	260	261	0.05%	0.006%
70	12.951	1944	1946	1948	rBV	463	412	0.07%	0.010%
71	13.116	1971	1973	1980	rVB2	589	884	0.16%	0.021%
72	13.268	1996	1998	2001	rVB	301	325	0.06%	0.008%
73	13.372	2013	2015	2018	rBV2	212	278	0.05%	0.007%
74	13.451	2024	2028	2029	rBV2	174	231	0.04%	0.005%
75	13.591	2049	2051	2056	rVB2	719	917	0.16%	0.022%
76	13.780	2077	2082	2083	rBV2	921	818	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042662.D
 Acq On : 28 Jul 2024 01:00
 Operator : JC/MD
 Sample : P3388-14 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	13.969	2109	2113	2116	rBV2	459	617	0.11%	0.015%
78	14.079	2127	2131	2133	rVB2	221	212	0.04%	0.005%
79	14.121	2137	2138	2145	rVV3	336	485	0.09%	0.012%
80	14.207	2148	2152	2156	rBV2	139	253	0.05%	0.006%
81	14.463	2193	2194	2197	rVV	264	228	0.04%	0.005%
82	14.542	2204	2207	2208	rBV2	272	236	0.04%	0.006%
83	14.560	2208	2210	2212	rVB	417	272	0.05%	0.006%
84	14.707	2230	2234	2236	rBV	271	369	0.07%	0.009%
85	14.920	2267	2269	2272	rVB2	374	243	0.04%	0.006%
86	14.963	2274	2276	2278	rVV	385	260	0.05%	0.006%
87	14.981	2278	2279	2282	rVV2	256	248	0.04%	0.006%
88	15.066	2292	2293	2296	rVB	393	264	0.05%	0.006%
89	15.097	2296	2298	2299	rBV2	361	322	0.06%	0.008%
90	15.158	2306	2308	2310	rBV2	360	286	0.05%	0.007%
91	15.310	2331	2333	2337	rBV	504	499	0.09%	0.012%
92	15.438	2352	2354	2357	rVB3	447	422	0.08%	0.010%
93	15.591	2377	2379	2380	rVB	649	309	0.06%	0.007%
94	15.682	2392	2394	2397	rVB	317	224	0.04%	0.005%
95	15.841	2416	2420	2422	rVB2	288	297	0.05%	0.007%
96	15.877	2425	2426	2431	rVB2	339	297	0.05%	0.007%
97	16.005	2445	2447	2449	rVV	271	229	0.04%	0.005%
98	16.322	2498	2499	2503	rBV3	251	292	0.05%	0.007%
99	16.389	2508	2510	2511	rBV	400	315	0.06%	0.007%
100	16.505	2527	2529	2530	rBV	253	218	0.04%	0.005%




Sum of corrected areas: 4204420

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042662.D
Acq On : 28 Jul 2024 01:00
Operator : JC/MD
Sample : P3388-14 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

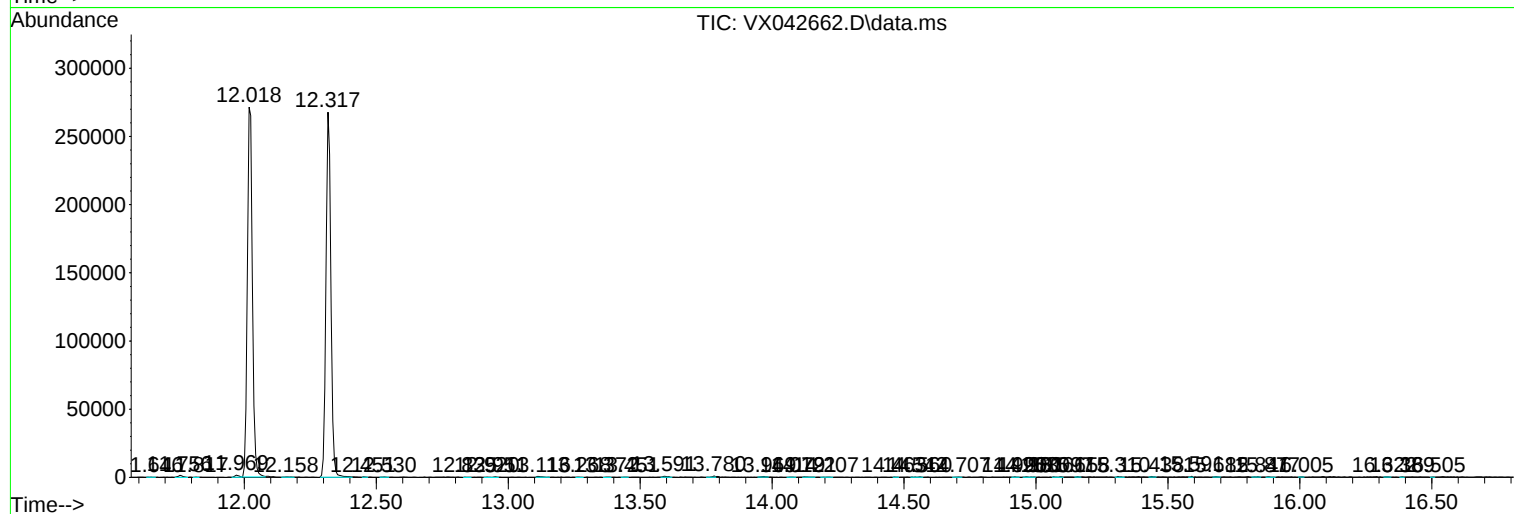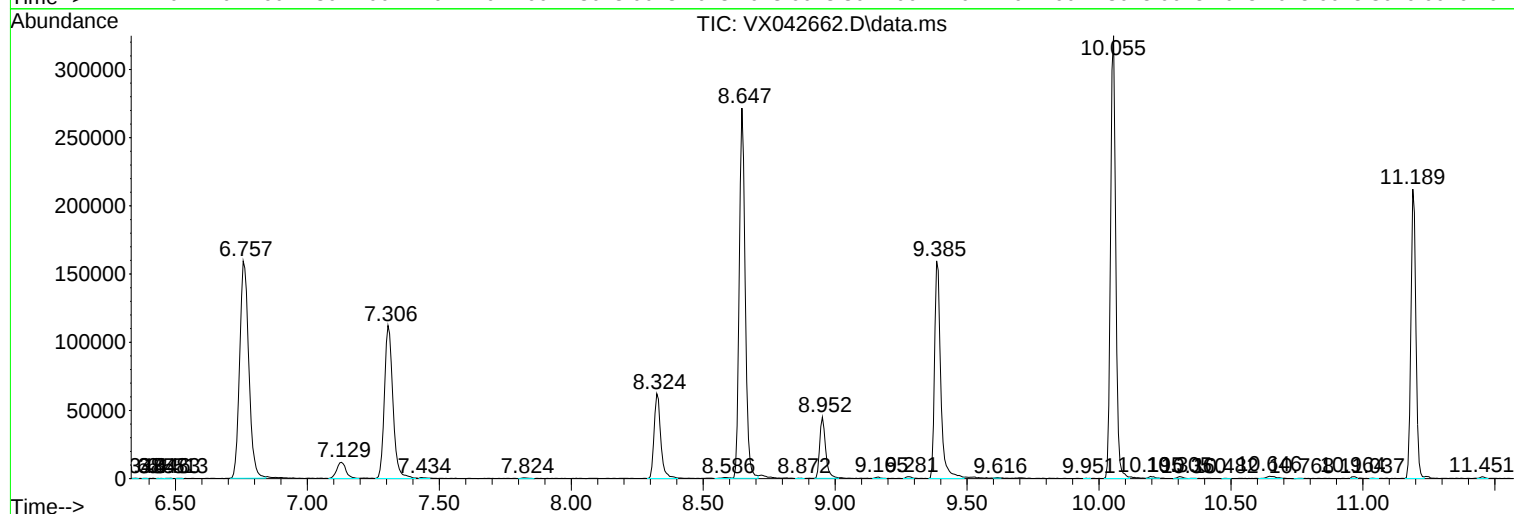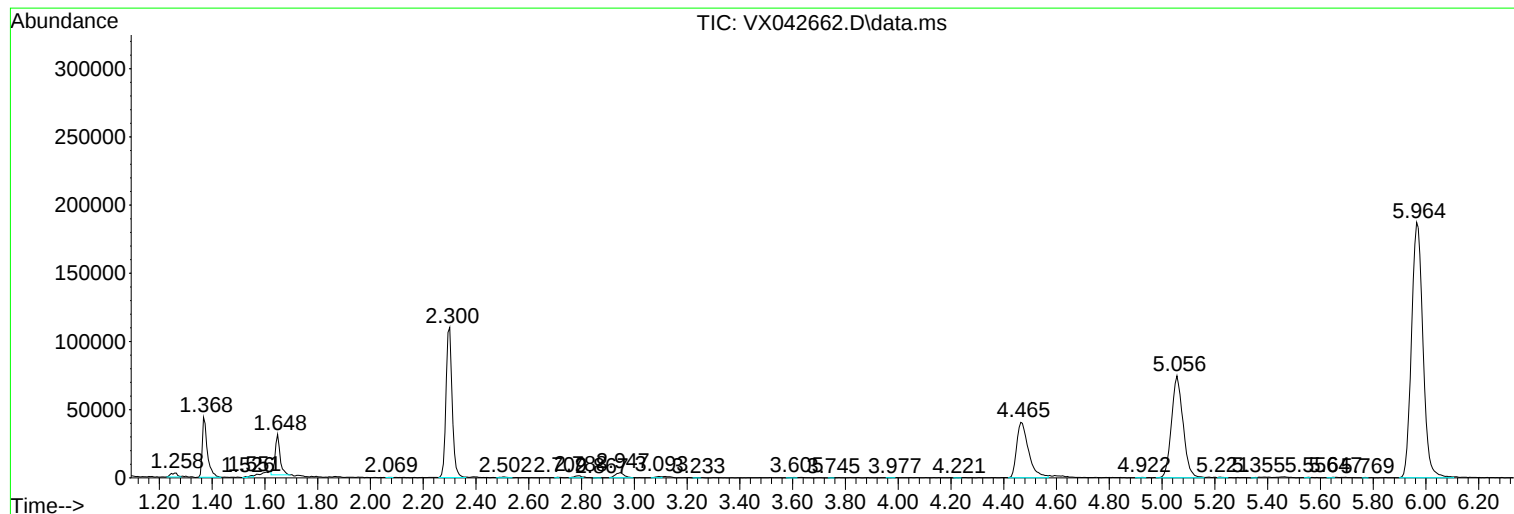

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042662.D
Acq On : 28 Jul 2024 01:00
Operator : JC/MD
Sample : P3388-14 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042662.D
Acq On : 28 Jul 2024 01:00
Operator : JC/MD
Sample : P3388-14 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------