

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042664.D
 Acq On : 28 Jul 2024 01:46
 Operator : JC/MD
 Sample : P3388-16 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	23	29	32	rBV4	3119	5295	0.96%	0.129%
2	1.368	43	46	60	rVB	43461	56805	10.31%	1.383%
3	1.575	70	80	81	rBV2	2590	4966	0.90%	0.121%
4	1.648	89	92	100	rVB	27422	36292	6.58%	0.884%
5	1.898	132	133	135	rBV	353	325	0.06%	0.008%
6	2.246	185	190	191	rBV	226	306	0.06%	0.007%
7	2.300	192	199	209	rVV	109294	171754	31.16%	4.182%
8	2.404	214	216	221	rVB	284	256	0.05%	0.006%
9	2.447	221	223	225	rVB	267	254	0.05%	0.006%
10	2.471	225	227	230	rBV	183	257	0.05%	0.006%
11	2.550	238	240	243	rBV2	198	198	0.04%	0.005%
12	2.630	250	253	256	rBV	211	216	0.04%	0.005%
13	2.782	276	278	280	rBV3	369	341	0.06%	0.008%
14	2.892	294	296	299	rVB	246	266	0.05%	0.006%
15	2.947	299	305	311	rBV3	1476	3523	0.64%	0.086%
16	3.032	315	319	321	rBV	245	339	0.06%	0.008%
17	3.215	347	349	352	rVB	398	341	0.06%	0.008%
18	3.318	364	366	369	rBB2	170	198	0.04%	0.005%
19	3.392	373	378	379	rBV	255	349	0.06%	0.008%
20	3.556	402	405	406	rBV	188	202	0.04%	0.005%
21	3.642	416	419	422	rBV2	154	221	0.04%	0.005%
22	4.178	506	507	511	rBV2	237	301	0.05%	0.007%
23	4.221	511	514	517	rBV2	199	276	0.05%	0.007%
24	4.300	524	527	528	rBV	180	199	0.04%	0.005%
25	4.465	546	554	574	rBV	38116	118594	21.51%	2.887%
26	4.800	605	609	612	rBV2	321	519	0.09%	0.013%
27	5.056	640	651	667	rBV	72966	227962	41.36%	5.550%
28	5.208	674	676	677	rVB	323	208	0.04%	0.005%
29	5.385	701	705	706	rBV2	253	285	0.05%	0.007%
30	5.544	729	731	734	rBV2	317	397	0.07%	0.010%
31	5.605	737	741	744	rBV2	245	404	0.07%	0.010%
32	5.964	790	800	818	rVV2	185217	551221	100.00%	13.421%
33	6.367	864	866	870	rVB2	313	409	0.07%	0.010%
34	6.409	870	873	875	rBB2	264	269	0.05%	0.007%
35	6.434	875	877	878	rBV	218	197	0.04%	0.005%
36	6.525	885	892	894	rBV2	211	393	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042664.D
 Acq On : 28 Jul 2024 01:46
 Operator : JC/MD
 Sample : P3388-16 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.763	922	931	946	rBV	157604	388373	70.46%	9.456%
38	7.056	977	979	981	rBV2	311	328	0.06%	0.008%
39	7.123	983	990	995	rBV6	1469	3486	0.63%	0.085%
40	7.202	999	1003	1004	rBV2	232	287	0.05%	0.007%
41	7.306	1011	1020	1035	rBV	113160	248925	45.16%	6.061%
42	7.690	1079	1083	1086	rBV2	213	243	0.04%	0.006%
43	7.745	1089	1092	1095	rBV	165	216	0.04%	0.005%
44	8.080	1146	1147	1149	rBV	250	207	0.04%	0.005%
45	8.141	1154	1157	1161	rBV2	296	496	0.09%	0.012%
46	8.214	1166	1169	1172	rBV	180	268	0.05%	0.007%
47	8.324	1181	1187	1204	rBV	60305	106979	19.41%	2.605%
48	8.513	1215	1218	1219	rBV	258	205	0.04%	0.005%
49	8.647	1234	1240	1251	rBV	266595	418874	75.99%	10.198%
50	8.836	1269	1271	1274	rVB3	260	314	0.06%	0.008%
51	8.952	1284	1290	1303	rBV	46446	69617	12.63%	1.695%
52	9.147	1318	1322	1325	rVB2	262	328	0.06%	0.008%
53	9.220	1329	1334	1336	rBV2	254	378	0.07%	0.009%
54	9.384	1356	1361	1377	rBV	159458	251591	45.64%	6.126%
55	9.701	1412	1413	1415	rVB	433	260	0.05%	0.006%
56	9.836	1432	1435	1438	rBV	179	286	0.05%	0.007%
57	9.866	1438	1440	1442	rVB2	256	242	0.04%	0.006%
58	9.897	1444	1445	1447	rBV	225	232	0.04%	0.006%
59	10.055	1465	1471	1483	rBV	320072	447480	81.18%	10.895%
60	10.214	1496	1497	1499	rVB2	485	293	0.05%	0.007%
61	10.622	1560	1564	1565	rBV2	191	246	0.04%	0.006%
62	10.963	1618	1620	1625	rBV2	171	312	0.06%	0.008%
63	11.018	1627	1629	1636	rVB2	178	330	0.06%	0.008%
64	11.073	1636	1638	1641	rBV2	196	216	0.04%	0.005%
65	11.189	1652	1657	1667	rBV	212560	273232	49.57%	6.652%
66	11.287	1671	1673	1675	rVB2	290	224	0.04%	0.005%
67	11.415	1691	1694	1696	rBV2	183	224	0.04%	0.005%
68	11.506	1705	1709	1712	rBV2	136	210	0.04%	0.005%
69	11.774	1748	1753	1754	rBV	232	395	0.07%	0.010%
70	11.793	1754	1756	1759	rVB	274	260	0.05%	0.006%
71	11.878	1765	1770	1772	rBV	167	301	0.05%	0.007%
72	11.969	1782	1785	1788	rBV	227	204	0.04%	0.005%
73	12.018	1788	1793	1804	rVV	268964	357327	64.82%	8.700%
74	12.219	1822	1826	1831	rVB2	224	433	0.08%	0.011%
75	12.317	1837	1842	1855	rBV	267338	340987	61.86%	8.302%
76	12.494	1869	1871	1874	rBV2	215	204	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042664.D
 Acq On : 28 Jul 2024 01:46
 Operator : JC/MD
 Sample : P3388-16 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.646	1893	1896	1897	rBV2	229	216	0.04%	0.005%
78	12.829	1923	1926	1928	rBV2	232	327	0.06%	0.008%
79	13.018	1955	1957	1961	rVB2	217	258	0.05%	0.006%
80	13.128	1973	1975	1978	rVV	242	260	0.05%	0.006%
81	13.353	2011	2012	2019	rVB2	158	304	0.06%	0.007%
82	13.585	2046	2050	2051	rBV	158	206	0.04%	0.005%
83	13.908	2099	2103	2106	rVB2	348	441	0.08%	0.011%
84	13.987	2112	2116	2117	rBV	247	326	0.06%	0.008%
85	14.091	2130	2133	2136	rBV2	193	256	0.05%	0.006%
86	14.524	2201	2204	2205	rBV	165	230	0.04%	0.006%
87	14.792	2245	2248	2251	rBV	398	599	0.11%	0.015%
88	14.847	2255	2257	2260	rVB2	320	324	0.06%	0.008%
89	14.883	2262	2263	2267	rVB	341	250	0.05%	0.006%
90	14.938	2270	2272	2274	rVB2	337	197	0.04%	0.005%
91	15.079	2293	2295	2296	rBV	275	213	0.04%	0.005%
92	15.225	2317	2319	2323	rVB2	249	261	0.05%	0.006%
93	15.389	2344	2346	2352	rVB2	740	1039	0.19%	0.025%
94	15.450	2352	2356	2358	rBV2	379	492	0.09%	0.012%
95	15.853	2421	2422	2423	rBV	430	223	0.04%	0.005%
96	15.902	2429	2430	2433	rVB2	353	316	0.06%	0.008%
97	15.938	2433	2436	2437	rBV	312	349	0.06%	0.008%
98	16.060	2454	2456	2457	rBV2	278	200	0.04%	0.005%
99	16.182	2474	2476	2479	rBV2	328	313	0.06%	0.008%
100	16.773	2571	2573	2575	rBV	296	268	0.05%	0.007%




Sum of corrected areas: 4107219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042664.D
Acq On : 28 Jul 2024 01:46
Operator : JC/MD
Sample : P3388-16 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

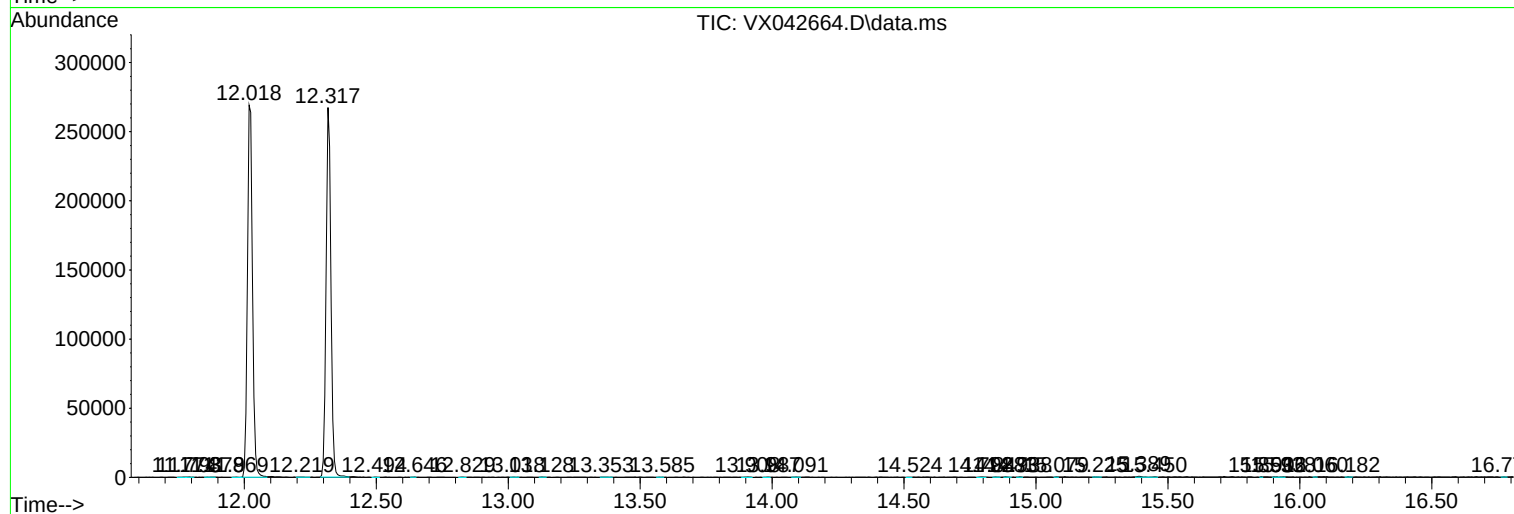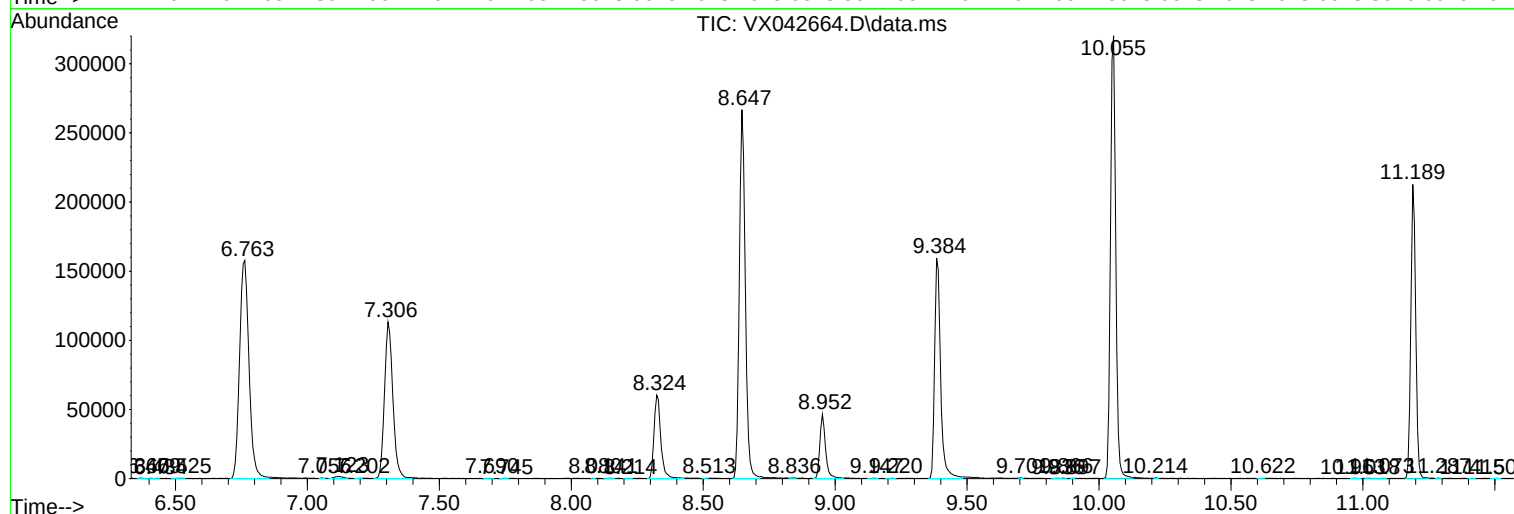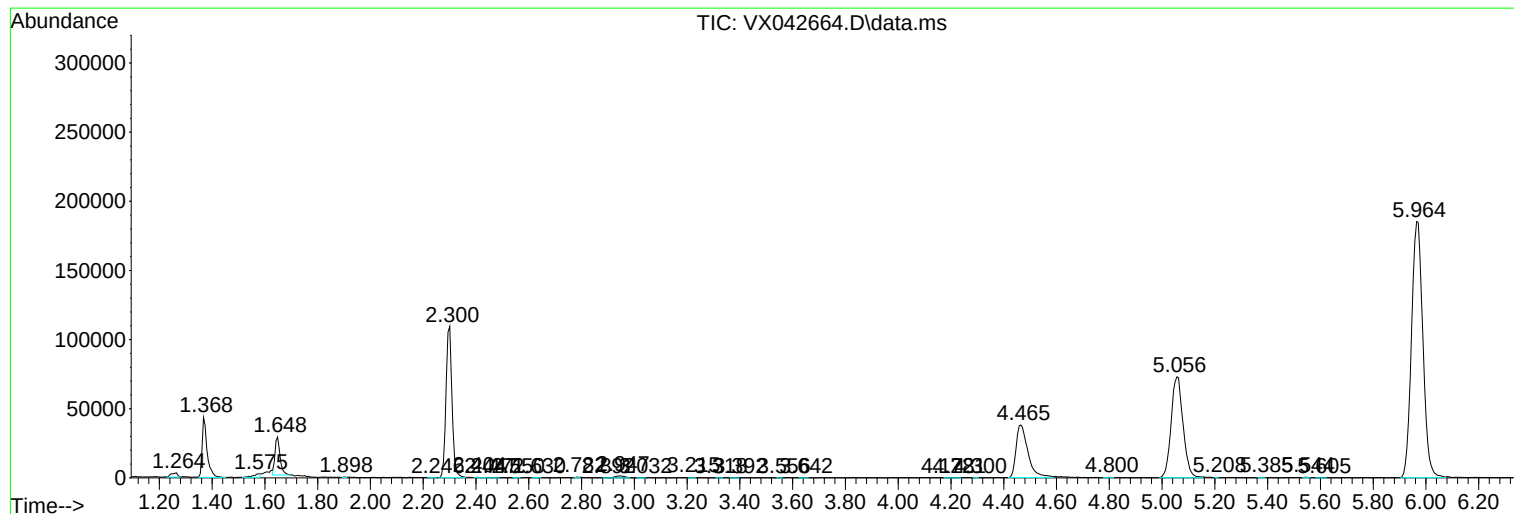

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042664.D
Acq On : 28 Jul 2024 01:46
Operator : JC/MD
Sample : P3388-16 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042664.D
Acq On : 28 Jul 2024 01:46
Operator : JC/MD
Sample : P3388-16 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc