

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042667.D
 Acq On : 28 Jul 2024 02:55
 Operator : JC/MD
 Sample : P3388-19 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rBV	43915	56641	10.04%	1.367%
2	1.526	70	72	73	rBV	677	447	0.08%	0.011%
3	1.648	89	92	103	rVB	32402	42114	7.46%	1.016%
4	2.057	157	159	160	rBV	289	167	0.03%	0.004%
5	2.075	160	162	164	rBV	351	219	0.04%	0.005%
6	2.294	192	198	210	rBV	107866	173485	30.75%	4.186%
7	2.380	210	212	213	rVB	473	192	0.03%	0.005%
8	2.532	235	237	240	rBV	312	252	0.04%	0.006%
9	2.941	298	304	316	rBV2	4348	9953	1.76%	0.240%
10	3.062	322	324	325	rBV	164	132	0.02%	0.003%
11	3.111	330	332	335	rVV	144	149	0.03%	0.004%
12	3.172	340	342	343	rBV	217	161	0.03%	0.004%
13	3.312	363	365	367	rBB	123	96	0.02%	0.002%
14	3.392	373	378	384	rBV	189	440	0.08%	0.011%
15	3.471	388	391	394	rBV2	170	282	0.05%	0.007%
16	3.520	398	399	401	rVB2	203	101	0.02%	0.002%
17	3.562	401	406	407	rBV2	184	273	0.05%	0.007%
18	3.678	423	425	428	rBV	267	297	0.05%	0.007%
19	3.745	434	436	440	rBB	313	273	0.05%	0.007%
20	3.794	441	444	445	rBV	98	113	0.02%	0.003%
21	3.818	445	448	449	rVB	212	191	0.03%	0.005%
22	3.831	449	450	455	rBB	257	369	0.07%	0.009%
23	3.910	462	463	465	rVB	179	124	0.02%	0.003%
24	4.032	482	483	486	rBV2	185	175	0.03%	0.004%
25	4.160	503	504	506	rBV	215	134	0.02%	0.003%
26	4.209	509	512	514	rBV2	266	341	0.06%	0.008%
27	4.465	545	554	569	rBV	40795	120189	21.30%	2.900%
28	5.062	639	652	668	rBV2	73432	231643	41.05%	5.590%
29	5.349	697	699	700	rVB	181	93	0.02%	0.002%
30	5.477	717	720	722	rBV	223	239	0.04%	0.006%
31	5.574	733	736	738	rBV	217	316	0.06%	0.008%
32	5.678	752	753	756	rBB	141	120	0.02%	0.003%
33	5.739	756	763	765	rBB2	264	489	0.09%	0.012%
34	5.763	765	767	768	rBV2	125	96	0.02%	0.002%
35	5.806	772	774	776	rBB	94	93	0.02%	0.002%
36	5.830	776	778	780	rBV	211	236	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042667.D
 Acq On : 28 Jul 2024 02:55
 Operator : JC/MD
 Sample : P3388-19 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.964	789	800	818	rBV3	190804	564228	100.00%	13.615%
38	6.318	856	858	859	rBV3	190	168	0.03%	0.004%
39	6.391	868	870	872	rVB2	280	164	0.03%	0.004%
40	6.409	872	873	876	rVB	204	168	0.03%	0.004%
41	6.440	876	878	879	rBV	276	235	0.04%	0.006%
42	6.635	908	910	913	rBV	234	270	0.05%	0.007%
43	6.763	921	931	948	rBV	158011	386563	68.51%	9.328%
44	7.074	979	982	983	rBV	412	378	0.07%	0.009%
45	7.117	984	989	994	rVV6	1467	3276	0.58%	0.079%
46	7.306	1012	1020	1034	rBV	112543	251547	44.58%	6.070%
47	7.482	1047	1049	1050	rBV	363	274	0.05%	0.007%
48	7.671	1079	1080	1082	rBV	244	231	0.04%	0.006%
49	7.726	1088	1089	1091	rVB	249	162	0.03%	0.004%
50	7.763	1091	1095	1097	rBV2	276	393	0.07%	0.009%
51	7.873	1111	1113	1116	rVB	289	243	0.04%	0.006%
52	8.031	1135	1139	1141	rBB2	268	367	0.07%	0.009%
53	8.068	1142	1145	1147	rBV	231	285	0.05%	0.007%
54	8.159	1157	1160	1162	rBV	226	294	0.05%	0.007%
55	8.324	1181	1187	1196	rBV	63430	107282	19.01%	2.589%
56	8.494	1212	1215	1217	rBV	406	458	0.08%	0.011%
57	8.598	1231	1232	1233	rBV	181	120	0.02%	0.003%
58	8.647	1233	1240	1255	rVV	273309	434862	77.07%	10.494%
59	8.915	1283	1284	1285	rBV	349	234	0.04%	0.006%
60	8.952	1285	1290	1300	rVV	46770	69583	12.33%	1.679%
61	9.177	1323	1327	1330	rBV2	196	301	0.05%	0.007%
62	9.202	1330	1331	1334	rVB	247	247	0.04%	0.006%
63	9.238	1334	1337	1338	rBV	282	349	0.06%	0.008%
64	9.384	1356	1361	1376	rBV	169373	258797	45.87%	6.245%
65	9.738	1417	1419	1421	rBV	206	174	0.03%	0.004%
66	10.055	1465	1471	1481	rBV	319499	440973	78.16%	10.641%
67	10.360	1519	1521	1527	rBV2	208	431	0.08%	0.010%
68	10.537	1549	1550	1551	rBV	205	104	0.02%	0.003%
69	10.646	1566	1568	1571	rBV2	264	316	0.06%	0.008%
70	10.890	1606	1608	1609	rBV	212	218	0.04%	0.005%
71	11.049	1631	1634	1635	rBV	310	324	0.06%	0.008%
72	11.140	1648	1649	1652	rBV	125	153	0.03%	0.004%
73	11.189	1652	1657	1666	rVV	209915	277720	49.22%	6.702%
74	11.323	1676	1679	1680	rBV	196	246	0.04%	0.006%
75	11.384	1688	1689	1690	rBV	204	105	0.02%	0.003%
76	11.457	1699	1701	1704	rBV	262	268	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042667.D
 Acq On : 28 Jul 2024 02:55
 Operator : JC/MD
 Sample : P3388-19 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.573	1718	1720	1721	rBV	166	96	0.02%	0.002%
78	11.847	1763	1765	1767	rBV	206	201	0.04%	0.005%
79	11.969	1784	1785	1788	rBV	253	314	0.06%	0.008%
80	12.018	1788	1793	1807	rVV	267220	353357	62.63%	8.527%
81	12.317	1837	1842	1853	rBV	270214	342605	60.72%	8.267%
82	12.512	1873	1874	1876	rBV	351	196	0.03%	0.005%
83	12.652	1895	1897	1898	rBV	238	214	0.04%	0.005%
84	12.738	1907	1911	1912	rBV2	298	361	0.06%	0.009%
85	12.780	1916	1918	1922	rVB	177	218	0.04%	0.005%
86	12.884	1933	1935	1940	rBV	132	193	0.03%	0.005%
87	13.055	1962	1963	1965	rBV	197	134	0.02%	0.003%
88	13.213	1988	1989	1992	rBB	156	137	0.02%	0.003%
89	13.256	1994	1996	1998	rBV2	240	262	0.05%	0.006%
90	13.445	2024	2027	2030	rBV2	162	252	0.04%	0.006%
91	13.609	2052	2054	2056	rBV	168	133	0.02%	0.003%
92	13.786	2082	2083	2084	rBV	198	107	0.02%	0.003%
93	14.060	2126	2128	2131	rBV	179	185	0.03%	0.004%
94	14.152	2142	2143	2145	rBV	183	157	0.03%	0.004%
95	14.365	2177	2178	2180	rBV	161	146	0.03%	0.004%
96	14.463	2192	2194	2195	rBV	357	245	0.04%	0.006%
97	14.780	2244	2246	2247	rBV	196	99	0.02%	0.002%
98	15.713	2397	2399	2402	rBV	472	512	0.09%	0.012%
99	15.920	2431	2433	2436	rBV	395	499	0.09%	0.012%
100	16.639	2550	2551	2552	rBV	426	245	0.04%	0.006%


Sum of corrected areas: 4144014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042667.D
Acq On : 28 Jul 2024 02:55
Operator : JC/MD
Sample : P3388-19 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

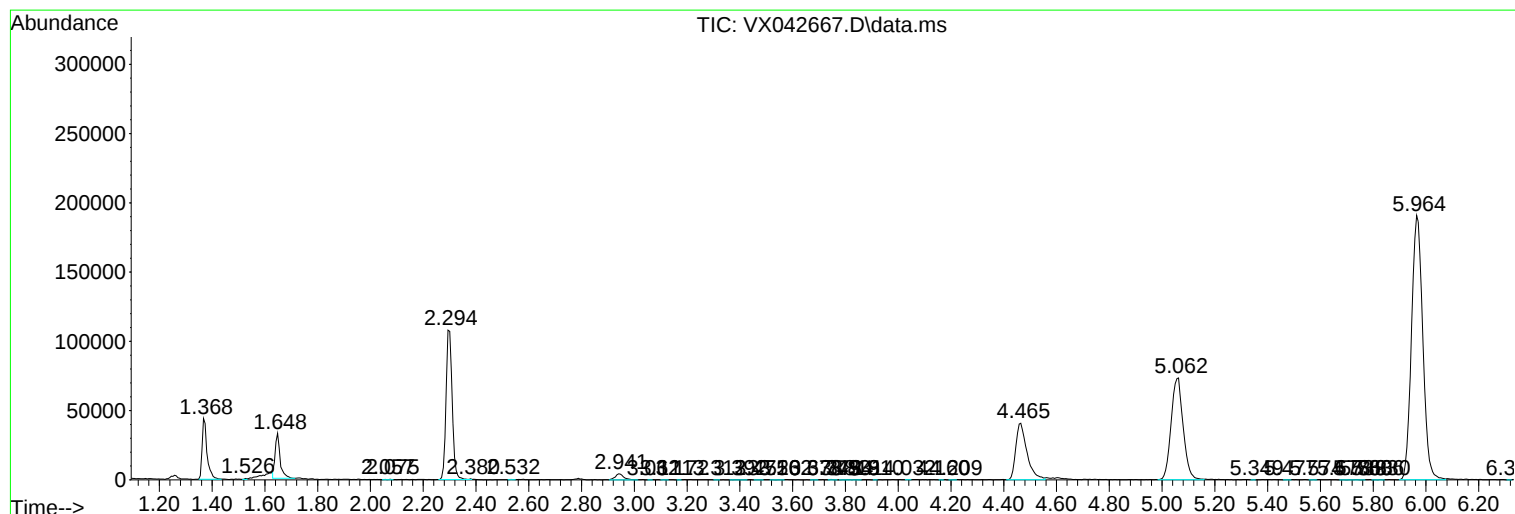

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042667.D
Acq On : 28 Jul 2024 02:55
Operator : JC/MD
Sample : P3388-19 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042667.D
Acq On : 28 Jul 2024 02:55
Operator : JC/MD
Sample : P3388-19 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------