

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042669.D
 Acq On : 28 Jul 2024 03:41
 Operator : JC/MD
 Sample : P3388-21 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	59	rVB	39575	55295	10.31%	1.359%
2	1.648	89	92	103	rVB	29759	38929	7.26%	0.957%
3	2.300	193	199	209	rBV	105859	165460	30.84%	4.066%
4	2.501	231	232	236	rVB3	263	190	0.04%	0.005%
5	2.709	265	266	270	rBV	186	191	0.04%	0.005%
6	2.831	284	286	288	rVB	131	101	0.02%	0.002%
7	2.947	298	305	316	rVV2	4082	10027	1.87%	0.246%
8	3.203	345	347	351	rBV	276	233	0.04%	0.006%
9	3.294	360	362	364	rBV2	93	90	0.02%	0.002%
10	3.349	370	371	372	rBV2	217	104	0.02%	0.003%
11	3.434	382	385	386	rBB2	123	97	0.02%	0.002%
12	3.489	390	394	395	rBB2	224	178	0.03%	0.004%
13	3.520	397	399	401	rBV2	179	174	0.03%	0.004%
14	3.587	407	410	411	rBV	69	69	0.01%	0.002%
15	3.684	424	426	429	rBV	170	199	0.04%	0.005%
16	3.751	434	437	438	rBB	171	165	0.03%	0.004%
17	3.770	438	440	442	rBV	103	101	0.02%	0.002%
18	3.794	443	444	446	rVV	198	130	0.02%	0.003%
19	3.818	446	448	451	rVV	254	269	0.05%	0.007%
20	3.873	455	457	458	rBB	148	103	0.02%	0.003%
21	3.891	458	460	461	rBB	159	98	0.02%	0.002%
22	3.940	466	468	470	rBV	90	101	0.02%	0.002%
23	3.959	470	471	474	rBV2	138	171	0.03%	0.004%
24	4.056	485	487	488	rBV	167	145	0.03%	0.004%
25	4.257	518	520	521	rBV	195	122	0.02%	0.003%
26	4.276	521	523	527	rVB	204	258	0.05%	0.006%
27	4.397	540	543	546	rBV2	236	328	0.06%	0.008%
28	4.465	546	554	571	rBV	40278	127707	23.80%	3.138%
29	5.050	642	650	664	rVB	70322	211805	39.48%	5.204%
30	5.391	703	706	709	rBV	249	399	0.07%	0.010%
31	5.440	712	714	716	rVB	227	140	0.03%	0.003%
32	5.464	716	718	719	rBV	237	182	0.03%	0.004%
33	5.678	750	753	754	rBV	171	153	0.03%	0.004%
34	5.806	771	774	775	rBV2	225	227	0.04%	0.006%
35	5.848	779	781	784	rVB	171	176	0.03%	0.004%
36	5.964	790	800	815	rBV3	182954	536514	100.00%	13.183%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042669.D
 Acq On : 28 Jul 2024 03:41
 Operator : JC/MD
 Sample : P3388-21 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.233	843	844	847	rBV2	194	210	0.04%	0.005%
38	6.361	863	865	866	rBV2	186	146	0.03%	0.004%
39	6.428	874	876	878	rBV2	188	192	0.04%	0.005%
40	6.482	883	885	888	rBV	248	252	0.05%	0.006%
41	6.556	895	897	898	rBV	216	159	0.03%	0.004%
42	6.690	918	919	920	rVB	281	103	0.02%	0.003%
43	6.757	920	930	944	rBV	149898	373622	69.64%	9.180%
44	7.043	975	977	979	rBV2	272	280	0.05%	0.007%
45	7.129	983	991	1004	rVV3	24208	58064	10.82%	1.427%
46	7.306	1012	1020	1031	rBV	106898	240909	44.90%	5.919%
47	7.647	1074	1076	1078	rBV	160	122	0.02%	0.003%
48	7.909	1116	1119	1120	rBV2	159	158	0.03%	0.004%
49	7.976	1126	1130	1133	rBV2	352	477	0.09%	0.012%
50	8.147	1156	1158	1162	rBV2	211	315	0.06%	0.008%
51	8.232	1171	1172	1173	rVB2	218	80	0.01%	0.002%
52	8.257	1173	1176	1177	rBV	234	212	0.04%	0.005%
53	8.324	1182	1187	1204	rVV	59386	102379	19.08%	2.516%
54	8.647	1234	1240	1256	rBV	261657	412213	76.83%	10.129%
55	8.952	1285	1290	1300	rBV	44367	66573	12.41%	1.636%
56	9.232	1332	1336	1339	rBV2	315	546	0.10%	0.013%
57	9.323	1348	1351	1356	rBV	261	505	0.09%	0.012%
58	9.384	1356	1361	1381	rVV	162034	251854	46.94%	6.188%
59	10.055	1465	1471	1483	rBV	316129	434747	81.03%	10.682%
60	10.323	1514	1515	1516	rBV	244	116	0.02%	0.003%
61	10.403	1526	1528	1531	rBV2	117	148	0.03%	0.004%
62	10.537	1548	1550	1554	rBV2	146	214	0.04%	0.005%
63	10.756	1583	1586	1588	rBV2	165	211	0.04%	0.005%
64	10.823	1595	1597	1598	rBV	186	144	0.03%	0.004%
65	10.872	1603	1605	1606	rBV	183	107	0.02%	0.003%
66	10.939	1614	1616	1619	rVB	194	109	0.02%	0.003%
67	11.061	1635	1636	1638	rBV	165	146	0.03%	0.004%
68	11.134	1646	1648	1649	rBV	220	187	0.03%	0.005%
69	11.189	1652	1657	1668	rVV	215134	276286	51.50%	6.789%
70	11.299	1673	1675	1677	rBV	134	136	0.03%	0.003%
71	11.335	1679	1681	1684	rBV	242	214	0.04%	0.005%
72	11.482	1703	1705	1707	rBV	152	155	0.03%	0.004%
73	11.530	1711	1713	1714	rBV	210	183	0.03%	0.004%
74	11.634	1727	1730	1731	rVB	233	191	0.04%	0.005%
75	11.652	1731	1733	1734	rBV	187	149	0.03%	0.004%
76	11.713	1739	1743	1744	rBV	192	245	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042669.D
 Acq On : 28 Jul 2024 03:41
 Operator : JC/MD
 Sample : P3388-21 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.768	1750	1752	1753	rBV	165	156	0.03%	0.004%
78	11.835	1760	1763	1768	rBB2	254	461	0.09%	0.011%
79	11.878	1768	1770	1772	rBB	231	193	0.04%	0.005%
80	11.896	1772	1773	1774	rBB	171	63	0.01%	0.002%
81	11.921	1774	1777	1780	rBV2	239	345	0.06%	0.008%
82	12.024	1788	1794	1810	rBV	273949	354256	66.03%	8.705%
83	12.189	1819	1821	1822	rBV	232	131	0.02%	0.003%
84	12.317	1837	1842	1851	rBV	262815	336546	62.73%	8.269%
85	12.579	1884	1885	1888	rBV	138	144	0.03%	0.004%
86	13.048	1961	1962	1965	rBV	221	224	0.04%	0.006%
87	13.518	2035	2039	2042	rBV	229	320	0.06%	0.008%
88	13.640	2058	2059	2060	rBV	139	86	0.02%	0.002%
89	13.737	2072	2075	2078	rBV2	279	441	0.08%	0.011%
90	14.127	2137	2139	2142	rBV	332	429	0.08%	0.011%
91	14.335	2171	2173	2175	rBV	268	281	0.05%	0.007%
92	14.444	2190	2191	2196	rBV2	171	286	0.05%	0.007%
93	14.530	2204	2205	2208	rBV	166	188	0.04%	0.005%
94	14.640	2222	2223	2226	rBV	207	216	0.04%	0.005%
95	14.670	2226	2228	2229	rBV2	210	184	0.03%	0.005%
96	14.798	2248	2249	2251	rBV	291	158	0.03%	0.004%
97	14.993	2280	2281	2284	rBV2	389	336	0.06%	0.008%
98	15.310	2331	2333	2335	rBV	268	175	0.03%	0.004%
99	15.414	2349	2350	2355	rBV	384	385	0.07%	0.009%
100	16.334	2500	2501	2502	rBV	286	108	0.02%	0.003%




Sum of corrected areas: 4069802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042669.D
Acq On : 28 Jul 2024 03:41
Operator : JC/MD
Sample : P3388-21 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

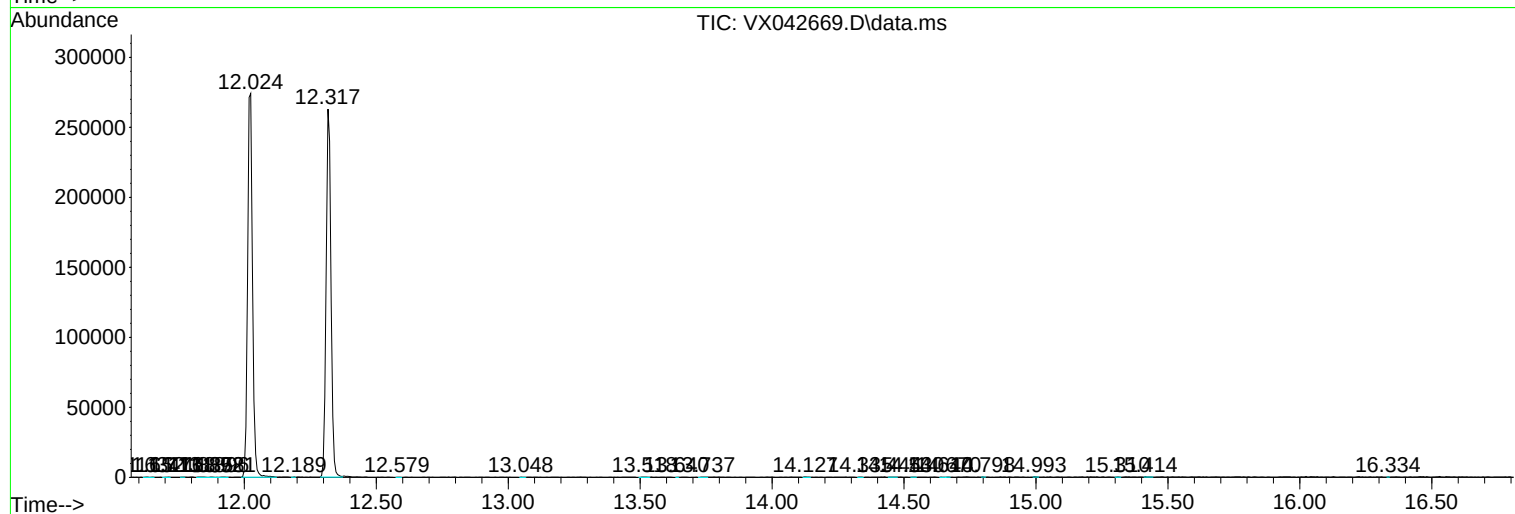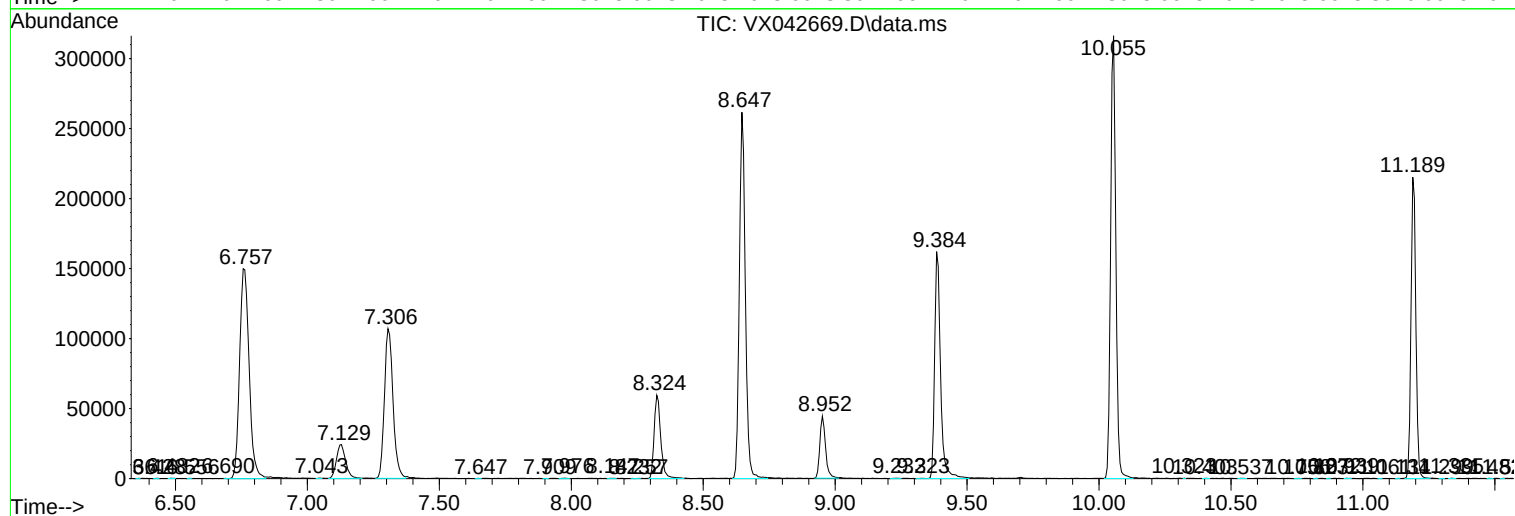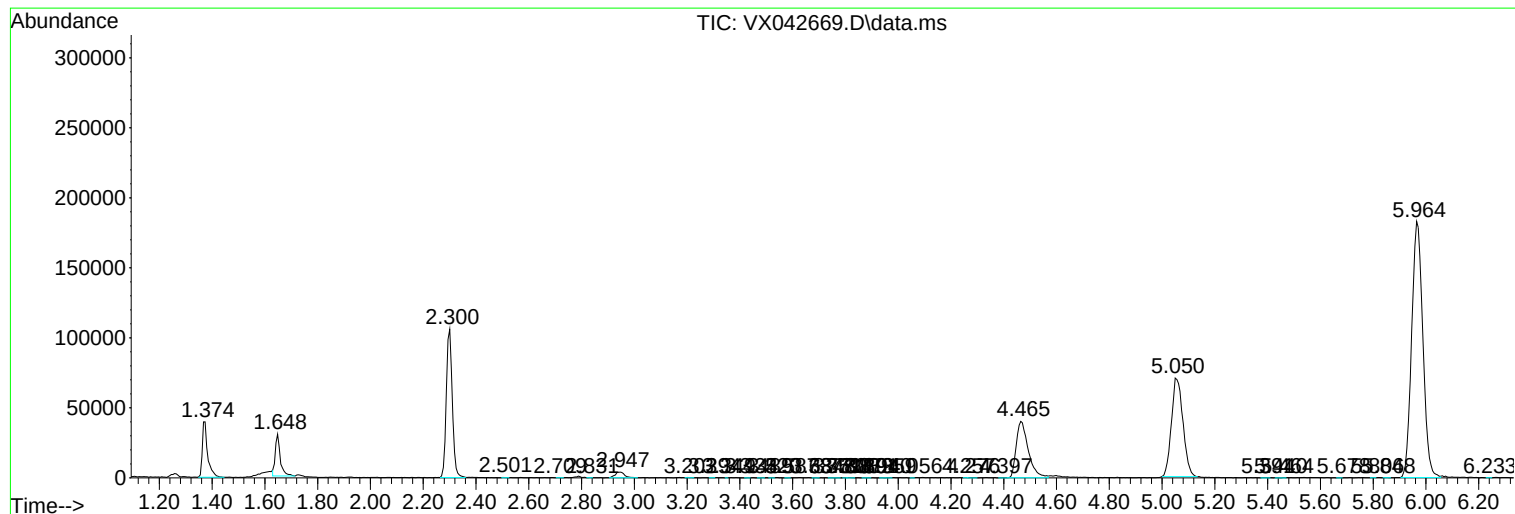

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042669.D
Acq On : 28 Jul 2024 03:41
Operator : JC/MD
Sample : P3388-21 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042669.D
Acq On : 28 Jul 2024 03:41
Operator : JC/MD
Sample : P3388-21 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
