

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042670.D
 Acq On : 28 Jul 2024 04:04
 Operator : JC/MD
 Sample : P3389-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	44500	55779	10.20%	1.383%
2	1.648	89	92	103	rVB	30964	39980	7.31%	0.991%
3	2.300	192	199	209	rBV	107264	169343	30.97%	4.199%
4	2.788	275	279	284	rVB4	1189	2293	0.42%	0.057%
5	2.831	284	286	290	rBV	290	383	0.07%	0.009%
6	2.886	293	295	296	rBV	147	104	0.02%	0.003%
7	2.941	299	304	315	rVB2	5477	12212	2.23%	0.303%
8	3.099	325	330	331	rBB	234	254	0.05%	0.006%
9	3.129	331	335	336	rBV	160	196	0.04%	0.005%
10	3.233	350	352	355	rBV2	282	283	0.05%	0.007%
11	3.264	355	357	359	rVB2	277	242	0.04%	0.006%
12	3.373	372	375	376	rVB	195	157	0.03%	0.004%
13	3.392	376	378	380	rBV	213	214	0.04%	0.005%
14	3.623	415	416	419	rBV	95	121	0.02%	0.003%
15	3.690	426	427	429	rBV2	146	108	0.02%	0.003%
16	3.764	438	439	442	rBV2	183	175	0.03%	0.004%
17	3.849	450	453	454	rBV	210	165	0.03%	0.004%
18	4.166	503	505	507	rVB	179	110	0.02%	0.003%
19	4.312	527	529	530	rVB	219	126	0.02%	0.003%
20	4.337	530	533	535	rBV2	226	286	0.05%	0.007%
21	4.398	541	543	544	rBV	229	160	0.03%	0.004%
22	4.465	546	554	569	rBV	39181	115762	21.17%	2.870%
23	4.946	631	633	634	rVB	223	127	0.02%	0.003%
24	5.056	640	651	668	rBV	72799	224516	41.06%	5.567%
25	5.282	684	688	691	rBV2	135	190	0.03%	0.005%
26	5.367	698	702	703	rBV	302	246	0.04%	0.006%
27	5.397	706	707	708	rVV	380	223	0.04%	0.006%
28	5.440	712	714	717	rBV	198	305	0.06%	0.008%
29	5.464	717	718	721	rVB	331	250	0.05%	0.006%
30	5.605	736	741	743	rBV2	262	379	0.07%	0.009%
31	5.653	747	749	750	rBV	170	133	0.02%	0.003%
32	5.684	753	754	760	rVB	216	275	0.05%	0.007%
33	5.964	789	800	818	rBV3	182121	546743	100.00%	13.556%
34	6.166	832	833	835	rBV	162	136	0.02%	0.003%
35	6.226	841	843	846	rVB2	326	294	0.05%	0.007%
36	6.257	847	848	850	rBV	209	147	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042670.D
Acq On : 28 Jul 2024 04:04
Operator : JC/MD
Sample : P3389-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Title : VOC Analysis

37	6.373	863	867	868	rBV	201	289	0.05%	0.007%
38	6.440	876	878	882	rBV2	184	222	0.04%	0.006%
39	6.531	890	893	894	rBV	274	244	0.04%	0.006%
40	6.690	918	919	921	rBV	194	143	0.03%	0.004%
41	6.757	922	930	946	rVV	156544	379331	69.38%	9.406%
42	7.068	978	981	982	rBV2	289	282	0.05%	0.007%
43	7.184	998	1000	1001	rVB	202	112	0.02%	0.003%
44	7.196	1001	1002	1004	rBV	411	353	0.06%	0.009%
45	7.306	1013	1020	1036	rBV	111649	247018	45.18%	6.125%
46	7.952	1123	1126	1130	rBV	180	307	0.06%	0.008%
47	8.049	1140	1142	1144	rBV2	179	157	0.03%	0.004%
48	8.098	1148	1150	1151	rBV	133	96	0.02%	0.002%
49	8.177	1161	1163	1165	rVB	298	213	0.04%	0.005%
50	8.220	1168	1170	1171	rBV	138	98	0.02%	0.002%
51	8.324	1181	1187	1200	rBV	61765	105723	19.34%	2.621%
52	8.464	1208	1210	1212	rBV	327	251	0.05%	0.006%
53	8.574	1226	1228	1230	rBV2	221	229	0.04%	0.006%
54	8.647	1234	1240	1256	rBV	266346	418634	76.57%	10.380%
55	8.952	1285	1290	1298	rBV	44233	67061	12.27%	1.663%
56	9.220	1332	1334	1335	rBV	121	117	0.02%	0.003%
57	9.263	1339	1341	1342	rVV	241	147	0.03%	0.004%
58	9.384	1356	1361	1379	rBV	163669	250199	45.76%	6.204%
59	9.695	1409	1412	1418	rVB3	1094	1899	0.35%	0.047%
60	9.750	1418	1421	1422	rBV	258	233	0.04%	0.006%
61	10.055	1465	1471	1483	rBV	318319	431236	78.87%	10.692%
62	10.275	1505	1507	1510	rVB2	161	134	0.02%	0.003%
63	10.305	1510	1512	1515	rBV	284	223	0.04%	0.006%
64	10.403	1527	1528	1531	rBV	214	198	0.04%	0.005%
65	10.451	1535	1536	1537	rBV	200	101	0.02%	0.003%
66	10.470	1537	1539	1545	rVB2	338	334	0.06%	0.008%
67	10.549	1551	1552	1557	rBV	265	238	0.04%	0.006%
68	10.665	1569	1571	1572	rBB	217	107	0.02%	0.003%
69	10.713	1578	1579	1581	rBV	242	179	0.03%	0.004%
70	10.768	1587	1588	1590	rBV	207	133	0.02%	0.003%
71	10.842	1596	1600	1601	rBV	211	202	0.04%	0.005%
72	11.024	1628	1630	1631	rBV	166	121	0.02%	0.003%
73	11.067	1635	1637	1639	rVB	204	130	0.02%	0.003%
74	11.189	1652	1657	1668	rBV	203259	269959	49.38%	6.694%
75	11.311	1674	1677	1679	rBV	169	166	0.03%	0.004%
76	11.445	1696	1699	1700	rBV	222	219	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042670.D
 Acq On : 28 Jul 2024 04:04
 Operator : JC/MD
 Sample : P3389-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.604	1723	1725	1730	rVB2	205	286	0.05%	0.007%
78	11.665	1733	1735	1737	rBV	299	297	0.05%	0.007%
79	11.817	1757	1760	1761	rBV	262	213	0.04%	0.005%
80	11.945	1777	1781	1784	rBV	320	500	0.09%	0.012%
81	12.024	1788	1794	1805	rBV	257903	344667	63.04%	8.546%
82	12.317	1837	1842	1850	rBV	260810	332716	60.85%	8.250%
83	12.786	1917	1919	1921	rBV	213	217	0.04%	0.005%
84	12.914	1938	1940	1941	rBV	254	139	0.03%	0.003%
85	12.975	1946	1950	1952	rBV	227	281	0.05%	0.007%
86	13.000	1952	1954	1958	rVB2	241	231	0.04%	0.006%
87	13.036	1958	1960	1962	rBV2	169	183	0.03%	0.005%
88	13.323	2006	2007	2012	rVB2	291	284	0.05%	0.007%
89	13.390	2016	2018	2021	rVB	310	273	0.05%	0.007%
90	13.420	2021	2023	2024	rBV	347	249	0.05%	0.006%
91	13.481	2030	2033	2035	rBV	281	313	0.06%	0.008%
92	13.536	2041	2042	2046	rBV2	157	188	0.03%	0.005%
93	13.695	2065	2068	2072	rBV2	246	395	0.07%	0.010%
94	13.737	2072	2075	2078	rVB	351	425	0.08%	0.011%
95	13.975	2113	2114	2116	rBV	187	151	0.03%	0.004%
96	14.213	2151	2153	2158	rBV2	167	303	0.06%	0.008%
97	14.774	2243	2245	2248	rBV2	428	503	0.09%	0.012%
98	15.024	2284	2286	2288	rBV	317	229	0.04%	0.006%
99	15.536	2368	2370	2371	rBV	608	389	0.07%	0.010%
100	16.597	2542	2544	2545	rBV	342	185	0.03%	0.005%

Sum of corrected areas: 4033072


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042670.D
Acq On : 28 Jul 2024 04:04
Operator : JC/MD
Sample : P3389-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

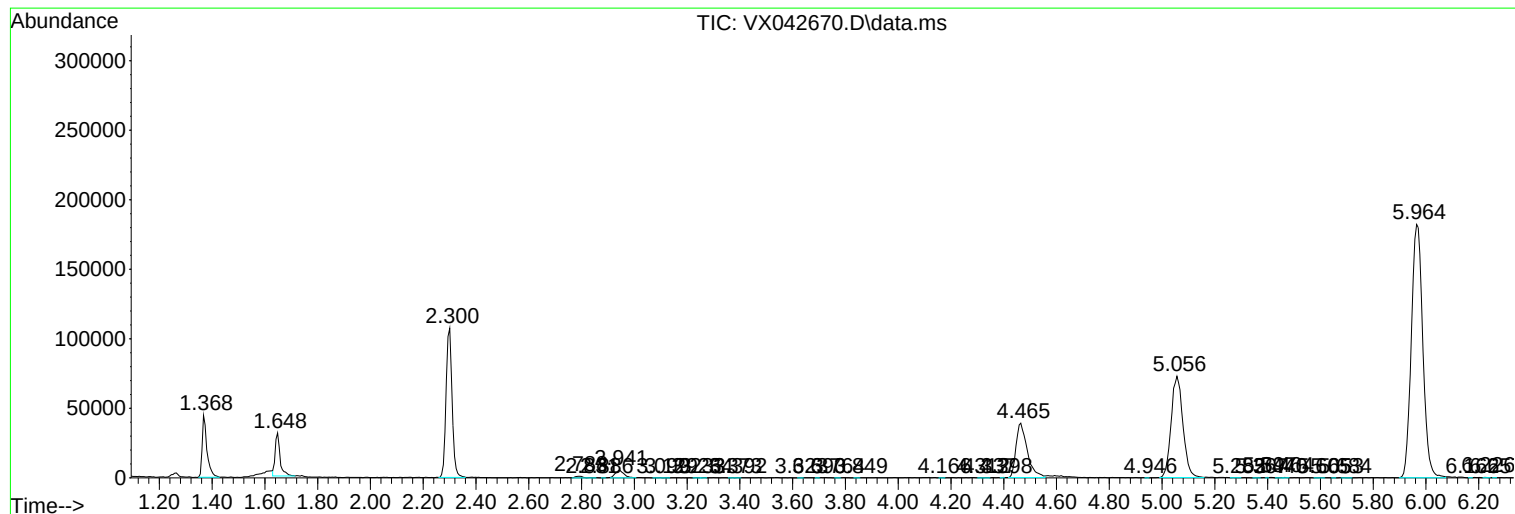

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042670.D
Acq On : 28 Jul 2024 04:04
Operator : JC/MD
Sample : P3389-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042670.D
Acq On : 28 Jul 2024 04:04
Operator : JC/MD
Sample : P3389-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------