

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042671.D
 Acq On : 28 Jul 2024 04:27
 Operator : JC/MD
 Sample : P3389-04 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	40798	55477	10.20%	1.374%
2	1.648	89	92	103	rVB	30920	39301	7.23%	0.974%
3	2.300	192	199	210	rVB	102832	166247	30.57%	4.119%
4	2.489	228	230	233	rBV	175	200	0.04%	0.005%
5	2.599	244	248	250	rBV3	281	491	0.09%	0.012%
6	2.703	262	265	267	rBB	205	228	0.04%	0.006%
7	2.788	273	279	285	rBB3	492	1171	0.22%	0.029%
8	2.831	285	286	289	rBV3	191	210	0.04%	0.005%
9	2.861	289	291	294	rVB	194	164	0.03%	0.004%
10	2.892	294	296	297	rBV	213	170	0.03%	0.004%
11	3.069	323	325	328	rBB	255	277	0.05%	0.007%
12	3.105	328	331	333	rBV	158	183	0.03%	0.005%
13	3.160	338	340	342	rVV	131	115	0.02%	0.003%
14	3.252	352	355	356	rBV	203	204	0.04%	0.005%
15	3.343	369	370	373	rBV	162	158	0.03%	0.004%
16	3.459	387	389	391	rBV	118	135	0.02%	0.003%
17	3.550	402	404	406	rBV	253	227	0.04%	0.006%
18	3.660	420	422	423	rBB	218	154	0.03%	0.004%
19	3.678	423	425	426	rBV	181	121	0.02%	0.003%
20	3.794	442	444	446	rBV	115	151	0.03%	0.004%
21	4.026	480	482	483	rBV	229	175	0.03%	0.004%
22	4.129	498	499	501	rBV	161	123	0.02%	0.003%
23	4.325	527	531	534	rBV2	156	192	0.04%	0.005%
24	4.465	546	554	573	rBV2	36548	114535	21.06%	2.837%
25	4.861	617	619	620	rVB	251	95	0.02%	0.002%
26	5.056	640	651	662	rBV2	73917	222186	40.86%	5.504%
27	5.239	679	681	684	rVB	241	240	0.04%	0.006%
28	5.269	684	686	690	rBV2	227	200	0.04%	0.005%
29	5.428	709	712	714	rBV	264	243	0.04%	0.006%
30	5.526	726	728	730	rBV	119	111	0.02%	0.003%
31	5.586	737	738	739	rBV	249	138	0.03%	0.003%
32	5.806	773	774	777	rBV	216	252	0.05%	0.006%
33	5.885	786	787	789	rBV	224	218	0.04%	0.005%
34	5.964	790	800	822	rVV2	182797	543833	100.00%	13.473%
35	6.336	859	861	863	rBV2	182	189	0.03%	0.005%
36	6.428	873	876	878	rVB	288	310	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042671.D
 Acq On : 28 Jul 2024 04:27
 Operator : JC/MD
 Sample : P3389-04 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.446	878	879	881	rBV	322	291	0.05%	0.007%
38	6.623	907	908	911	rBV	145	175	0.03%	0.004%
39	6.763	922	931	949	rBV	155201	379379	69.76%	9.399%
40	7.117	984	989	997	rBV4	1934	5108	0.94%	0.127%
41	7.306	1012	1020	1040	rBV	112864	246281	45.29%	6.101%
42	7.860	1110	1111	1113	rVB	291	131	0.02%	0.003%
43	7.885	1114	1115	1117	rBB	247	152	0.03%	0.004%
44	7.928	1118	1122	1126	rBV2	238	398	0.07%	0.010%
45	8.190	1163	1165	1166	rBV	214	118	0.02%	0.003%
46	8.220	1169	1170	1171	rBV	206	105	0.02%	0.003%
47	8.324	1181	1187	1200	rBV	60122	103399	19.01%	2.562%
48	8.531	1220	1221	1223	rBV	358	242	0.04%	0.006%
49	8.555	1223	1225	1227	rVB	285	201	0.04%	0.005%
50	8.592	1229	1231	1232	rBV	188	149	0.03%	0.004%
51	8.647	1234	1240	1252	rBV	269433	419395	77.12%	10.390%
52	8.952	1285	1290	1301	rBV	43393	65762	12.09%	1.629%
53	9.122	1316	1318	1325	rBV	274	583	0.11%	0.014%
54	9.250	1338	1339	1341	rBV	364	212	0.04%	0.005%
55	9.385	1356	1361	1378	rBV	160900	249171	45.82%	6.173%
56	9.702	1411	1413	1414	rBV	414	199	0.04%	0.005%
57	9.915	1446	1448	1451	rBB	201	232	0.04%	0.006%
58	9.939	1451	1452	1456	rBV	229	249	0.05%	0.006%
59	9.982	1456	1459	1461	rBV	156	183	0.03%	0.005%
60	10.055	1465	1471	1487	rVV	311814	440382	80.98%	10.910%
61	10.323	1514	1515	1517	rVB	238	107	0.02%	0.003%
62	10.543	1549	1551	1552	rBV	168	174	0.03%	0.004%
63	10.964	1618	1620	1624	rVB	280	318	0.06%	0.008%
64	11.006	1624	1627	1628	rBV	255	278	0.05%	0.007%
65	11.067	1635	1637	1639	rBV	153	129	0.02%	0.003%
66	11.189	1652	1657	1665	rBV	214476	274278	50.43%	6.795%
67	11.342	1680	1682	1685	rVB	262	266	0.05%	0.007%
68	11.384	1686	1689	1690	rBV	200	200	0.04%	0.005%
69	11.427	1694	1696	1700	rBV2	202	286	0.05%	0.007%
70	11.531	1710	1713	1715	rBV	150	152	0.03%	0.004%
71	11.579	1719	1721	1722	rBV	270	161	0.03%	0.004%
72	11.762	1748	1751	1752	rBV	232	224	0.04%	0.006%
73	11.854	1762	1766	1768	rBV2	172	288	0.05%	0.007%
74	11.909	1773	1775	1776	rBV	203	190	0.03%	0.005%
75	11.976	1784	1786	1788	rBV	204	242	0.04%	0.006%
76	12.018	1788	1793	1804	rBV	276589	353928	65.08%	8.768%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042671.D
 Acq On : 28 Jul 2024 04:27
 Operator : JC/MD
 Sample : P3389-04 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1852	rBV	258294	338828	62.30%	8.394%
78	12.445	1861	1863	1865	rVB2	263	174	0.03%	0.004%
79	12.494	1869	1871	1874	rBB2	292	256	0.05%	0.006%
80	12.536	1874	1878	1881	rBV2	229	440	0.08%	0.011%
81	12.591	1886	1887	1890	rBV2	209	208	0.04%	0.005%
82	12.774	1915	1917	1919	rBV	187	161	0.03%	0.004%
83	12.817	1923	1924	1926	rBV	196	170	0.03%	0.004%
84	13.140	1976	1977	1980	rBV	219	256	0.05%	0.006%
85	13.244	1993	1994	1995	rBV	173	103	0.02%	0.003%
86	13.323	2005	2007	2009	rBV	199	228	0.04%	0.006%
87	13.530	2040	2041	2043	rBV	229	163	0.03%	0.004%
88	13.609	2052	2054	2055	rBV	171	148	0.03%	0.004%
89	13.914	2100	2104	2107	rBV2	267	510	0.09%	0.013%
90	14.018	2120	2121	2124	rBV	220	147	0.03%	0.004%
91	14.128	2138	2139	2143	rVB2	392	331	0.06%	0.008%
92	14.329	2171	2172	2174	rBV2	224	202	0.04%	0.005%
93	14.451	2189	2192	2193	rBV	231	280	0.05%	0.007%
94	14.469	2193	2195	2196	rVV	185	102	0.02%	0.003%
95	14.536	2204	2206	2207	rBV	153	143	0.03%	0.004%
96	14.579	2212	2213	2215	rVV	264	164	0.03%	0.004%
97	14.920	2268	2269	2273	rBV2	274	203	0.04%	0.005%
98	15.030	2283	2287	2289	rBV3	383	595	0.11%	0.015%
99	15.316	2332	2334	2336	rBV3	247	215	0.04%	0.005%
100	16.158	2470	2472	2474	rBV	485	376	0.07%	0.009%


Sum of corrected areas: 4036545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042671.D
Acq On : 28 Jul 2024 04:27
Operator : JC/MD
Sample : P3389-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

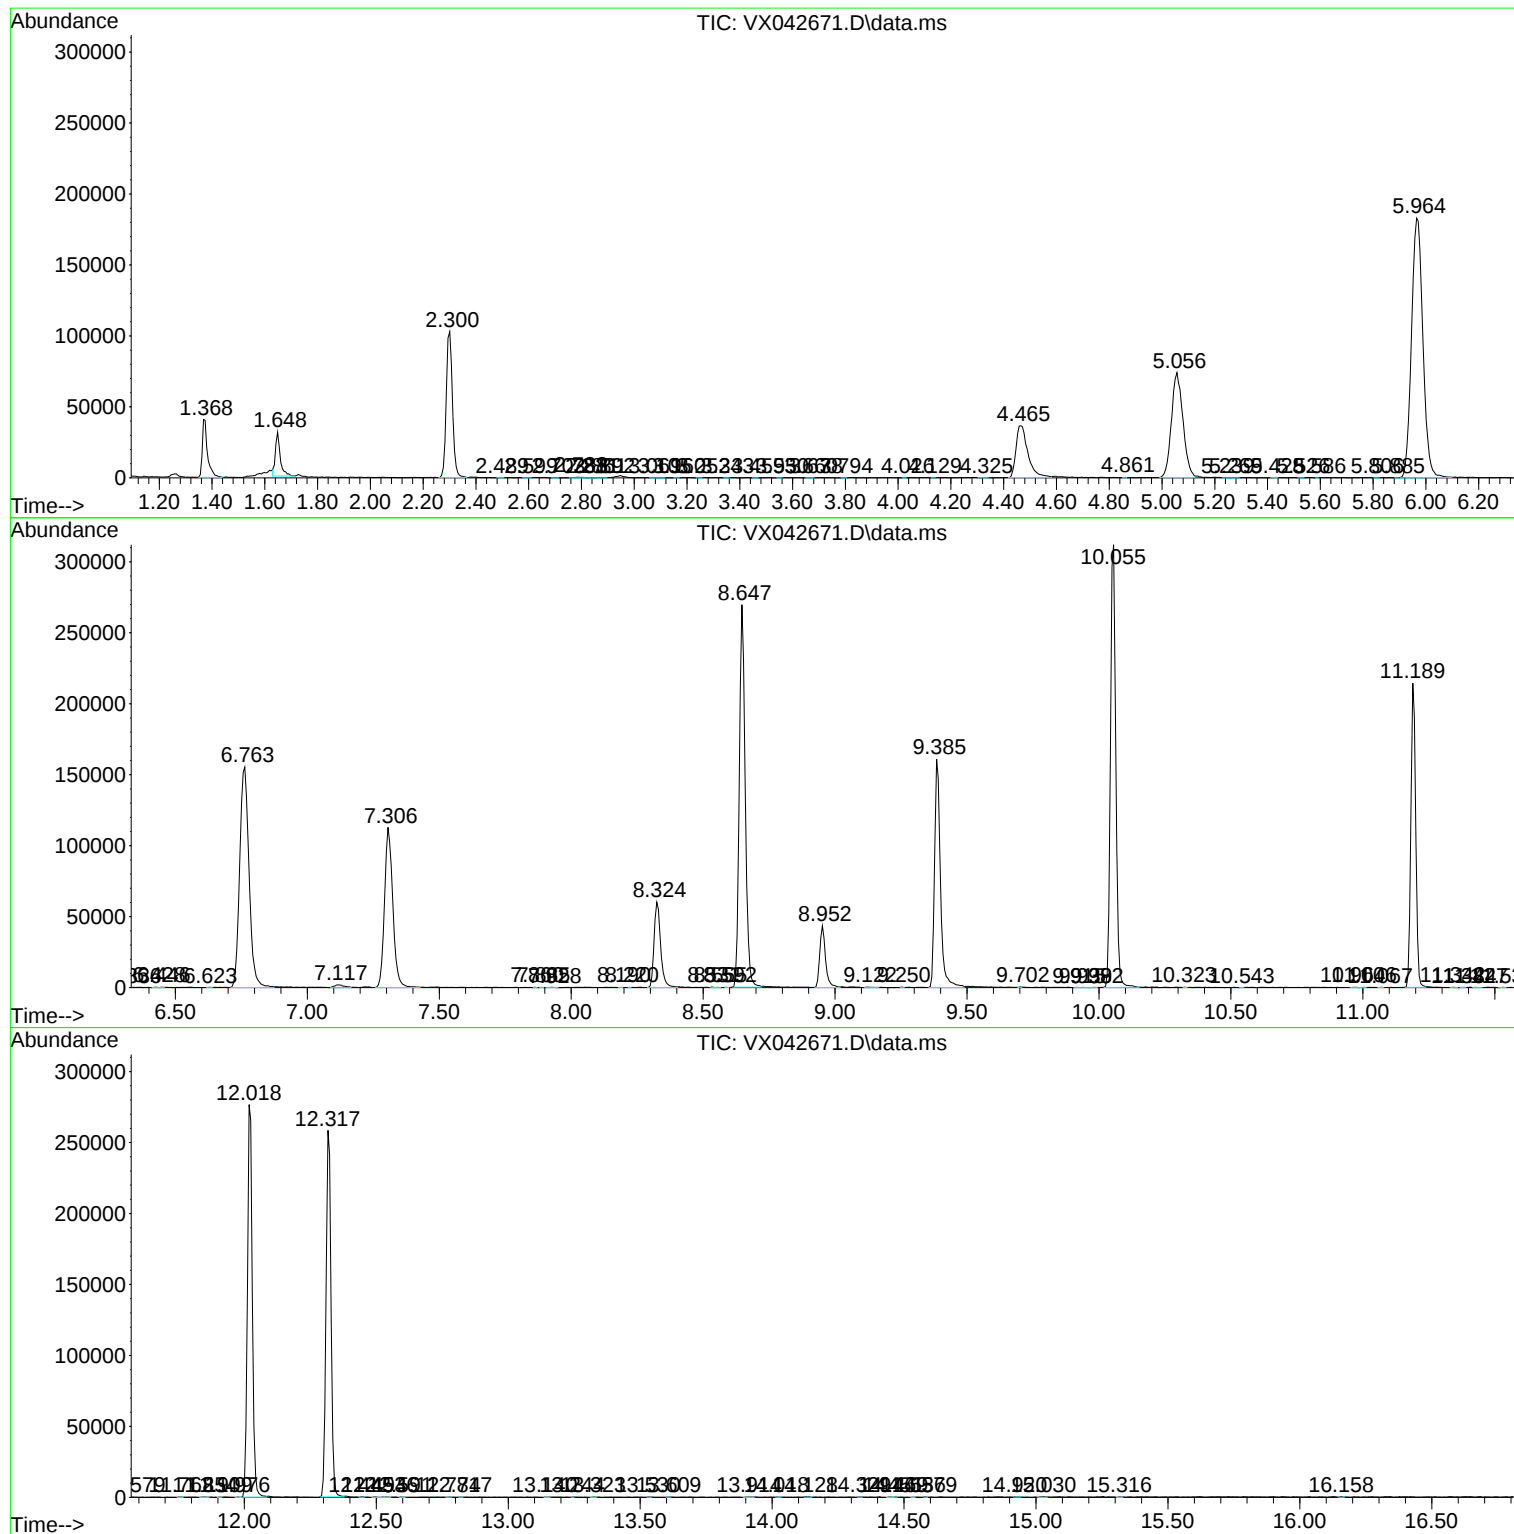

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042671.D
Acq On : 28 Jul 2024 04:27
Operator : JC/MD
Sample : P3389-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042671.D
Acq On : 28 Jul 2024 04:27
Operator : JC/MD
Sample : P3389-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------