

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042672.D
 Acq On : 28 Jul 2024 04:50
 Operator : JC/MD
 Sample : P3389-05 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	28	rBV2	2112	2419	0.42%	0.057%
2	1.367	43	46	58	rVB	51017	63415	10.91%	1.483%
3	1.648	89	92	102	rVB	35903	46634	8.02%	1.090%
4	2.105	166	167	170	rBV2	340	260	0.04%	0.006%
5	2.300	193	199	210	rVB	117790	186360	32.05%	4.357%
6	2.648	253	256	257	rBV	210	207	0.04%	0.005%
7	2.715	266	267	270	rVV	303	185	0.03%	0.004%
8	2.788	274	279	284	rVB4	802	1281	0.22%	0.030%
9	2.946	297	305	312	rBV	5517	11594	1.99%	0.271%
10	3.154	338	339	342	rBB	194	153	0.03%	0.004%
11	3.318	365	366	368	rVB	256	142	0.02%	0.003%
12	3.337	368	369	371	rBV	237	237	0.04%	0.006%
13	3.404	377	380	382	rBV	218	245	0.04%	0.006%
14	3.483	390	393	394	rBV	128	157	0.03%	0.004%
15	3.556	402	405	407	rVB2	211	228	0.04%	0.005%
16	3.611	412	414	417	rBB	187	176	0.03%	0.004%
17	3.660	420	422	424	rBV	164	166	0.03%	0.004%
18	3.745	434	436	437	rBV	189	161	0.03%	0.004%
19	3.763	437	439	442	rVB	234	219	0.04%	0.005%
20	3.873	455	457	459	rBB	245	175	0.03%	0.004%
21	3.904	459	462	463	rBB	174	170	0.03%	0.004%
22	3.922	463	465	468	rBV	197	241	0.04%	0.006%
23	4.129	498	499	501	rBV	217	184	0.03%	0.004%
24	4.208	510	512	514	rBV	191	169	0.03%	0.004%
25	4.343	531	534	535	rBV	223	221	0.04%	0.005%
26	4.464	546	554	569	rBV	40987	123129	21.18%	2.879%
27	4.855	616	618	624	rVB2	278	327	0.06%	0.008%
28	5.050	640	650	668	rBV	77022	240964	41.45%	5.634%
29	5.446	713	715	717	rBV	307	248	0.04%	0.006%
30	5.672	749	752	754	rBV	154	189	0.03%	0.004%
31	5.739	760	763	765	rBV	308	349	0.06%	0.008%
32	5.964	789	800	815	rBV2	196443	581406	100.00%	13.594%
33	6.226	840	843	844	rBV	206	233	0.04%	0.005%
34	6.598	902	904	905	rVB	252	152	0.03%	0.004%
35	6.617	905	907	908	rBV	166	141	0.02%	0.003%
36	6.763	922	931	943	rBV	163604	393337	67.65%	9.197%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042672.D
 Acq On : 28 Jul 2024 04:50
 Operator : JC/MD
 Sample : P3389-05 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.043	975	977	978	rVB	321	207	0.04%	0.005%
38	7.123	984	990	996	rVB3	1776	3830	0.66%	0.090%
39	7.202	1000	1003	1004	rBV	340	262	0.05%	0.006%
40	7.305	1012	1020	1034	rBV	115746	257554	44.30%	6.022%
41	7.677	1079	1081	1082	rBV	273	198	0.03%	0.005%
42	7.811	1102	1103	1106	rBV2	186	219	0.04%	0.005%
43	7.842	1106	1108	1111	rVB	232	236	0.04%	0.006%
44	8.043	1140	1141	1143	rBV	207	162	0.03%	0.004%
45	8.177	1162	1163	1165	rBV	249	212	0.04%	0.005%
46	8.250	1173	1175	1176	rBV	322	153	0.03%	0.004%
47	8.324	1182	1187	1197	rBV	64778	108254	18.62%	2.531%
48	8.500	1214	1216	1217	rBV	233	170	0.03%	0.004%
49	8.519	1217	1219	1223	rVV2	207	217	0.04%	0.005%
50	8.580	1225	1229	1231	rBV	330	506	0.09%	0.012%
51	8.647	1234	1240	1257	rBV	290809	451173	77.60%	10.549%
52	8.872	1273	1277	1278	rBV	325	398	0.07%	0.009%
53	8.951	1285	1290	1303	rBV	46586	71084	12.23%	1.662%
54	9.134	1319	1320	1322	rBV	285	225	0.04%	0.005%
55	9.293	1344	1346	1348	rBV	167	174	0.03%	0.004%
56	9.384	1356	1361	1375	rBV	177972	264418	45.48%	6.182%
57	9.518	1382	1383	1386	rBV3	884	581	0.10%	0.014%
58	9.817	1428	1432	1434	rBV	271	384	0.07%	0.009%
59	10.000	1458	1462	1463	rBV2	180	176	0.03%	0.004%
60	10.055	1465	1471	1484	rVV	319700	450886	77.55%	10.542%
61	10.213	1494	1497	1499	rBV	294	355	0.06%	0.008%
62	10.409	1527	1529	1532	rBV2	261	307	0.05%	0.007%
63	10.476	1539	1540	1544	rBV	186	142	0.02%	0.003%
64	10.640	1565	1567	1568	rBV	227	148	0.03%	0.003%
65	10.695	1574	1576	1578	rVB	239	171	0.03%	0.004%
66	10.719	1578	1580	1584	rBV2	227	353	0.06%	0.008%
67	10.762	1584	1587	1591	rVB2	295	405	0.07%	0.009%
68	11.018	1625	1629	1631	rBV2	222	312	0.05%	0.007%
69	11.043	1631	1633	1634	rBV	312	171	0.03%	0.004%
70	11.189	1652	1657	1671	rBV	221927	286395	49.26%	6.696%
71	11.494	1705	1707	1709	rBV	226	179	0.03%	0.004%
72	11.652	1731	1733	1734	rBV	229	180	0.03%	0.004%
73	11.866	1765	1768	1772	rBV2	266	351	0.06%	0.008%
74	11.981	1784	1787	1788	rBV	264	307	0.05%	0.007%
75	12.018	1788	1793	1805	rVV	272147	359524	61.84%	8.406%
76	12.317	1837	1842	1850	rBV	270886	353524	60.81%	8.266%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042672.D
 Acq On : 28 Jul 2024 04:50
 Operator : JC/MD
 Sample : P3389-05 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.439	1861	1862	1867	rBV2	340	517	0.09%	0.012%
78	12.762	1913	1915	1918	rBV2	354	348	0.06%	0.008%
79	12.926	1941	1942	1945	rBV2	300	259	0.04%	0.006%
80	12.975	1948	1950	1952	rBV2	261	270	0.05%	0.006%
81	13.164	1980	1981	1982	rBV2	232	154	0.03%	0.004%
82	13.231	1990	1992	1995	rBV	288	294	0.05%	0.007%
83	13.280	1999	2000	2003	rBV	169	135	0.02%	0.003%
84	13.341	2008	2010	2012	rBV	197	176	0.03%	0.004%
85	13.652	2059	2061	2063	rBV	322	266	0.05%	0.006%
86	13.823	2085	2089	2092	rVB2	226	270	0.05%	0.006%
87	13.890	2099	2100	2102	rBV2	159	152	0.03%	0.004%
88	13.938	2106	2108	2110	rBV	263	278	0.05%	0.006%
89	14.164	2144	2145	2146	rBV	189	137	0.02%	0.003%
90	14.219	2151	2154	2156	rBV	230	285	0.05%	0.007%
91	14.237	2156	2157	2160	rBV	188	176	0.03%	0.004%
92	14.298	2165	2167	2169	rBV	130	142	0.02%	0.003%
93	14.499	2197	2200	2201	rBV2	228	297	0.05%	0.007%
94	14.652	2224	2225	2228	rBV2	346	296	0.05%	0.007%
95	14.707	2231	2234	2236	rBV2	231	288	0.05%	0.007%
96	15.048	2288	2290	2293	rBV3	278	294	0.05%	0.007%
97	15.121	2301	2302	2303	rBV3	229	130	0.02%	0.003%
98	15.389	2342	2346	2347	rBV2	727	784	0.13%	0.018%
99	15.584	2377	2378	2380	rBV	299	161	0.03%	0.004%
100	16.072	2456	2458	2463	rBV2	274	516	0.09%	0.012%




Sum of corrected areas: 4277002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042672.D
Acq On : 28 Jul 2024 04:50
Operator : JC/MD
Sample : P3389-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

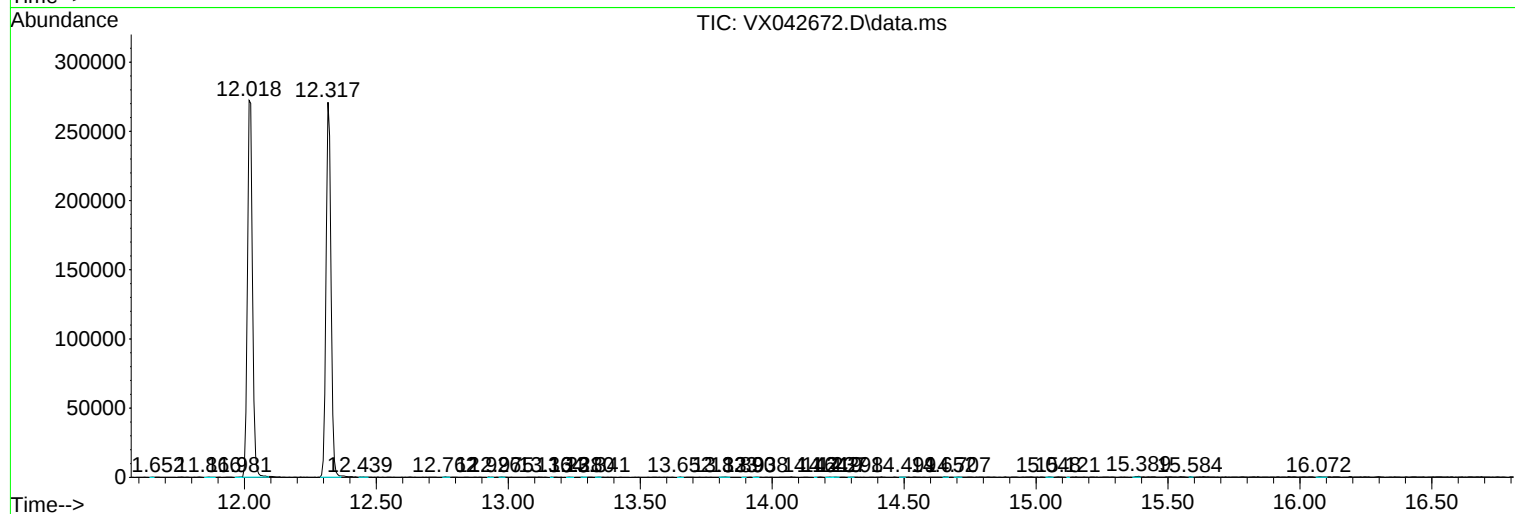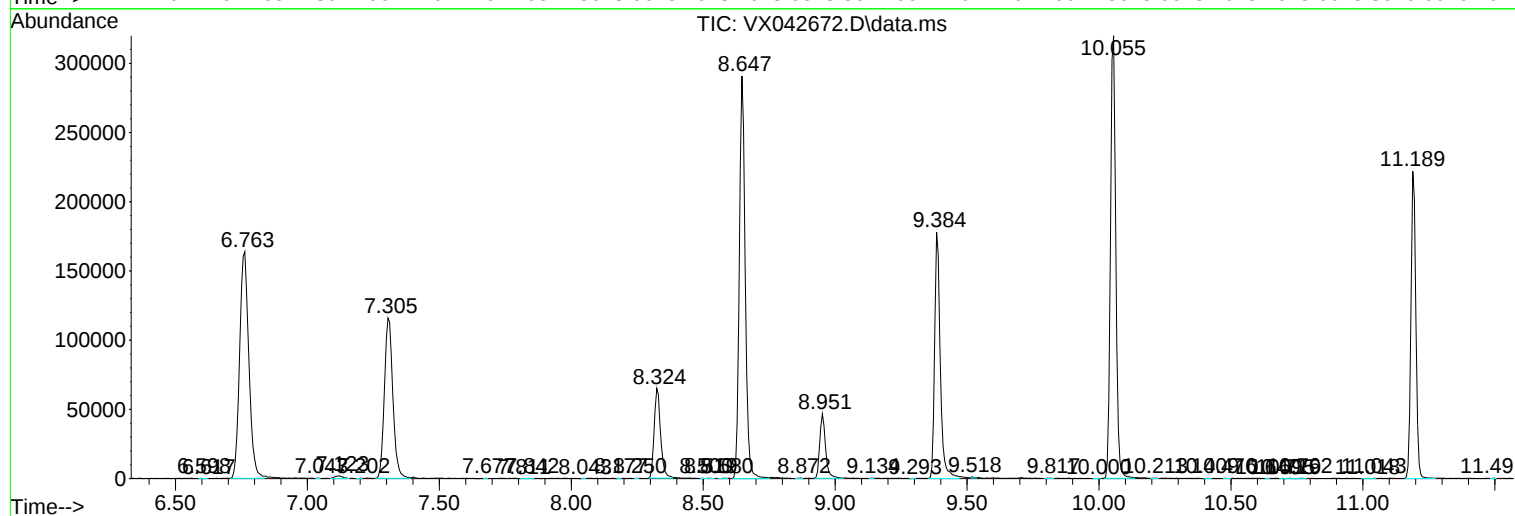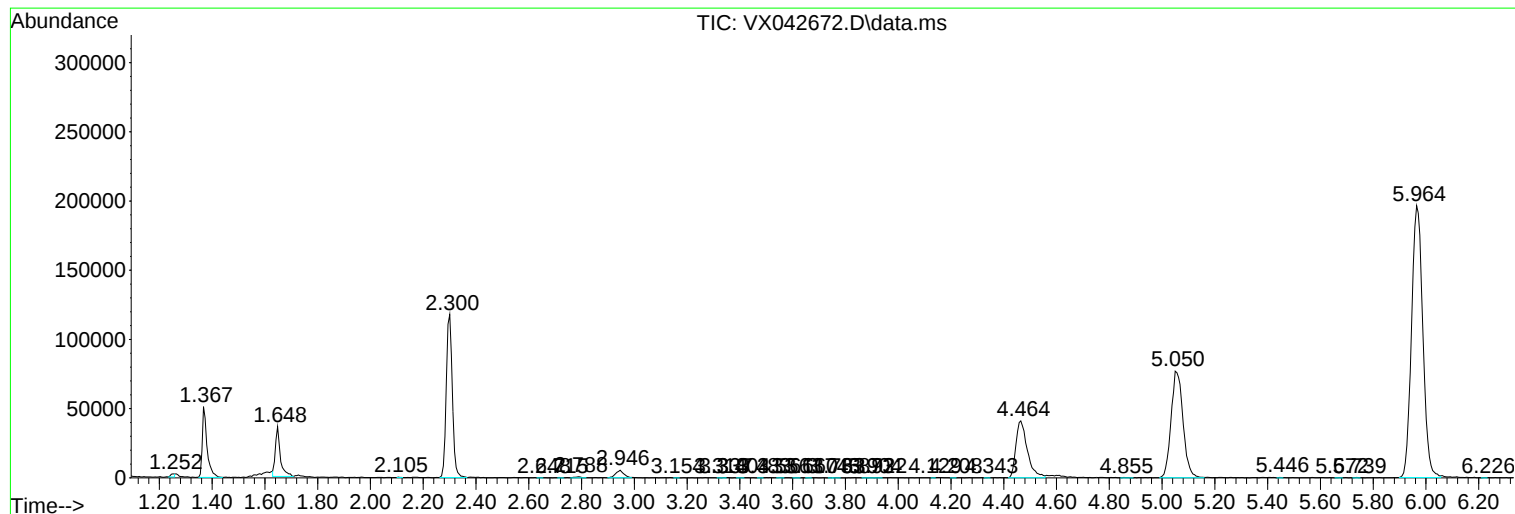

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042672.D
Acq On : 28 Jul 2024 04:50
Operator : JC/MD
Sample : P3389-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042672.D
Acq On : 28 Jul 2024 04:50
Operator : JC/MD
Sample : P3389-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc