

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042673.D
 Acq On : 28 Jul 2024 05:13
 Operator : JC/MD
 Sample : P3389-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	62	rVB	48073	63521	11.14%	1.506%
2	1.648	89	92	104	rVB	32847	42727	7.49%	1.013%
3	2.300	193	199	210	rVB	117615	183708	32.20%	4.355%
4	2.508	231	233	236	rBV	208	229	0.04%	0.005%
5	2.654	256	257	261	rBV2	220	271	0.05%	0.006%
6	2.794	272	280	285	rVB4	926	1884	0.33%	0.045%
7	2.886	291	295	296	rBV	243	300	0.05%	0.007%
8	2.946	297	305	315	rVV	4720	10813	1.90%	0.256%
9	3.111	330	332	335	rBV	209	225	0.04%	0.005%
10	3.166	340	341	344	rVB	172	166	0.03%	0.004%
11	3.196	344	346	347	rBV	193	169	0.03%	0.004%
12	3.239	350	353	354	rBV	239	240	0.04%	0.006%
13	3.355	369	372	374	rVB	249	241	0.04%	0.006%
14	3.550	401	404	406	rBV	136	203	0.04%	0.005%
15	3.574	406	408	411	rVV	285	282	0.05%	0.007%
16	3.769	436	440	442	rBB	191	263	0.05%	0.006%
17	3.806	443	446	449	rBV	136	210	0.04%	0.005%
18	3.928	463	466	468	rBB	187	165	0.03%	0.004%
19	4.074	486	490	493	rBV2	169	259	0.05%	0.006%
20	4.464	545	554	568	rBV	40364	121531	21.30%	2.881%
21	4.739	597	599	600	rVB2	312	155	0.03%	0.004%
22	4.836	614	615	618	rVB	145	147	0.03%	0.003%
23	4.891	621	624	625	rBV2	269	328	0.06%	0.008%
24	5.056	639	651	667	rVV	75584	232494	40.76%	5.512%
25	5.288	688	689	692	rBV2	198	262	0.05%	0.006%
26	5.342	696	698	699	rBV	196	141	0.02%	0.003%
27	5.659	748	750	751	rBV	258	143	0.03%	0.003%
28	5.806	771	774	775	rBV	218	244	0.04%	0.006%
29	5.964	789	800	815	rBV2	193022	570445	100.00%	13.523%
30	6.421	873	875	878	rVB2	239	195	0.03%	0.005%
31	6.452	878	880	881	rBV	181	187	0.03%	0.004%
32	6.574	899	900	902	rBV	228	184	0.03%	0.004%
33	6.757	921	930	945	rBV	161020	394487	69.15%	9.352%
34	7.013	970	972	975	rBV	274	302	0.05%	0.007%
35	7.110	982	988	997	rBV6	2049	4659	0.82%	0.110%
36	7.177	997	999	1002	rBV	245	195	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042673.D
 Acq On : 28 Jul 2024 05:13
 Operator : JC/MD
 Sample : P3389-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.208	1002	1004	1012	rBV3	327	717	0.13%	0.017%
38	7.305	1012	1020	1031	rBV	115647	258390	45.30%	6.126%
39	7.574	1063	1064	1066	rBV2	190	163	0.03%	0.004%
40	7.696	1082	1084	1086	rVB	225	187	0.03%	0.004%
41	7.720	1086	1088	1090	rBV	227	261	0.05%	0.006%
42	7.787	1097	1099	1100	rBV	252	188	0.03%	0.004%
43	8.019	1135	1137	1139	rBV	227	203	0.04%	0.005%
44	8.324	1181	1187	1198	rBV	64387	107118	18.78%	2.539%
45	8.543	1221	1223	1225	rVB2	310	190	0.03%	0.005%
46	8.647	1234	1240	1254	rBV	276721	438839	76.93%	10.403%
47	8.951	1285	1290	1304	rBV	45546	70455	12.35%	1.670%
48	9.250	1335	1339	1341	rBV2	180	292	0.05%	0.007%
49	9.384	1356	1361	1374	rBV	169216	257131	45.08%	6.096%
50	9.860	1435	1439	1441	rBV	362	425	0.07%	0.010%
51	9.890	1441	1444	1446	rVV2	217	292	0.05%	0.007%
52	9.939	1449	1452	1456	rVB2	322	429	0.08%	0.010%
53	9.970	1456	1457	1458	rBV2	238	141	0.02%	0.003%
54	10.055	1465	1471	1483	rBV	324969	448614	78.64%	10.635%
55	10.274	1505	1507	1509	rBV	216	227	0.04%	0.005%
56	10.598	1557	1560	1561	rBV	183	184	0.03%	0.004%
57	10.738	1579	1583	1587	rBB	212	362	0.06%	0.009%
58	10.774	1587	1589	1593	rBV	221	391	0.07%	0.009%
59	10.835	1598	1599	1606	rVB	302	452	0.08%	0.011%
60	10.890	1606	1608	1609	rBV	180	164	0.03%	0.004%
61	10.988	1623	1624	1626	rBV	212	199	0.03%	0.005%
62	11.067	1633	1637	1638	rBV	268	305	0.05%	0.007%
63	11.128	1645	1647	1648	rBV	255	248	0.04%	0.006%
64	11.189	1652	1657	1664	rBV	208694	279538	49.00%	6.627%
65	11.299	1673	1675	1676	rBV	256	234	0.04%	0.006%
66	11.341	1680	1682	1684	rVV	235	245	0.04%	0.006%
67	11.390	1688	1690	1693	rVB	278	228	0.04%	0.005%
68	11.622	1726	1728	1729	rBV	128	139	0.02%	0.003%
69	11.713	1741	1743	1746	rBV	217	218	0.04%	0.005%
70	11.738	1746	1747	1749	rVB	287	137	0.02%	0.003%
71	11.756	1749	1750	1752	rBV	202	154	0.03%	0.004%
72	11.841	1760	1764	1765	rBV	194	212	0.04%	0.005%
73	12.018	1788	1793	1806	rVV	275144	360535	63.20%	8.547%
74	12.317	1837	1842	1853	rBV	279016	350952	61.52%	8.320%
75	12.439	1860	1862	1865	rVB	422	246	0.04%	0.006%
76	12.615	1888	1891	1893	rBV	214	230	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
 Data File : VX042673.D
 Acq On : 28 Jul 2024 05:13
 Operator : JC/MD
 Sample : P3389-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.670	1898	1900	1905	rBB	314	450	0.08%	0.011%
78	12.719	1905	1908	1909	rBV	248	277	0.05%	0.007%
79	12.786	1918	1919	1920	rBV	266	141	0.02%	0.003%
80	12.829	1924	1926	1929	rBV	228	331	0.06%	0.008%
81	12.981	1949	1951	1953	rBV2	246	238	0.04%	0.006%
82	13.073	1962	1966	1967	rBV2	169	211	0.04%	0.005%
83	13.176	1982	1983	1986	rBV	232	200	0.04%	0.005%
84	13.341	2008	2010	2012	rVV	240	208	0.04%	0.005%
85	13.365	2012	2014	2019	rVV2	307	435	0.08%	0.010%
86	13.420	2019	2023	2024	rVV2	198	177	0.03%	0.004%
87	13.603	2050	2053	2056	rVB	404	466	0.08%	0.011%
88	13.646	2056	2060	2061	rBV	237	268	0.05%	0.006%
89	13.902	2100	2102	2106	rVB2	382	469	0.08%	0.011%
90	13.932	2106	2107	2109	rBV2	352	266	0.05%	0.006%
91	13.975	2113	2114	2116	rBV	225	228	0.04%	0.005%
92	14.237	2154	2157	2158	rBV2	272	282	0.05%	0.007%
93	14.249	2158	2159	2162	rVB	389	272	0.05%	0.006%
94	14.316	2169	2170	2173	rVB	362	240	0.04%	0.006%
95	14.390	2180	2182	2184	rBB	186	147	0.03%	0.003%
96	14.414	2184	2186	2187	rBV	286	184	0.03%	0.004%
97	14.633	2221	2222	2224	rBV	187	155	0.03%	0.004%
98	14.743	2238	2240	2241	rBV	338	258	0.05%	0.006%
99	15.371	2341	2343	2344	rBV	370	376	0.07%	0.009%
100	16.499	2527	2528	2531	rBV	331	371	0.07%	0.009%

Sum of corrected areas: 4218260




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042673.D
Acq On : 28 Jul 2024 05:13
Operator : JC/MD
Sample : P3389-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

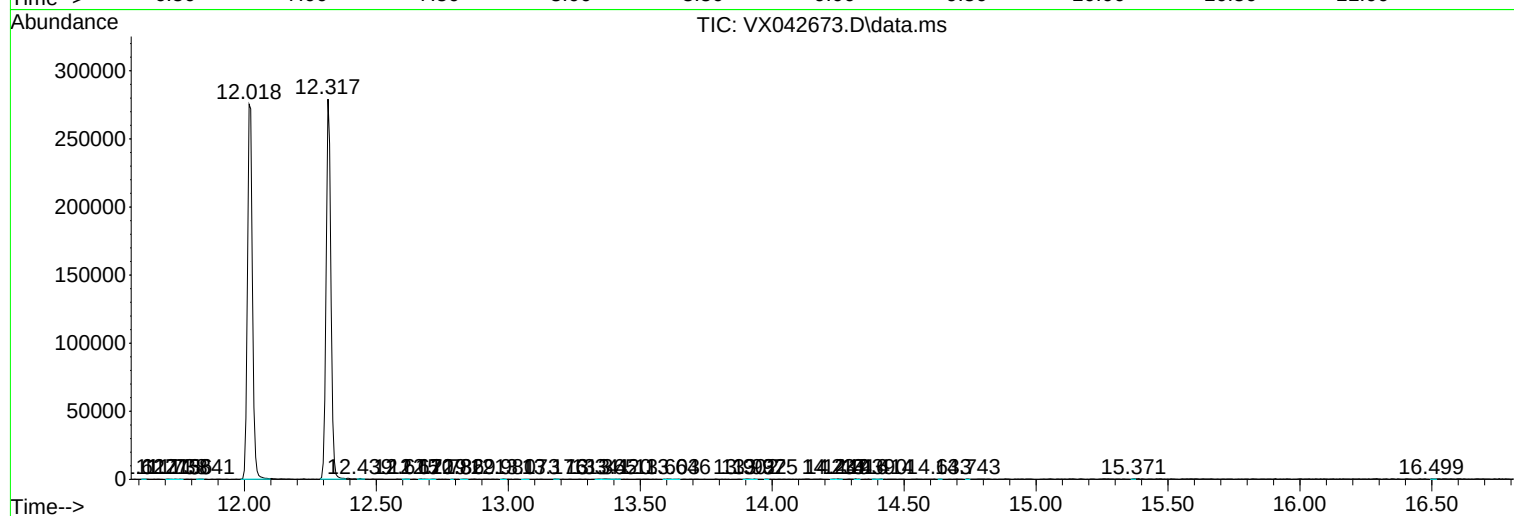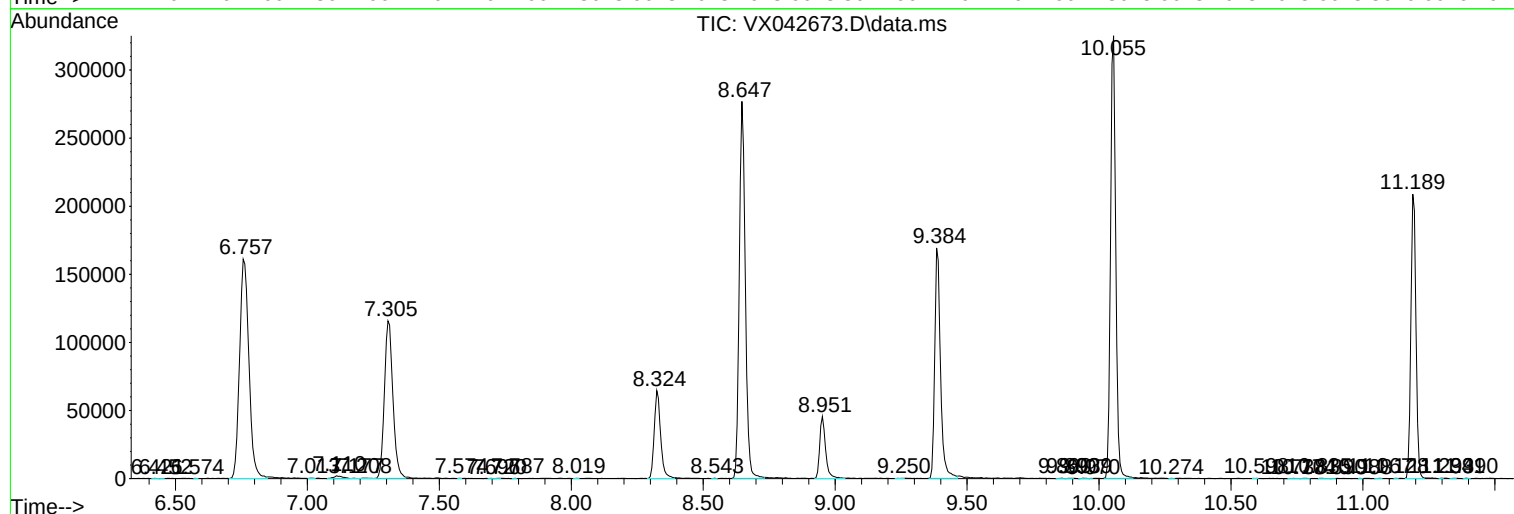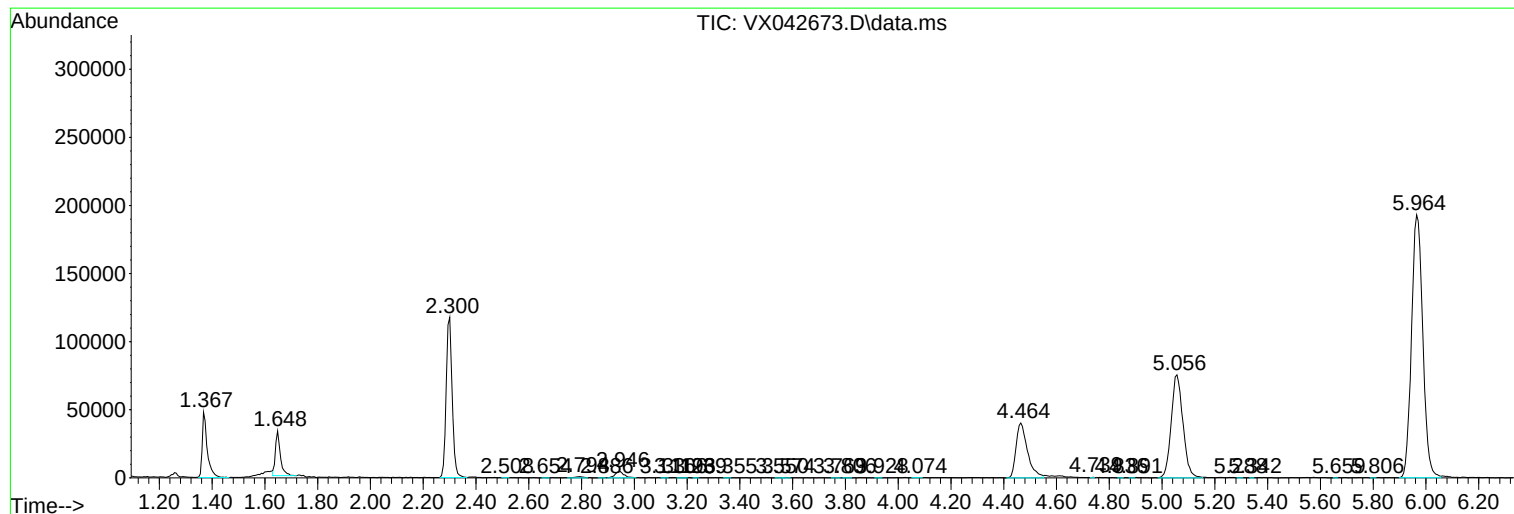

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042673.D
Acq On : 28 Jul 2024 05:13
Operator : JC/MD
Sample : P3389-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042673.D
Acq On : 28 Jul 2024 05:13
Operator : JC/MD
Sample : P3389-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------