
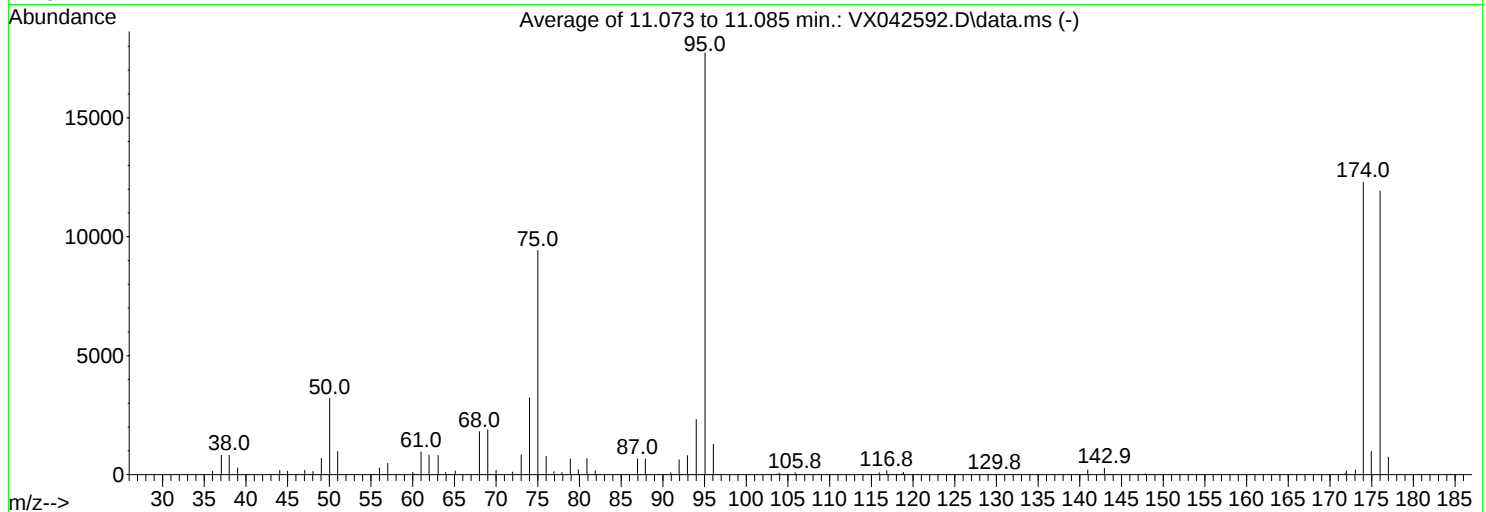


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072824\
Data File : VX042592.D
Acq On : 26 Jul 2024 10:10
Operator : JC/MD
Sample : BFB686
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB686

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM072624WMA.M
Title : VOC Analysis
Last Update : Mon Jul 29 03:03:42 2024

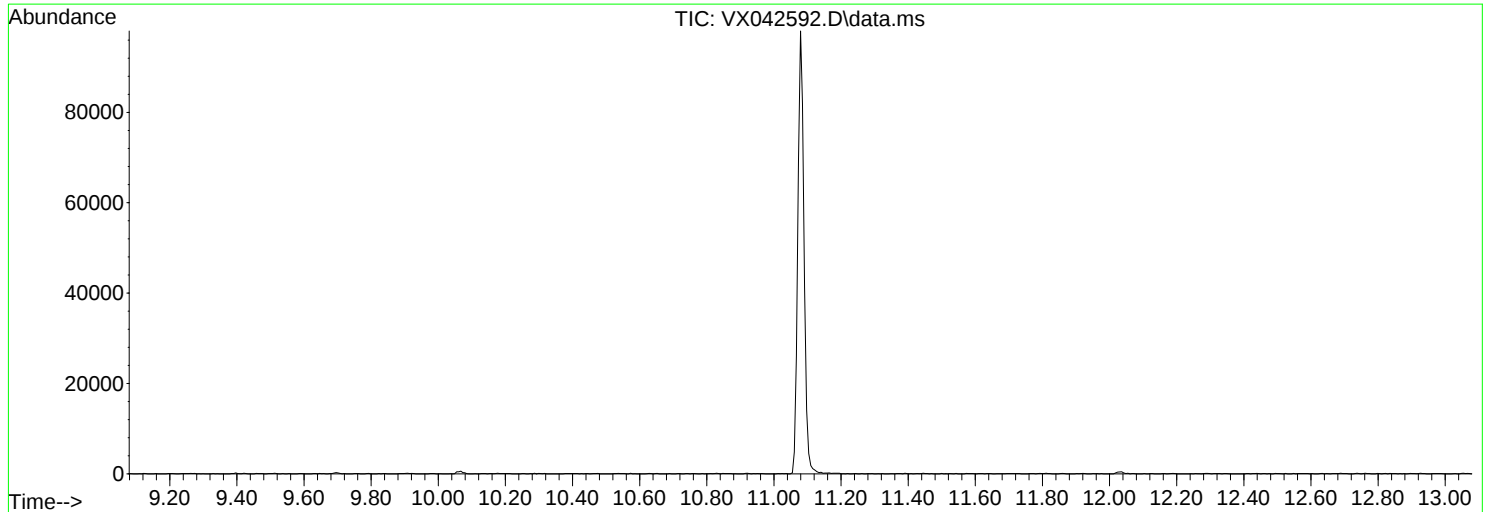

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	3203	PASS
75	95	30	80	53.1	9419	PASS
95	95	100	100	100.0	17729	PASS
96	95	5	9	7.2	1276	PASS
173	174	0.00	2	1.6	195	PASS
174	95	50	120	69.4	12297	PASS
175	174	5	9	7.9	975	PASS
176	174	95	101	97.0	11923	PASS
177	176	5	9	6.1	732	PASS

m/z

Abundance

Instrument :
MSVOA_X
ClientSampleId :
BFB686

m/z	Abundance
36.10	190.0
37.00	760.0
38.00	867.0
39.10	265.0
44.00	198.0
45.00	136.0
47.00	201.0
48.00	106.0
49.10	503.0
50.10	2938.0
51.00	820.0
56.00	234.0
57.00	438.0
60.00	167.0
61.00	861.0
62.00	777.0
63.00	734.0
64.00	90.0
65.10	115.0
68.00	1569.0
69.00	1719.0
70.10	127.0
71.90	100.0
73.00	652.0
74.00	2889.0
75.00	8573.0
76.00	689.0
77.00	116.0
78.00	81.0
78.90	589.0
79.90	153.0
80.90	575.0
82.00	155.0
86.90	530.0
87.90	443.0
91.10	55.0
92.00	514.0
93.00	654.0
94.00	1890.0
95.00	15338.0
96.00	1210.0
116.00	70.0
116.80	116.0
118.00	51.0
118.70	104.0
140.90	121.0
142.90	179.0
147.90	51.0
171.80	128.0
173.00	170.0
174.00	9273.0
174.90	661.0
176.00	8621.0
177.00	580.0

Instrument :
MSVOA_X
ClientSampleId :
BFB686

m/z	Abundance
35.90	167.0
37.10	968.0
38.00	871.0
38.90	327.0
40.10	59.0
44.10	223.0
45.10	145.0
47.10	200.0
48.00	159.0
49.00	935.0
50.00	3773.0
51.00	1304.0
56.10	358.0
57.00	521.0
60.00	145.0
61.10	1157.0
61.90	909.0
63.00	972.0
64.00	92.0
65.10	219.0
68.00	2288.0
69.00	2362.0
69.90	194.0
72.00	115.0
73.00	1052.0
74.00	3728.0
75.00	10707.0
76.00	966.0
76.90	117.0
77.90	87.0
78.90	820.0
79.90	208.0
80.90	774.0
81.90	218.0
86.90	859.0
87.90	877.0
90.90	92.0
92.00	699.0
93.00	1011.0
94.00	2879.0
95.10	20720.0
96.00	1507.0
103.70	83.0
104.00	97.0
104.90	54.0
105.90	123.0
115.90	101.0
116.90	246.0
118.90	186.0
129.80	52.0
141.00	203.0
143.00	276.0
147.90	62.0
172.00	299.0
173.00	219.0
174.00	14084.0
175.00	1139.0
176.00	14213.0
177.00	779.0

Instrument :
MSVOA_X
ClientSampleId :
BFB686

m/z	Abundance
36.00	87.0
37.00	706.0
38.00	701.0
39.00	253.0
44.10	110.0
44.90	156.0
47.00	142.0
48.10	141.0
49.00	618.0
50.00	2897.0
51.00	789.0
55.90	250.0
57.00	471.0
60.20	71.0
60.90	854.0
62.00	783.0
63.10	689.0
63.90	108.0
65.10	128.0
68.00	1565.0
69.00	1588.0
70.00	240.0
72.00	102.0
73.00	795.0
74.00	3056.0
75.00	8976.0
76.00	646.0
76.90	126.0
77.80	96.0
78.90	567.0
79.80	254.0
80.90	676.0
81.80	105.0
87.00	617.0
87.90	657.0
90.90	92.0
91.90	669.0
92.90	745.0
94.00	2167.0
95.00	17128.0
96.10	1111.0
103.90	107.0
105.80	112.0
115.90	76.0
116.90	141.0
118.80	97.0
141.00	254.0
142.90	341.0
145.00	56.0
171.90	151.0
173.10	197.0
174.00	13535.0
175.00	1125.0
176.00	12936.0
177.00	836.0

Instrument :
MSVOA_X
ClientSampleId :
BFB686