

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072919\
 Data File : VX011142.D
 Acq On : 29 Jul 2019 13:51
 Operator : JC/SP
 Sample : K4018-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SU19-MSW0411

Quant Time: Jul 30 05:42:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 24 05:39:23 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	188728	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	299850	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	283123	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	133364	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	103100	51.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.70%	
35) Dibromofluoromethane	5.50	113	94495	49.65	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.30%	
50) Toluene-d8	8.71	98	363434	50.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.82%	
62) 4-Bromofluorobenzene	11.13	95	129338	49.29	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.58%	
Target Compounds						
16) Acetone	2.44	43	5616	6.193	ug/l #	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072919\
Data File : VX011142.D
Acq On : 29 Jul 2019 13:51
Operator : JC/SP
Sample : K4018-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SU19-MSW0411

Quant Time: Jul 30 05:42:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 24 05:39:23 2019
Response via : Initial Calibration

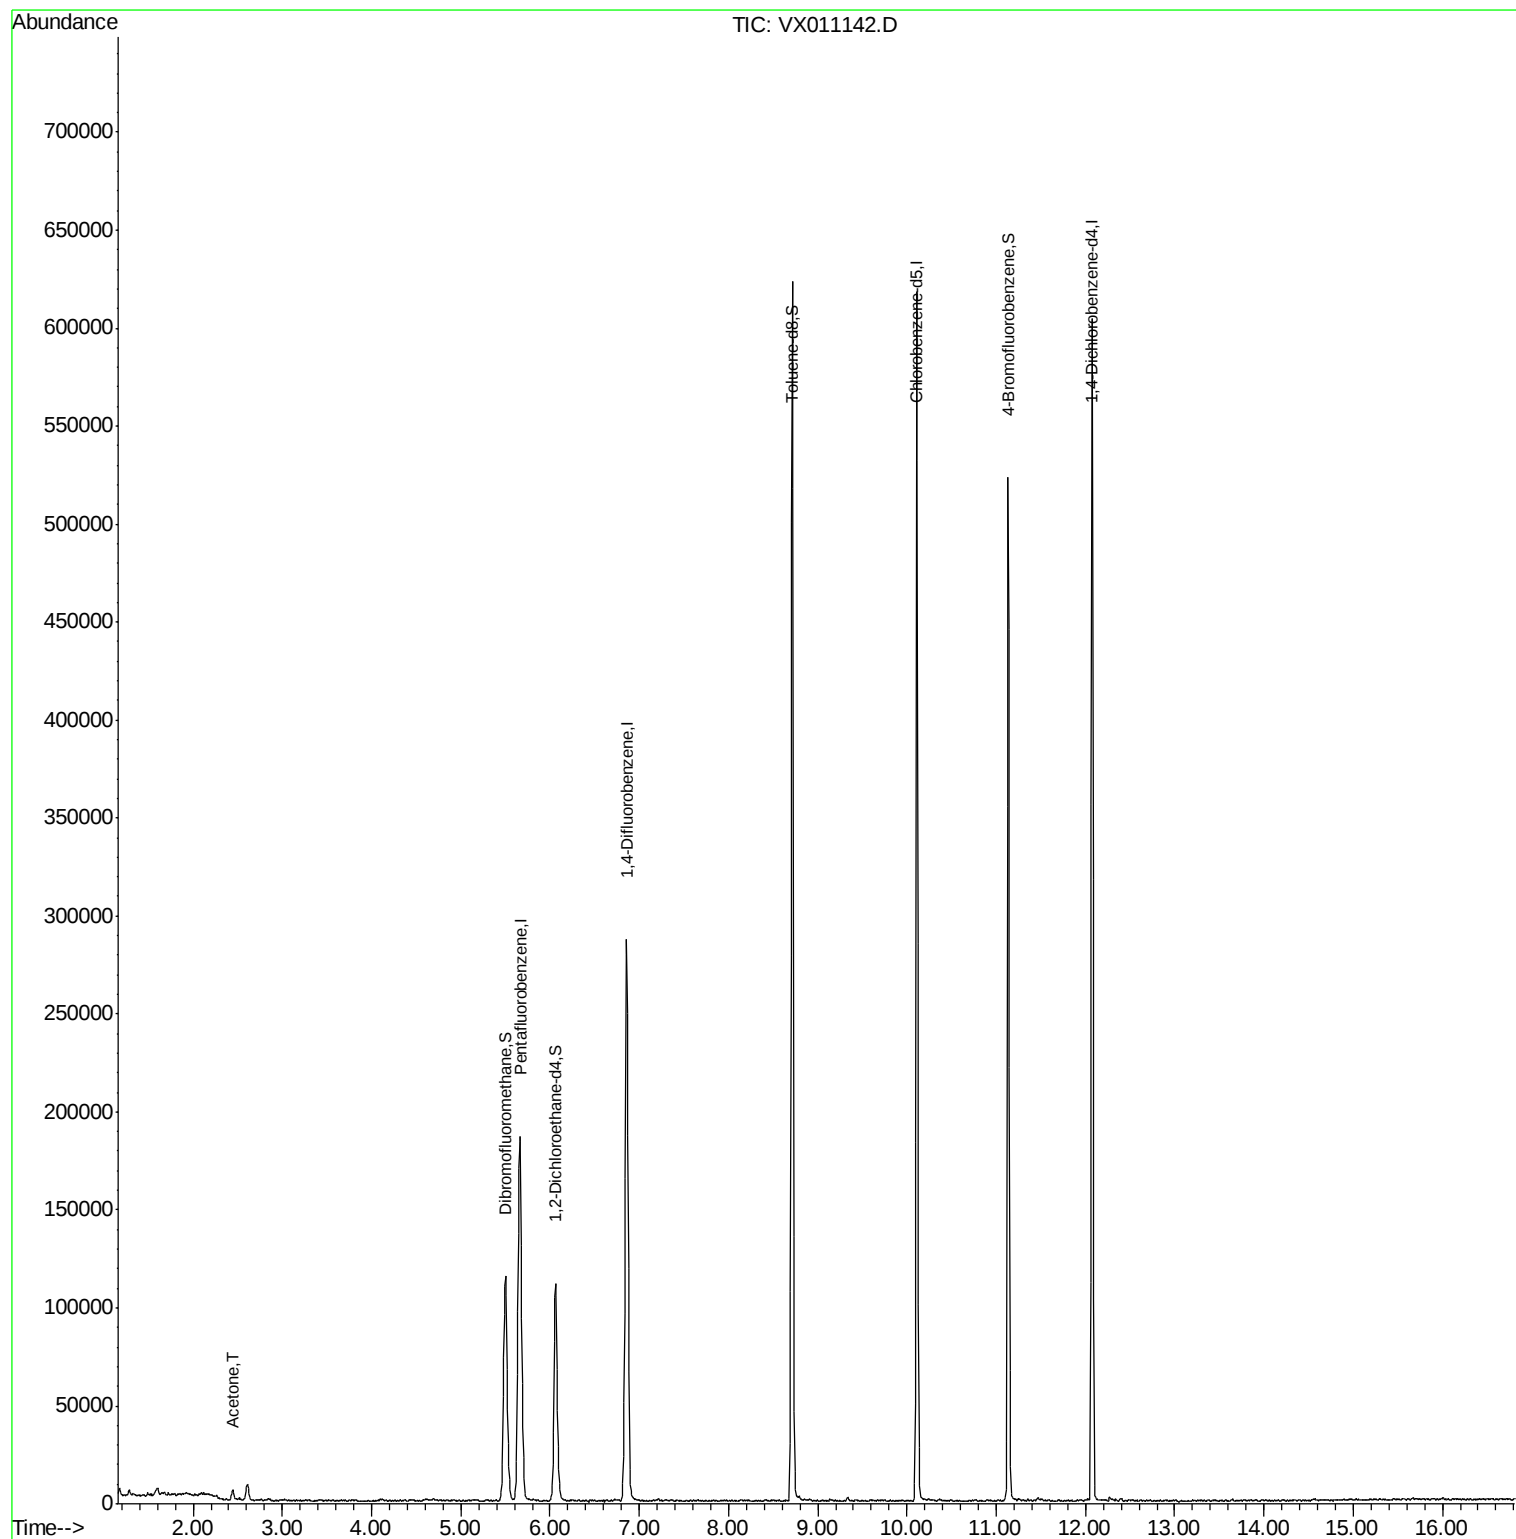

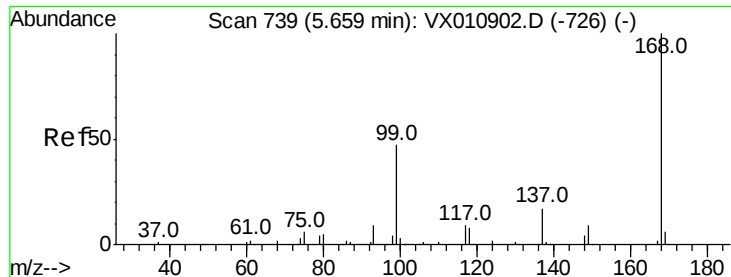

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX011142.D

Acq: 29 Jul 2019 13:51

Instrument :

MSVOA_X

ClientSampleId :


SU19-MSW0411

Tot Ion:168 Resp: 188728

Ion Ratio Lower Upper

168 100

99 48.4 37.6 56.4

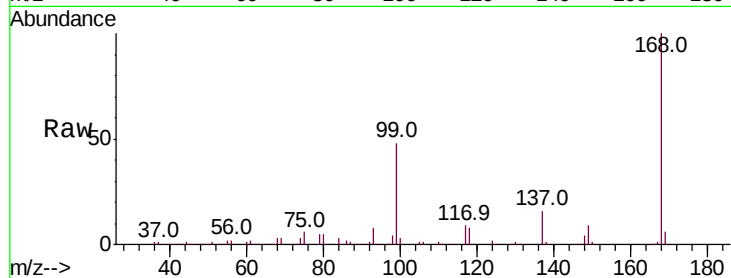

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

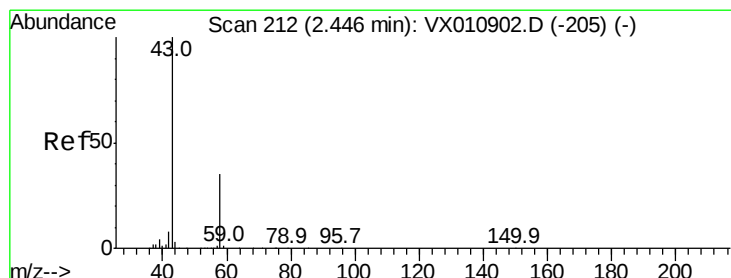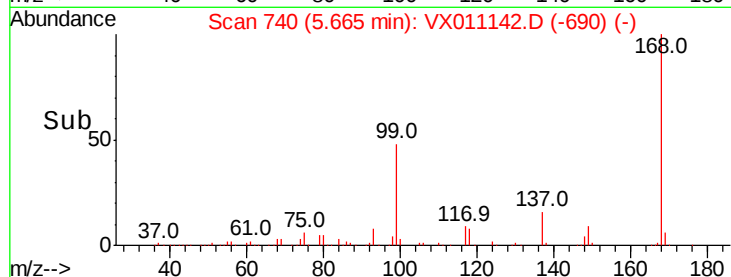

#16

Acetone

Concen: 6.193 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX011142.D


Acq: 29 Jul 2019 13:51

Tgt Ion: 43 Resp: 5616

Ion Ratio Lower Upper

43 100

58 44.2 27.7 41.5#

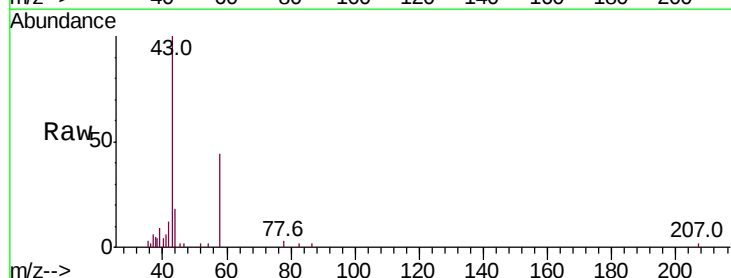

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.44


3000


2000

1000

0

Time--> 2.40 2.45 2.50 2.55

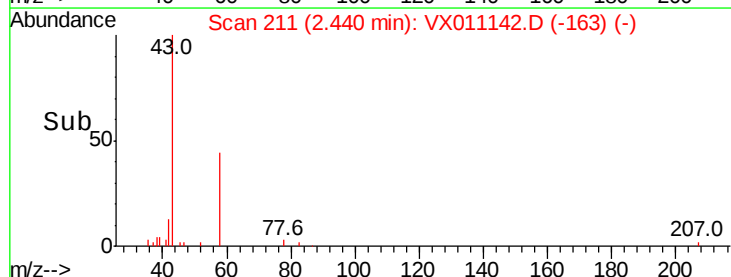

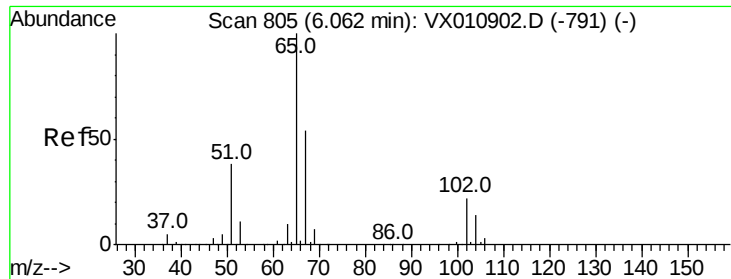

#33

1,2-Dichloroethane-d4

Concen: 51.350 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX011142.D

Acq: 29 Jul 2019 13:51

Instrument :

MSVOA_X

ClientSampleId :


SU19-MSW0411

Tot Ion: 65 Resp: 103100

Ion Ratio Lower Upper




65 100

67 52.7 0.0 107.8

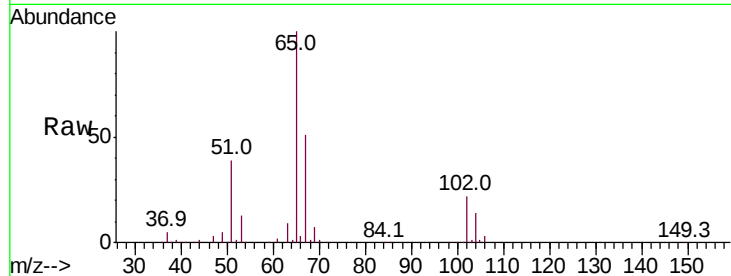

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

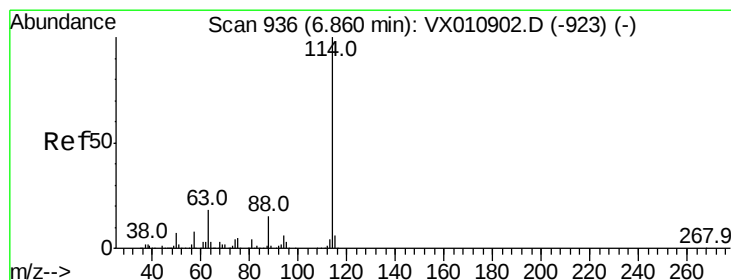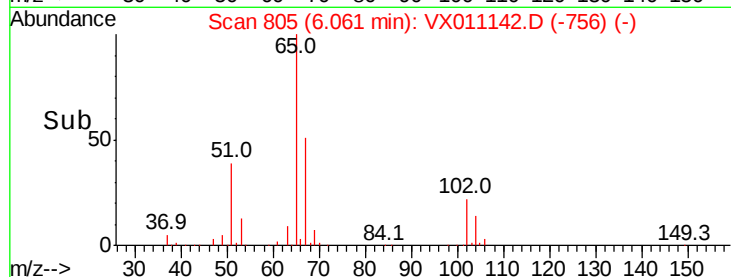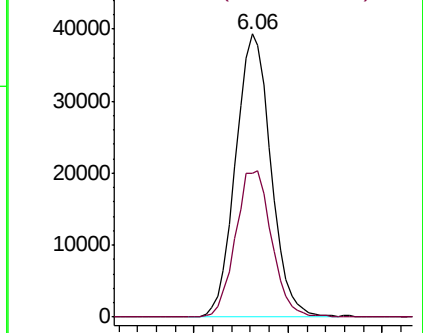

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX011142.D

Acq: 29 Jul 2019 13:51


Tgt Ion: 114 Resp: 299850

Ion Ratio Lower Upper

114 100

63 18.4 0.0 35.6



88 14.3 0.0 29.8

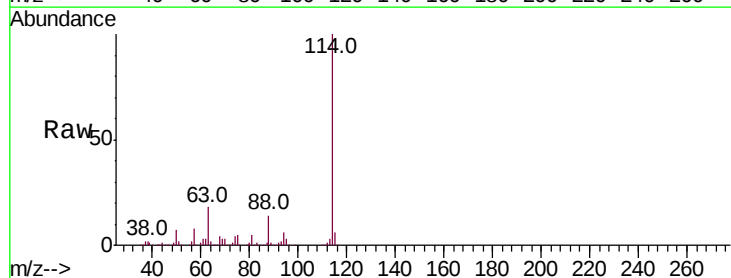


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

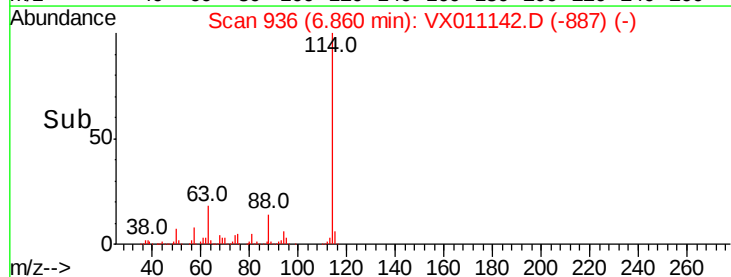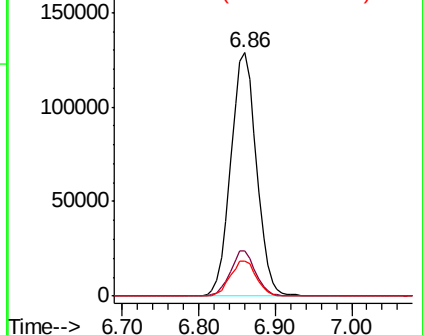

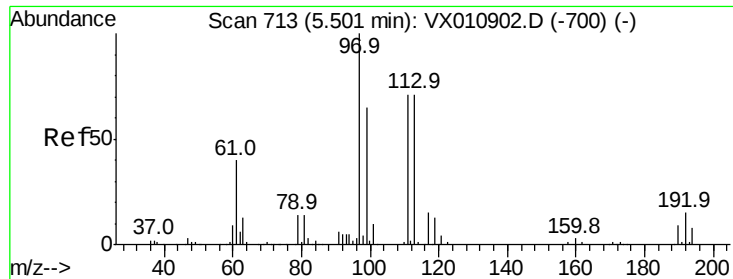

#35

Dibromofluoromethane

Concen: 49.650 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX011142.D

Acq: 29 Jul 2019 13:51

Instrument :

MSVOA_X

ClientSampleId :

SU19-MSW0411


Tot Ion:113 Resp: 94495

Ion Ratio Lower Upper

113 100

111 103.5 82.3 123.5




192 22.1 17.4 26.2

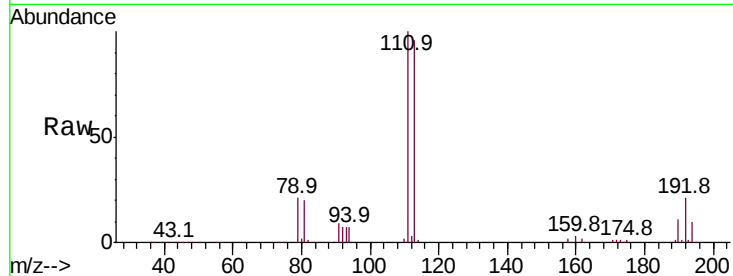

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

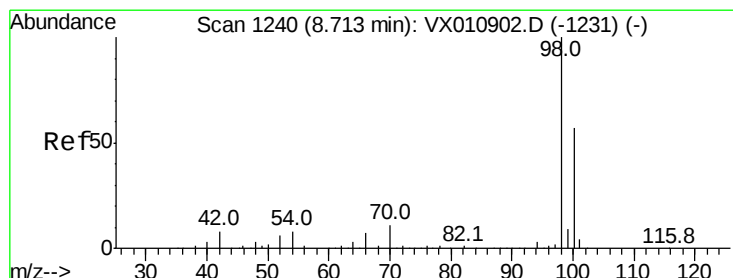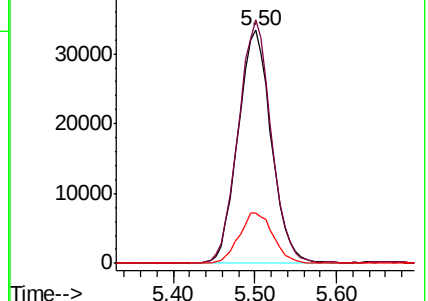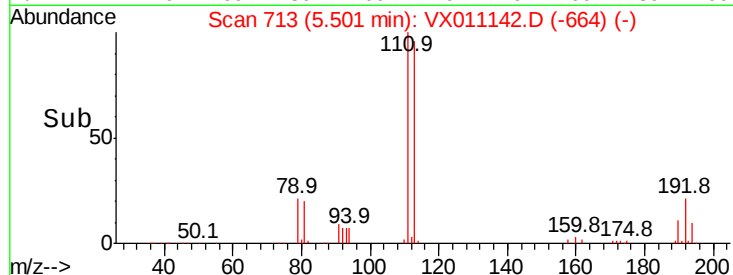

#50

Toluene-d8

Concen: 50.914 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX011142.D


Acq: 29 Jul 2019 13:51

Tgt Ion: 98 Resp: 363434

Ion Ratio Lower Upper



98 100


100 63.7 50.6 75.8

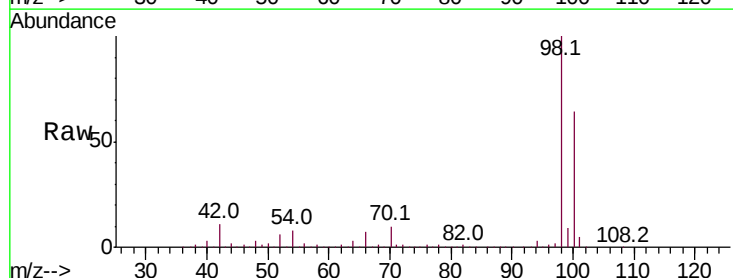

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

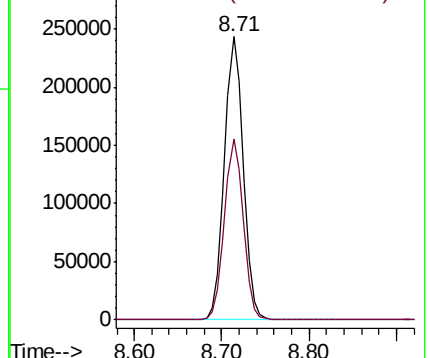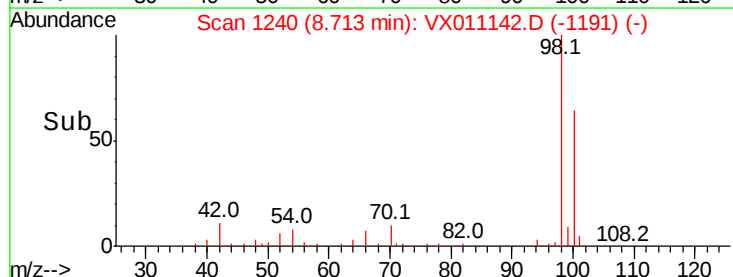

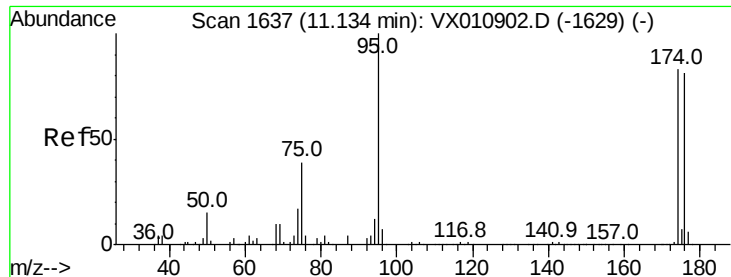

#62

4-Bromofluorobenzene

Concen: 49.294 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX011142.D

Acq: 29 Jul 2019 13:51

Instrument :

MSVOA_X

ClientSampleId :

SU19-MSW0411


Tot Ion: 95 Resp: 129338

Ion Ratio Lower Upper

95 100

174 89.4 0.0 180.6




176 87.4 0.0 173.8

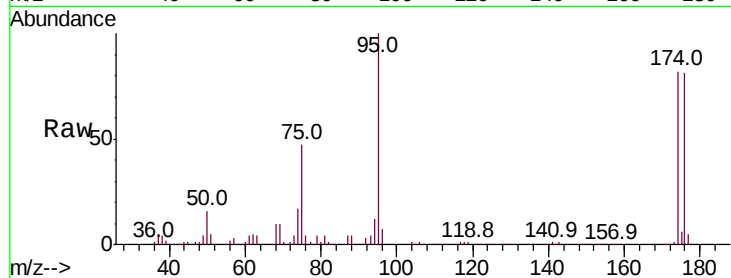

Abundance Ion 94.90 (94.60 to 95.60): VX011142.D (-1588) (-)

Ion 173.80 (173.50 to 174.50): VX011142.D (-1588) (-)

Ion 175.80 (175.50 to 176.50): VX011142.D (-1588) (-)

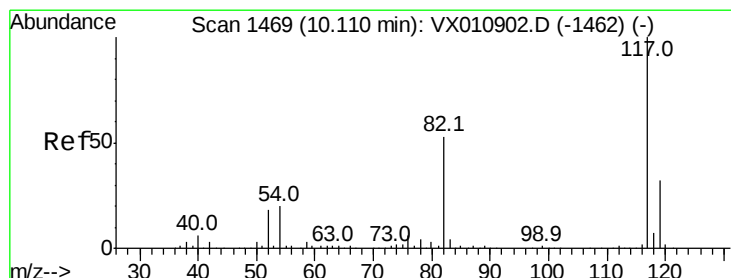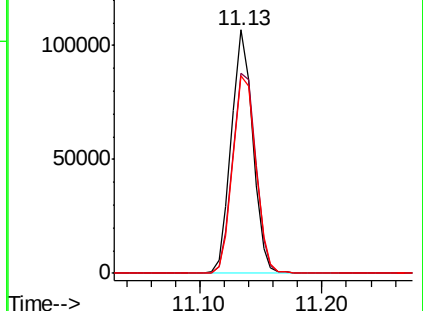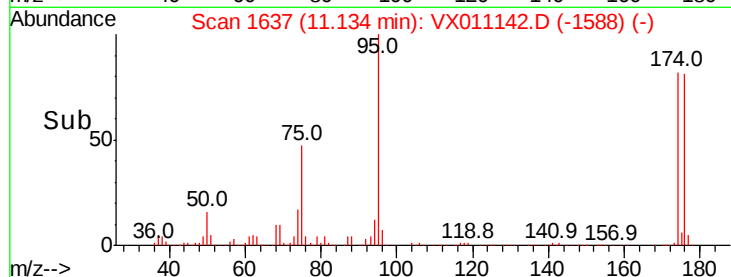

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX011142.D

Acq: 29 Jul 2019 13:51


Tgt Ion: 117 Resp: 283123

Ion Ratio Lower Upper

117 100

82 52.3 42.6 63.8



119 31.7 25.9 38.9

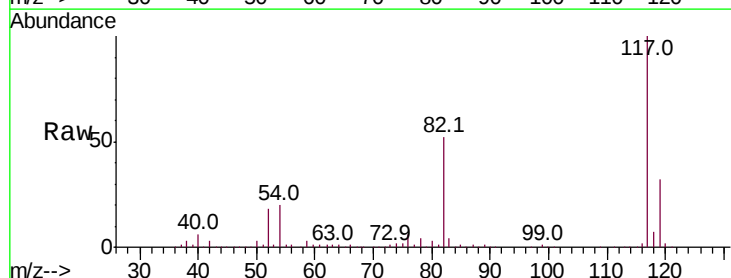


Abundance Ion 116.90 (116.60 to 117.60): VX011142.D (-1420) (-)

Ion 82.00 (81.70 to 82.70): VX011142.D (-1420) (-)

Ion 118.90 (118.60 to 119.60): VX011142.D (-1420) (-)

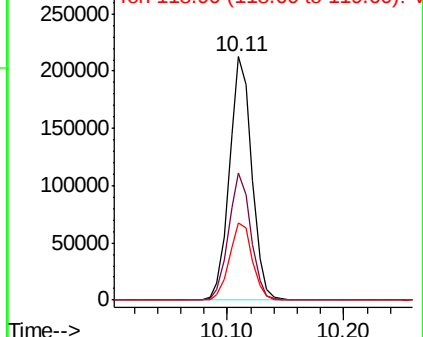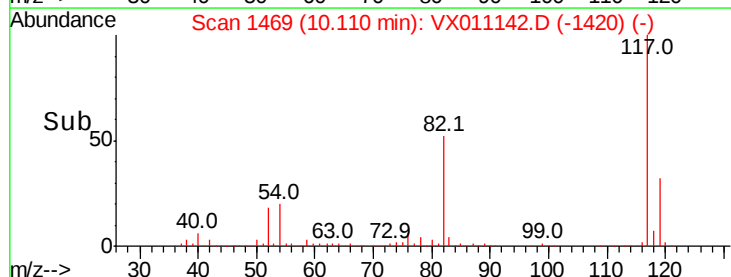

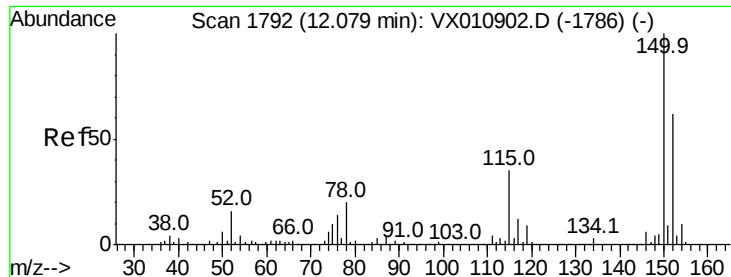

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. -0.00 min
 Lab File: VX011142.D
 Acq: 29 Jul 2019 13:51

Instrument :
 MSVOA_X
 ClientSampleId :
 SU19-MSW0411

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.2	39.7	119.1
150	155.6	0.0	345.6

