
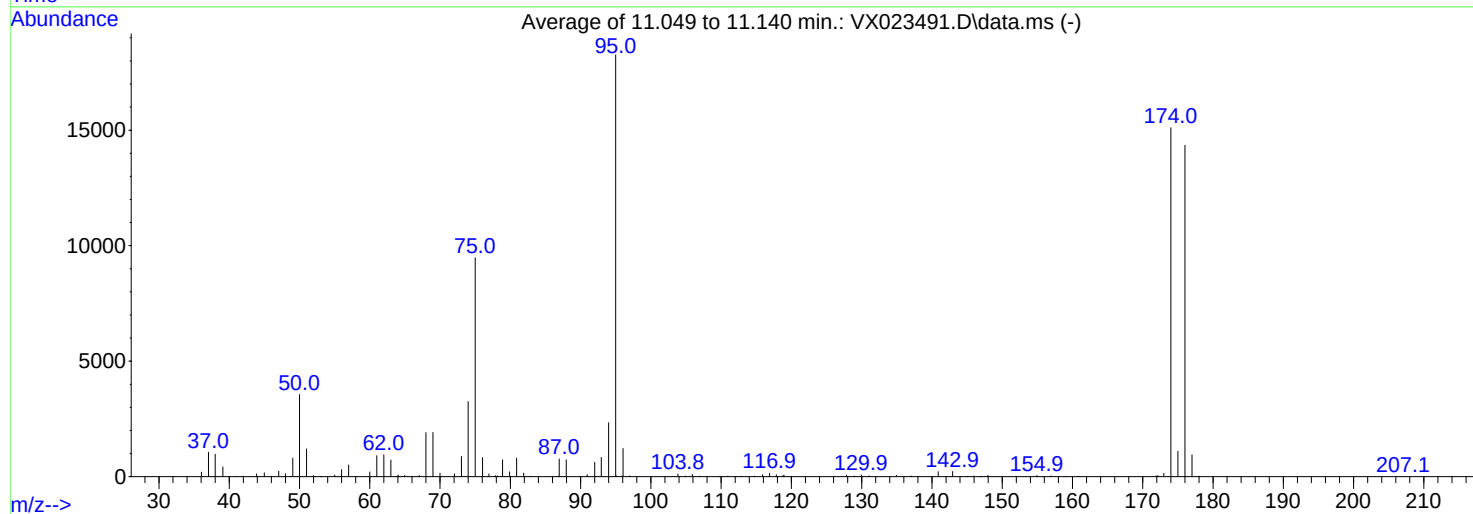


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072921\
Data File : VX023491.D
Acq On : 28 Jul 2021 14:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X072921W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Jul 29 03:13:17 2021

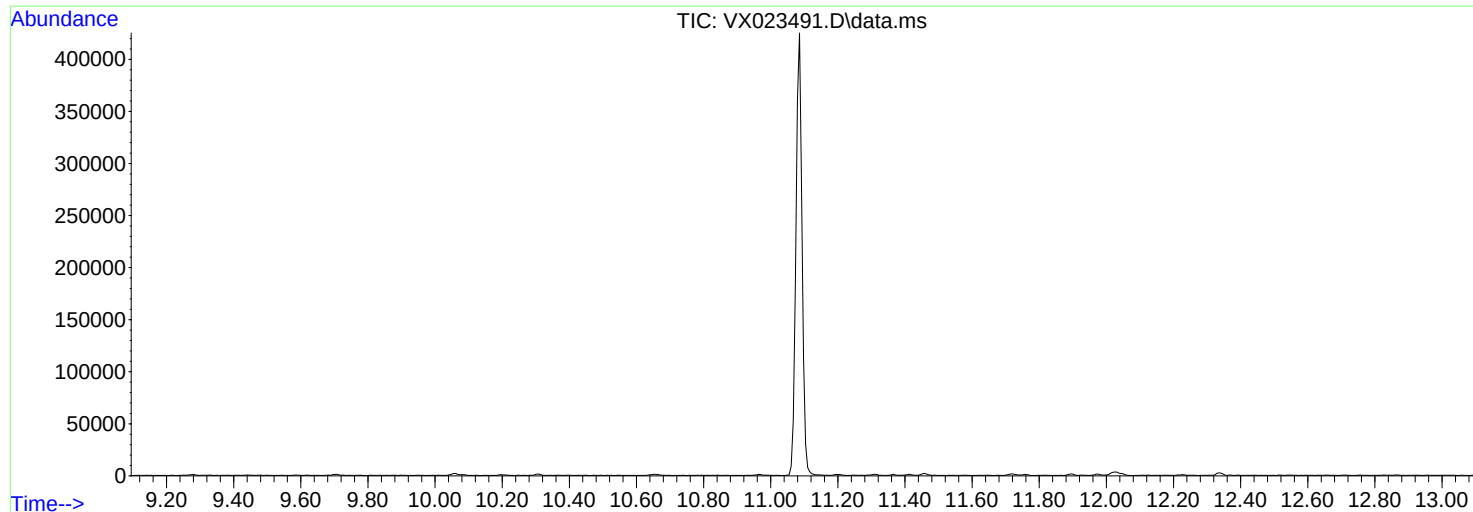

AutoFind: Averaged scan 1634 to 1649; Bkg corrected with scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	3551	PASS
75	95	30	60	51.9	9474	PASS
95	95	100	100	100.0	18262	PASS
96	95	5	9	6.7	1221	PASS
173	174	0.00	2	1.0	144	PASS
174	95	50	100	82.7	15105	PASS
175	174	5	9	7.3	1099	PASS
176	174	95	101	95.0	14344	PASS
177	176	5	9	6.6	940	PASS