

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072922\
 Data File : VX030307.D
 Acq On : 29 Jul 2022 16:56
 Operator : JC/MD
 Sample : N3861-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-13

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	20	25	28	rBV	32847	46248	3.67%	0.776%
2	1.569	69	79	81	rBV6	6094	13342	1.06%	0.224%
3	1.746	104	108	116	rVB	26509	35800	2.84%	0.600%
4	2.215	180	185	195	rVB	17526	30862	2.45%	0.518%
5	2.782	270	278	283	rBV4	7380	16795	1.33%	0.282%
6	2.867	286	292	302	rVB2	19553	42233	3.35%	0.708%
7	3.733	426	434	443	rBV4	6506	16111	1.28%	0.270%
8	4.099	485	494	503	rBV6	5168	14536	1.15%	0.244%
9	4.312	517	529	539	rBV3	11049	31220	2.48%	0.524%
10	4.428	539	548	556	rVV4	5700	15953	1.27%	0.268%
11	5.391	694	706	718	rBV2	141726	418518	33.20%	7.020%
12	5.556	724	733	748	rVB	156567	440940	34.98%	7.396%
13	5.964	788	800	811	rBV	173689	459465	36.45%	7.707%
14	6.769	922	932	944	rBV	254590	632229	50.16%	10.604%
15	7.172	993	998	1006	rVB3	7309	15349	1.22%	0.257%
16	8.653	1231	1241	1251	rBV	799348	1260479	100.00%	21.142%
17	10.055	1463	1471	1481	rBV	589818	788970	62.59%	13.233%
18	11.085	1634	1640	1649	rBV	604901	775304	61.51%	13.004%
19	12.024	1787	1794	1806	rBV	750742	907626	72.01%	15.224%




Sum of corrected areas: 5961980

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072922\
Data File : VX030307.D
Acq On : 29 Jul 2022 16:56
Operator : JC/MD
Sample : N3861-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

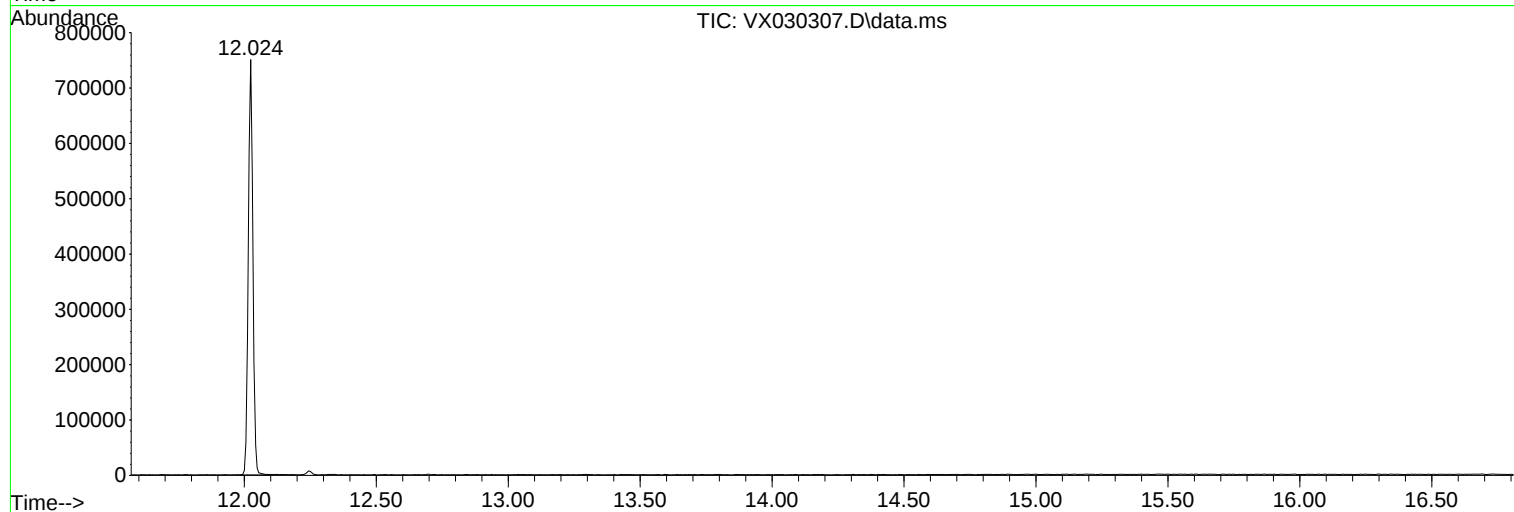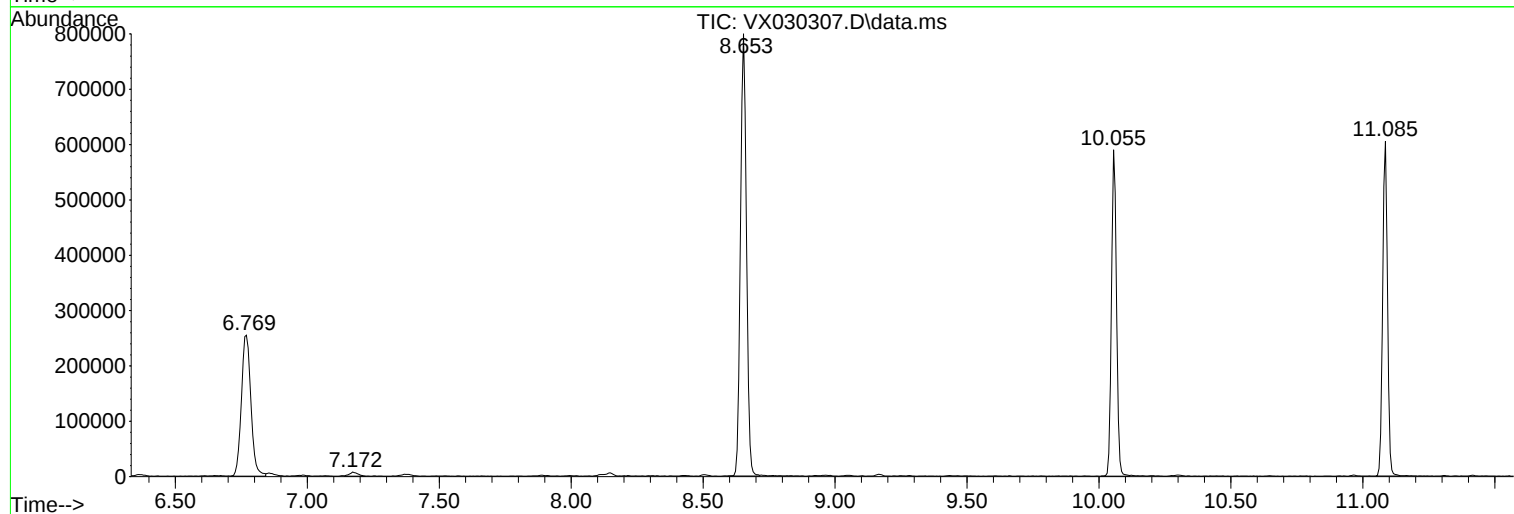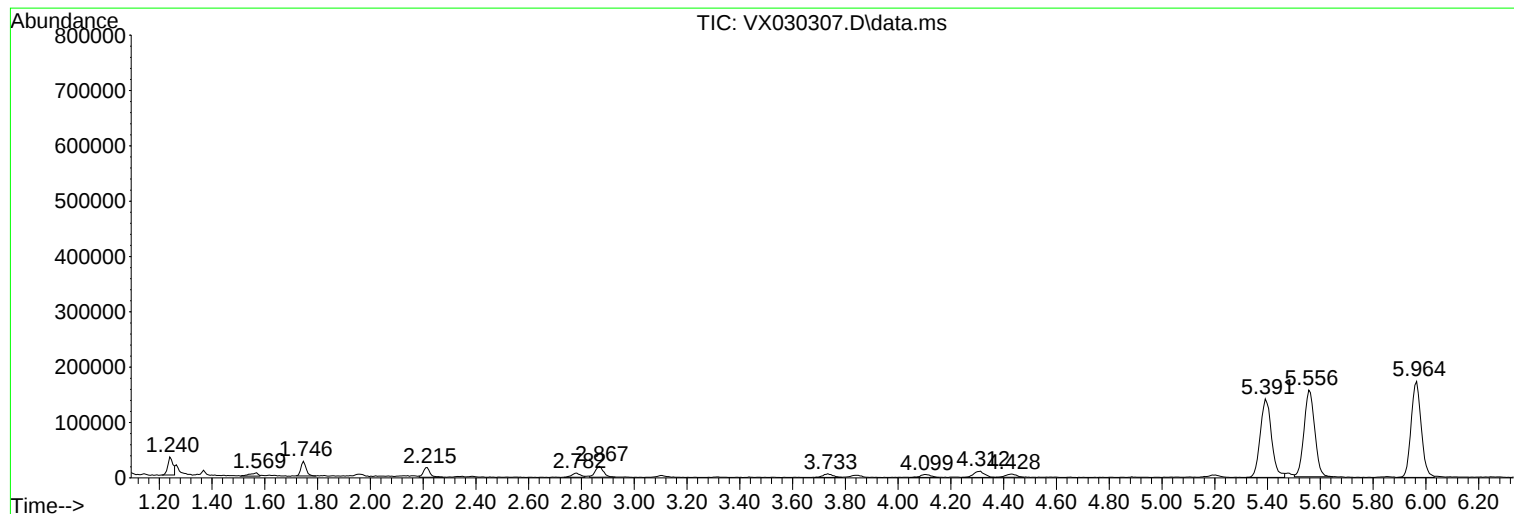

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072922\
Data File : VX030307.D
Acq On : 29 Jul 2022 16:56
Operator : JC/MD
Sample : N3861-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.240	5.24 ug/l	46248	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			2-Aminoethyl hydrogen sulfate	141	C2H7NO4S	000926-39-6	9
4			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
5			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4

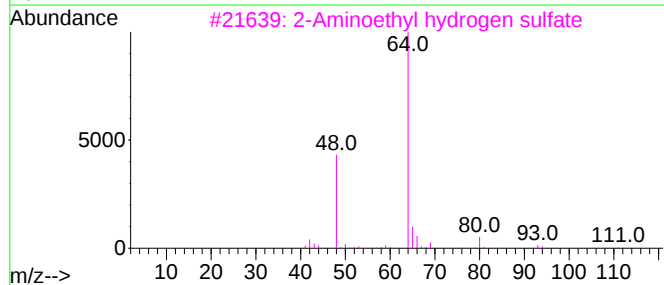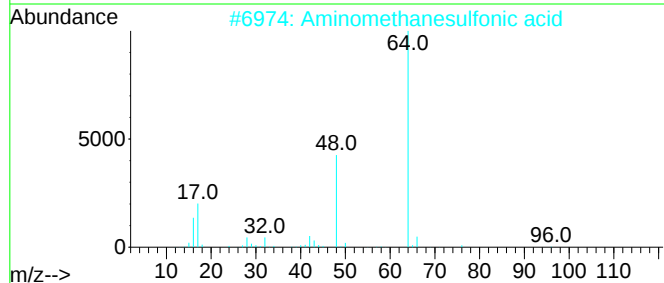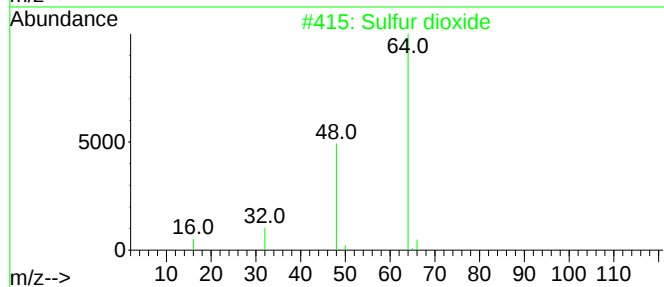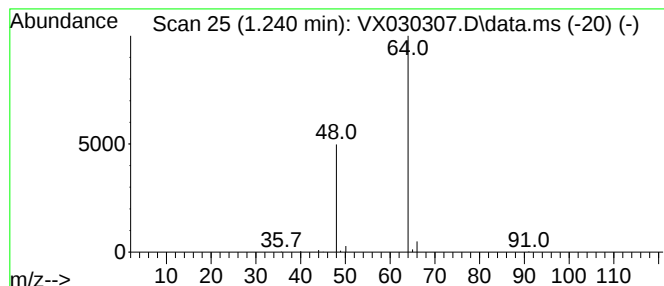

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072922\
Data File : VX030307.D
Acq On : 29 Jul 2022 16:56
Operator : JC/MD
Sample : N3861-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.240	5.2	ug/l	46248	1	5.556	440940	50.0