

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042677.D
 Acq On : 29 Jul 2024 09:54
 Operator : JC/MD
 Sample : VX0729MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 11:59:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	179275	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	163055	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	60985	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	43882	40.290	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.580%
7) Chloroethane-d5	1.648	69	26839	59.800	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	119.600%
11) 1,1-Dichloroethene-d2	2.300	65	24045	44.807	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.620%
21) 2-Butanone-d5	4.459	46	89690	111.107	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.110%
24) Chloroform-d	5.050	84	115657	48.514	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.020%
26) 1,2-Dichloroethane-d4	5.952	65	78850	51.267	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.540%
32) Benzene-d6	5.971	84	221712	48.994	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.980%
36) 1,2-Dichloropropane-d6	7.306	67	68484	51.134	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.260%
41) Toluene-d8	8.647	98	194234	47.871	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.740%
43) trans-1,3-Dichloroprop...	8.952	79	29227	46.632	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.260%
47) 2-Hexanone-d5	9.385	63	61303	102.375	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.380%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	96383	49.982	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.960%
66) 1,2-Dichlorobenzene-d4	12.317	152	60214	52.245	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.480%
Target Compounds						
37) 1,2-Dichloropropane	7.300	63	8169	6.299	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042677.D
Acq On : 29 Jul 2024 09:54
Operator : JC/MD
Sample : VX0729MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 29 11:59:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration

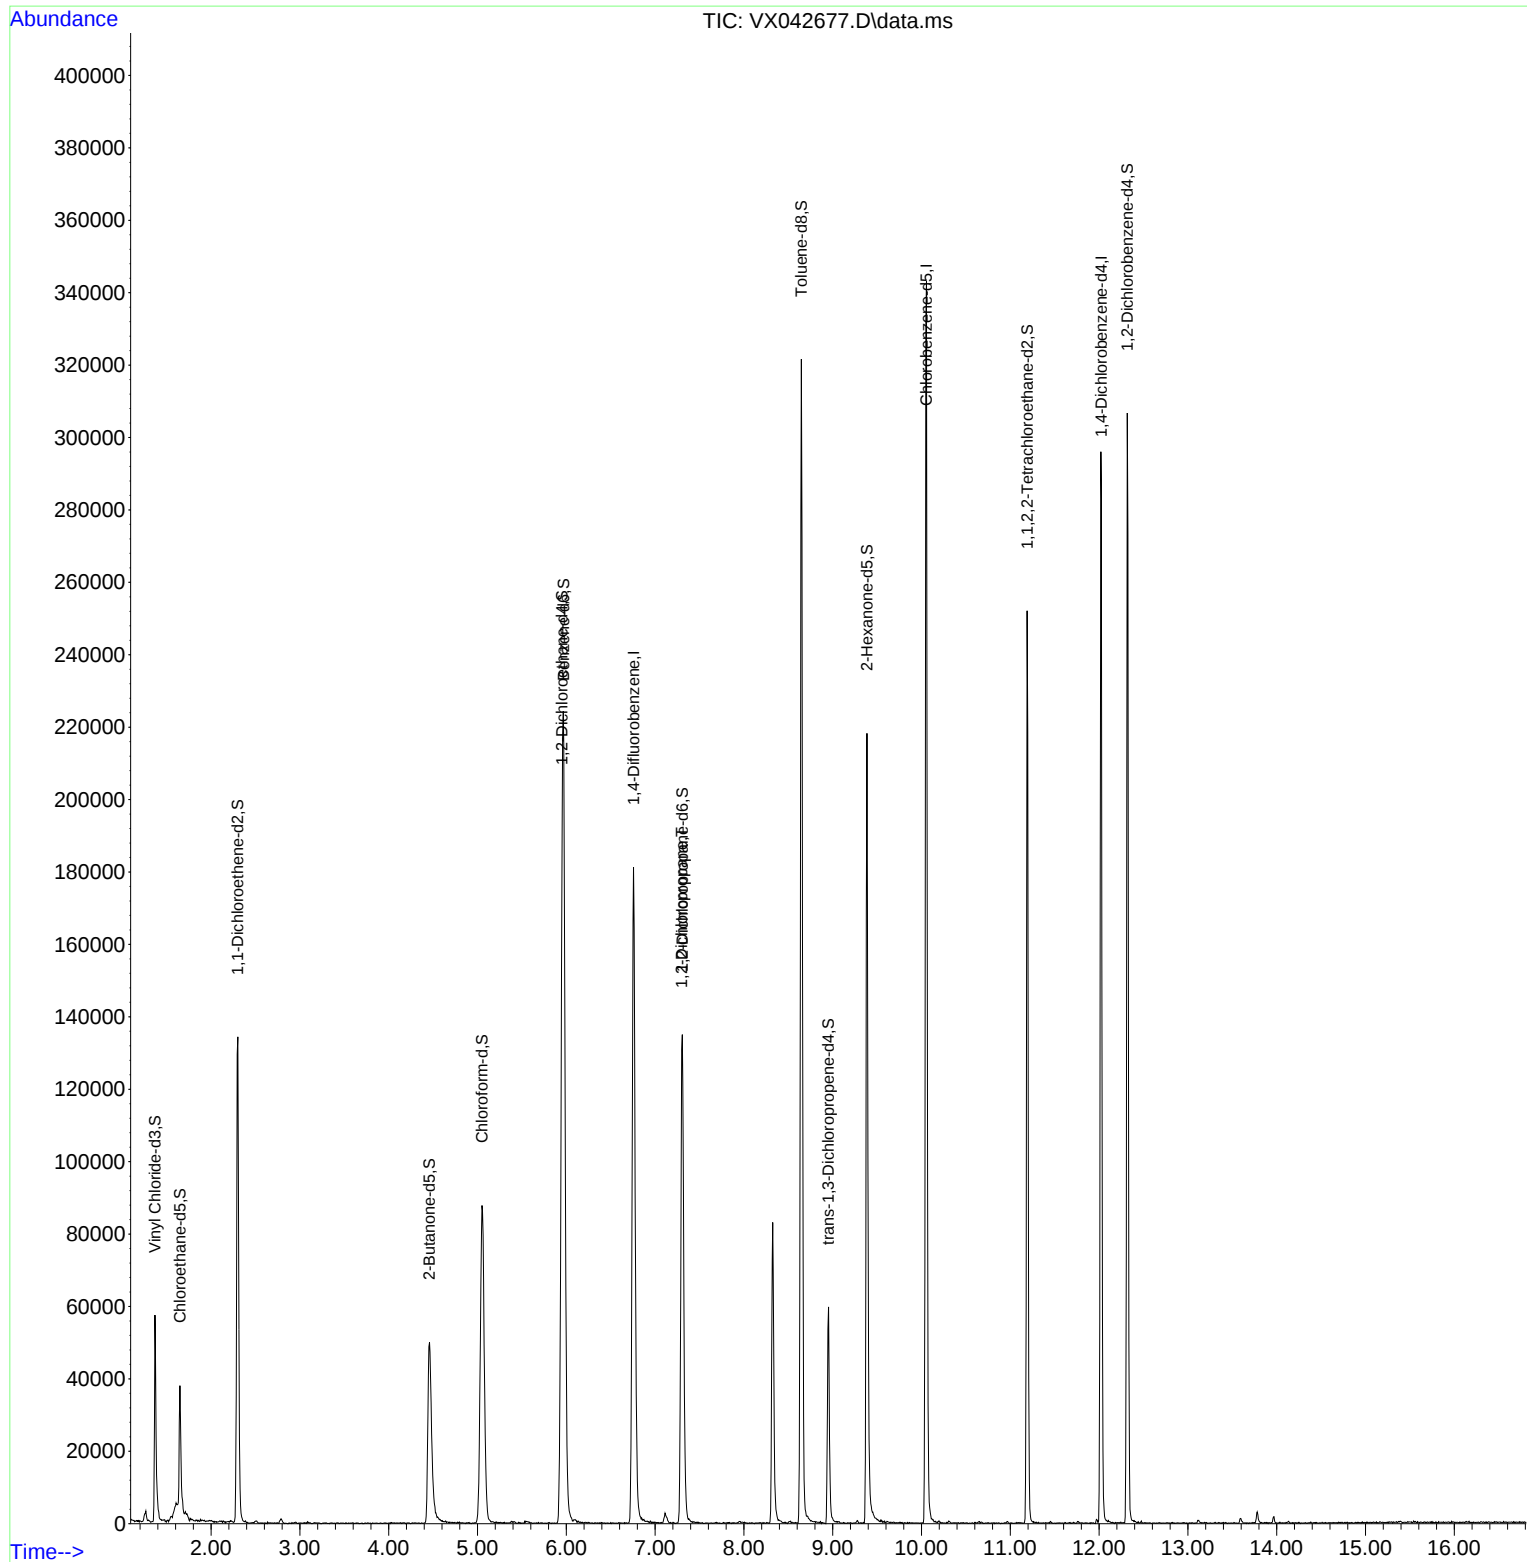

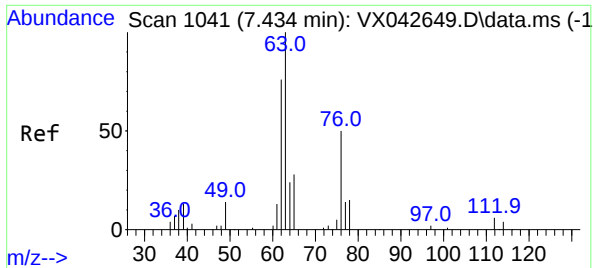

#37
1,2-Dichloropropane
Concen: 6.299 ug/L
RT: 7.300 min Scan# 10
Delta R.T. -0.134 min
Lab File: VX042677.D
Acq: 29 Jul 2024 09:54

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 8169
Ion Ratio Lower Upper
63 100
112 0.0 3.7 5.5#

