

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042679.D
 Acq On : 29 Jul 2024 10:51
 Operator : JC/MD
 Sample : P3335-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 29 11:59:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	177510	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	159489	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	63718	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	44689	41.439	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.880%
7) Chloroethane-d5	1.648	69	23927	53.842	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.680%
11) 1,1-Dichloroethene-d2	2.294	65	24536	46.176	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.360%
21) 2-Butanone-d5	4.458	46	83633	104.634	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.630%
24) Chloroform-d	5.050	84	116349	49.290	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.580%
26) 1,2-Dichloroethane-d4	5.952	65	80292	52.724	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.440%
32) Benzene-d6	5.970	84	228073	51.526	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.060%
36) 1,2-Dichloropropane-d6	7.299	67	71029	54.220	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.440%
41) Toluene-d8	8.647	98	196613	49.541	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.080%
43) trans-1,3-Dichloroprop...	8.952	79	29050	47.386	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.780%
47) 2-Hexanone-d5	9.384	63	60163	102.718	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.720%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	99831	52.927	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.860%
66) 1,2-Dichlorobenzene-d4	12.317	152	65085	54.049	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.100%
Target Compounds						Qvalue
13) Acetone	2.386	43	3155	5.050	ug/L	97
61) 1,2,3-Trichloropropane	12.018	75	8243	5.592	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042679.D
Acq On : 29 Jul 2024 10:51
Operator : JC/MD
Sample : P3335-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 29 11:59:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration

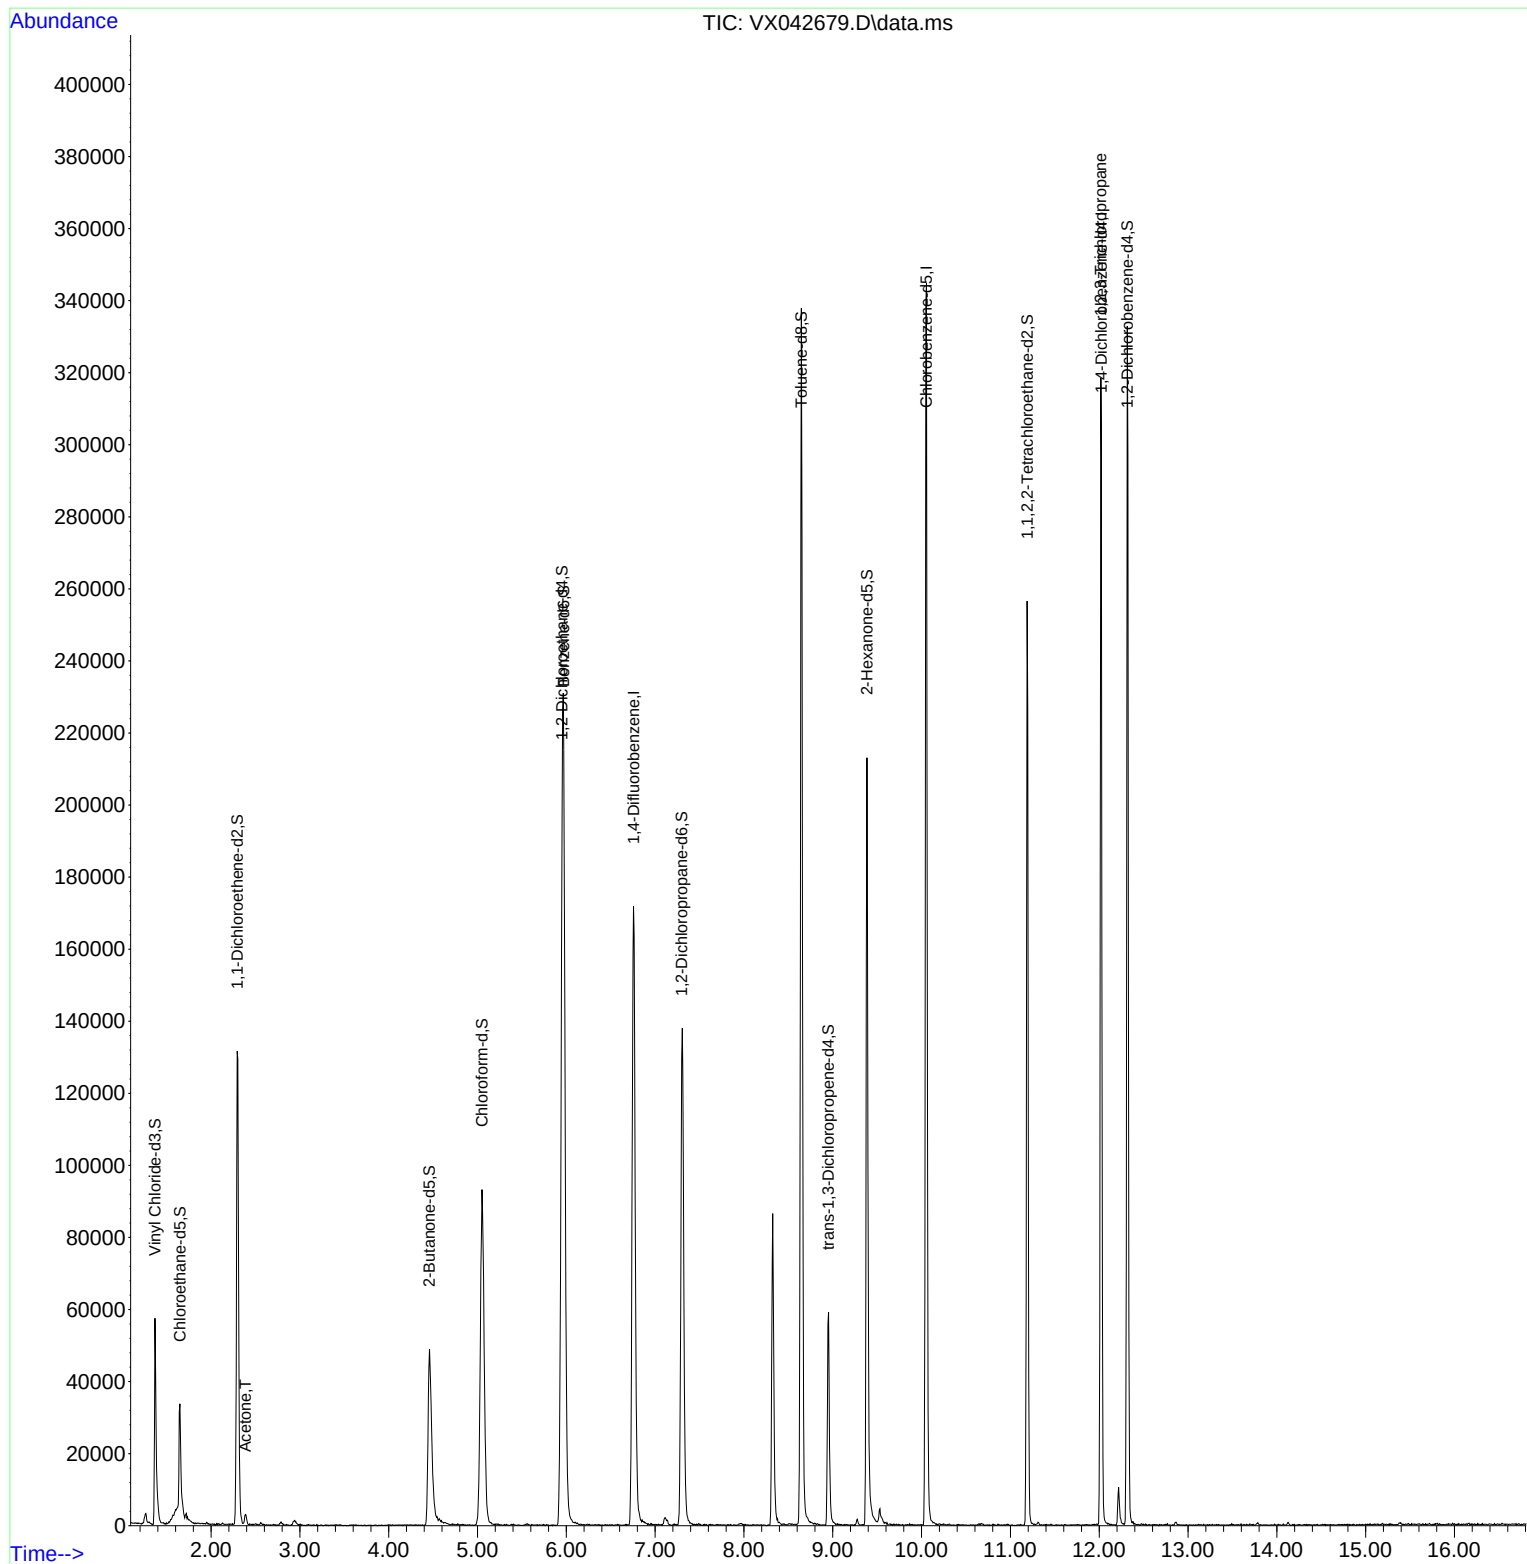



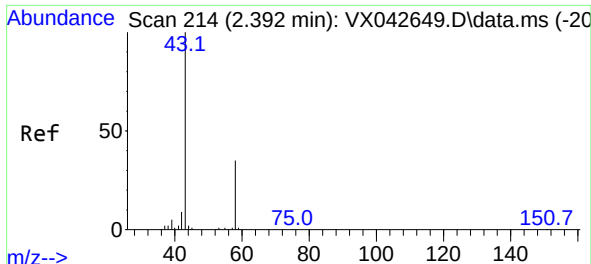


#13
Acetone
Concen: 5.050 ug/L
RT: 2.386 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX042679.D
Acq: 29 Jul 2024 10:51

Instrument :
MSVOA_X
ClientSampleId :

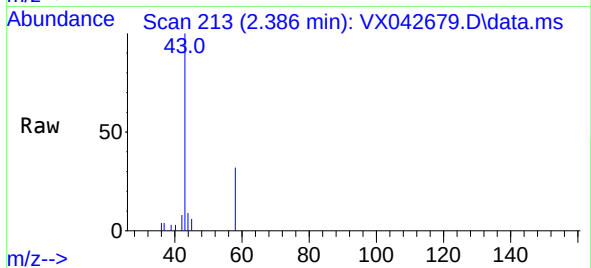

Tgt Ion: 43 Resp: 3155
Ion Ratio Lower Upper
43 100
58 33.0 0.0 62.4

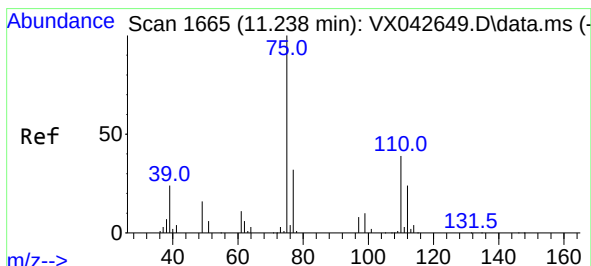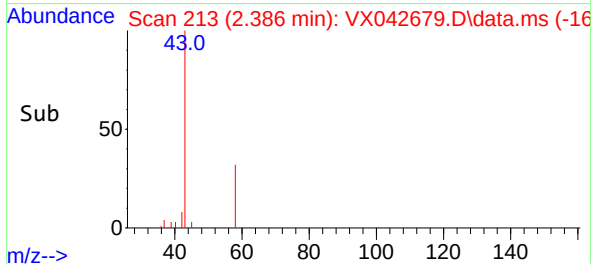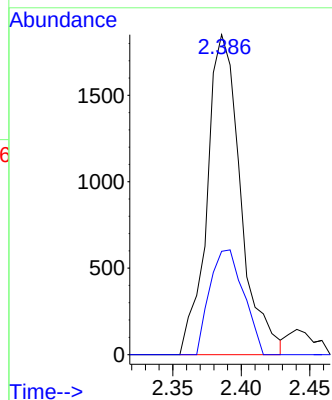

#61
1,2,3-Trichloropropane
Concen: 5.592 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX042679.D
Acq: 29 Jul 2024 10:51

Tgt Ion: 75 Resp: 8243
Ion Ratio Lower Upper
75 100
77 31.1 26.2 39.4
110 4.0 33.0 49.4#

