

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042689.D
 Acq On : 29 Jul 2024 14:40
 Operator : JC/MD
 Sample : P3335-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 30 12:59:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 30 02:11:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	166090	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	149800	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	55314	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	40184	39.823	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.640%
7) Chloroethane-d5	1.648	69	19544	47.003	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.000%
11) 1,1-Dichloroethene-d2	2.294	65	21906	44.061	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.120%
21) 2-Butanone-d5	4.465	46	83838	112.102	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.100%
24) Chloroform-d	5.056	84	108254	49.014	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.020%
26) 1,2-Dichloroethane-d4	5.958	65	76142	53.437	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.880%
32) Benzene-d6	5.970	84	211220	50.805	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.620%
36) 1,2-Dichloropropane-d6	7.312	67	66421	53.982	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.960%
41) Toluene-d8	8.647	98	176550	47.363	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.720%
43) trans-1,3-Dichloroprop...	8.952	79	26706	46.380	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.760%
47) 2-Hexanone-d5	9.384	63	59801	108.703	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.700%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	93862	52.981	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.960%
66) 1,2-Dichlorobenzene-d4	12.323	152	57796	55.288	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.580%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.024	75	7274	5.684	ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042689.D
Acq On : 29 Jul 2024 14:40
Operator : JC/MD
Sample : P3335-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 30 12:59:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 30 02:11:54 2024
Response via : Initial Calibration

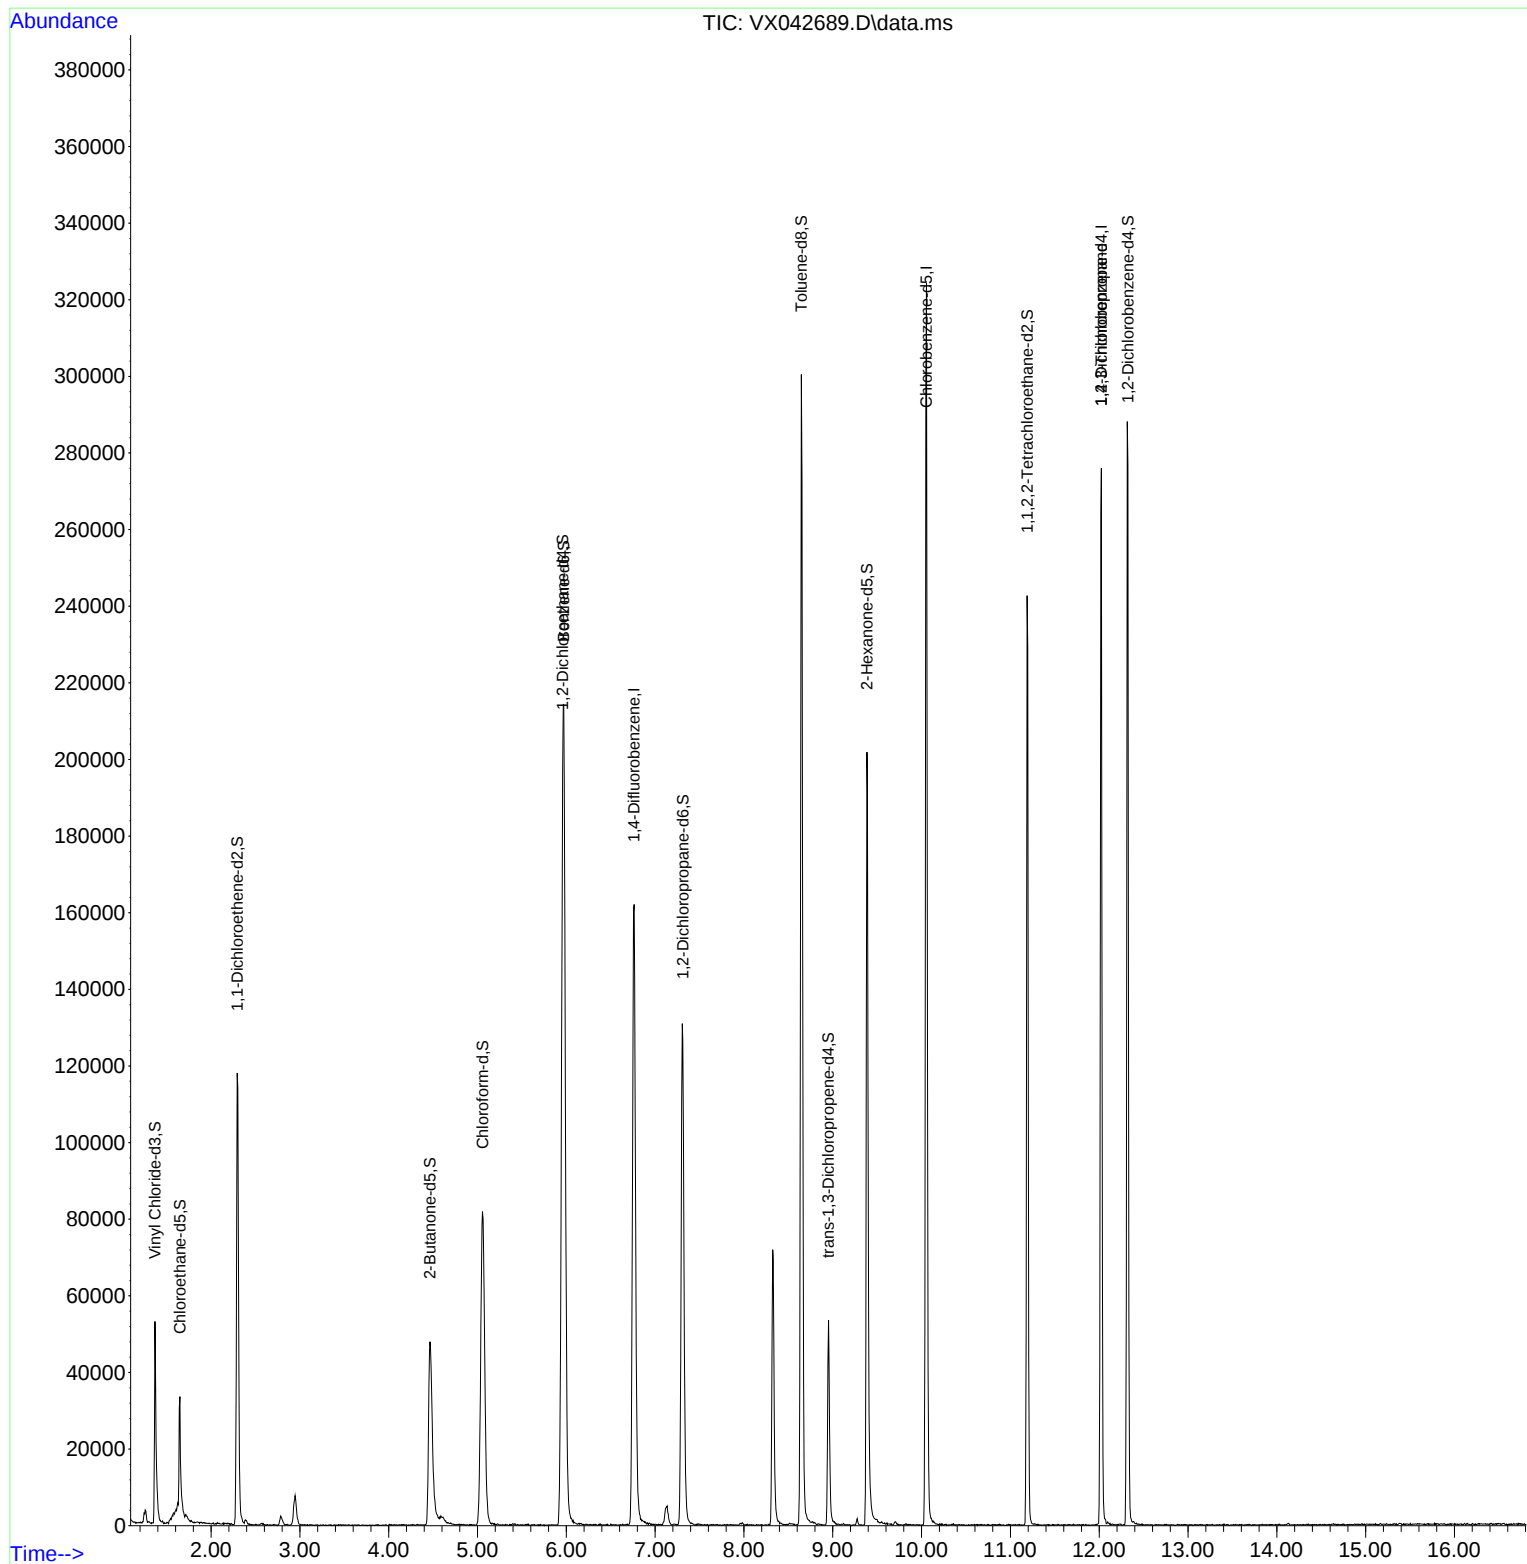

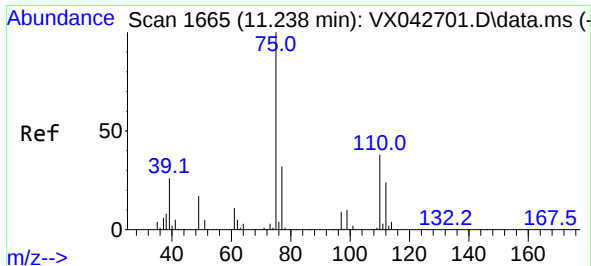

#61
1,2,3-Trichloropropane
Concen: 5.684 ug/L
RT: 12.024 min Scan# 11
Delta R.T. 0.787 min
Lab File: VX042689.D
Acq: 29 Jul 2024 14:40

Instrument :
MSVOA_X
ClientSampleId :

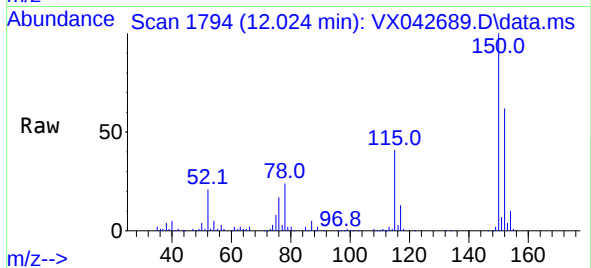

Tgt Ion:	75	Resp:	7274
Ion	Ratio	Lower	Upper
75	100		
77	38.0	26.2	39.4
110	3.3	33.0	49.4#

