

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042713.D
 Acq On : 29 Jul 2024 23:58
 Operator : JC/MD
 Sample : P3388-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 30 05:30:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 30 02:11:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	168110	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	151240	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	58626	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	27657	27.080	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	54.160%#
7) Chloroethane-d5	1.715	69	991	2.355	ug/L	0.07
Spiked Amount	50.000	Range	70 - 130	Recovery	=	4.700%#
11) 1,1-Dichloroethene-d2	2.300	65	15599	30.999	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.000%
21) 2-Butanone-d5	4.465	46	73108	96.580	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.580%
24) Chloroform-d	5.056	84	88166	39.439	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.880%
26) 1,2-Dichloroethane-d4	5.952	65	61824	42.867	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.740%
32) Benzene-d6	5.970	84	159655	38.036	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.080%
36) 1,2-Dichloropropane-d6	7.306	67	52165	41.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.980%
41) Toluene-d8	8.647	98	137032	36.412	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	72.820%#
43) trans-1,3-Dichloroprop...	8.952	79	20023	34.443	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.880%
47) 2-Hexanone-d5	9.384	63	50019	90.056	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.060%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	78699	43.999	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.000%
66) 1,2-Dichlorobenzene-d4	12.317	152	49098	44.314	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.620%
Target Compounds						
					Qvalue	
13) Acetone	2.392	43	2882	4.871	ug/L	99
61) 1,2,3-Trichloropropane	12.018	75	7263	5.355	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042713.D
Acq On : 29 Jul 2024 23:58
Operator : JC/MD
Sample : P3388-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 30 05:30:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 30 02:11:54 2024
Response via : Initial Calibration

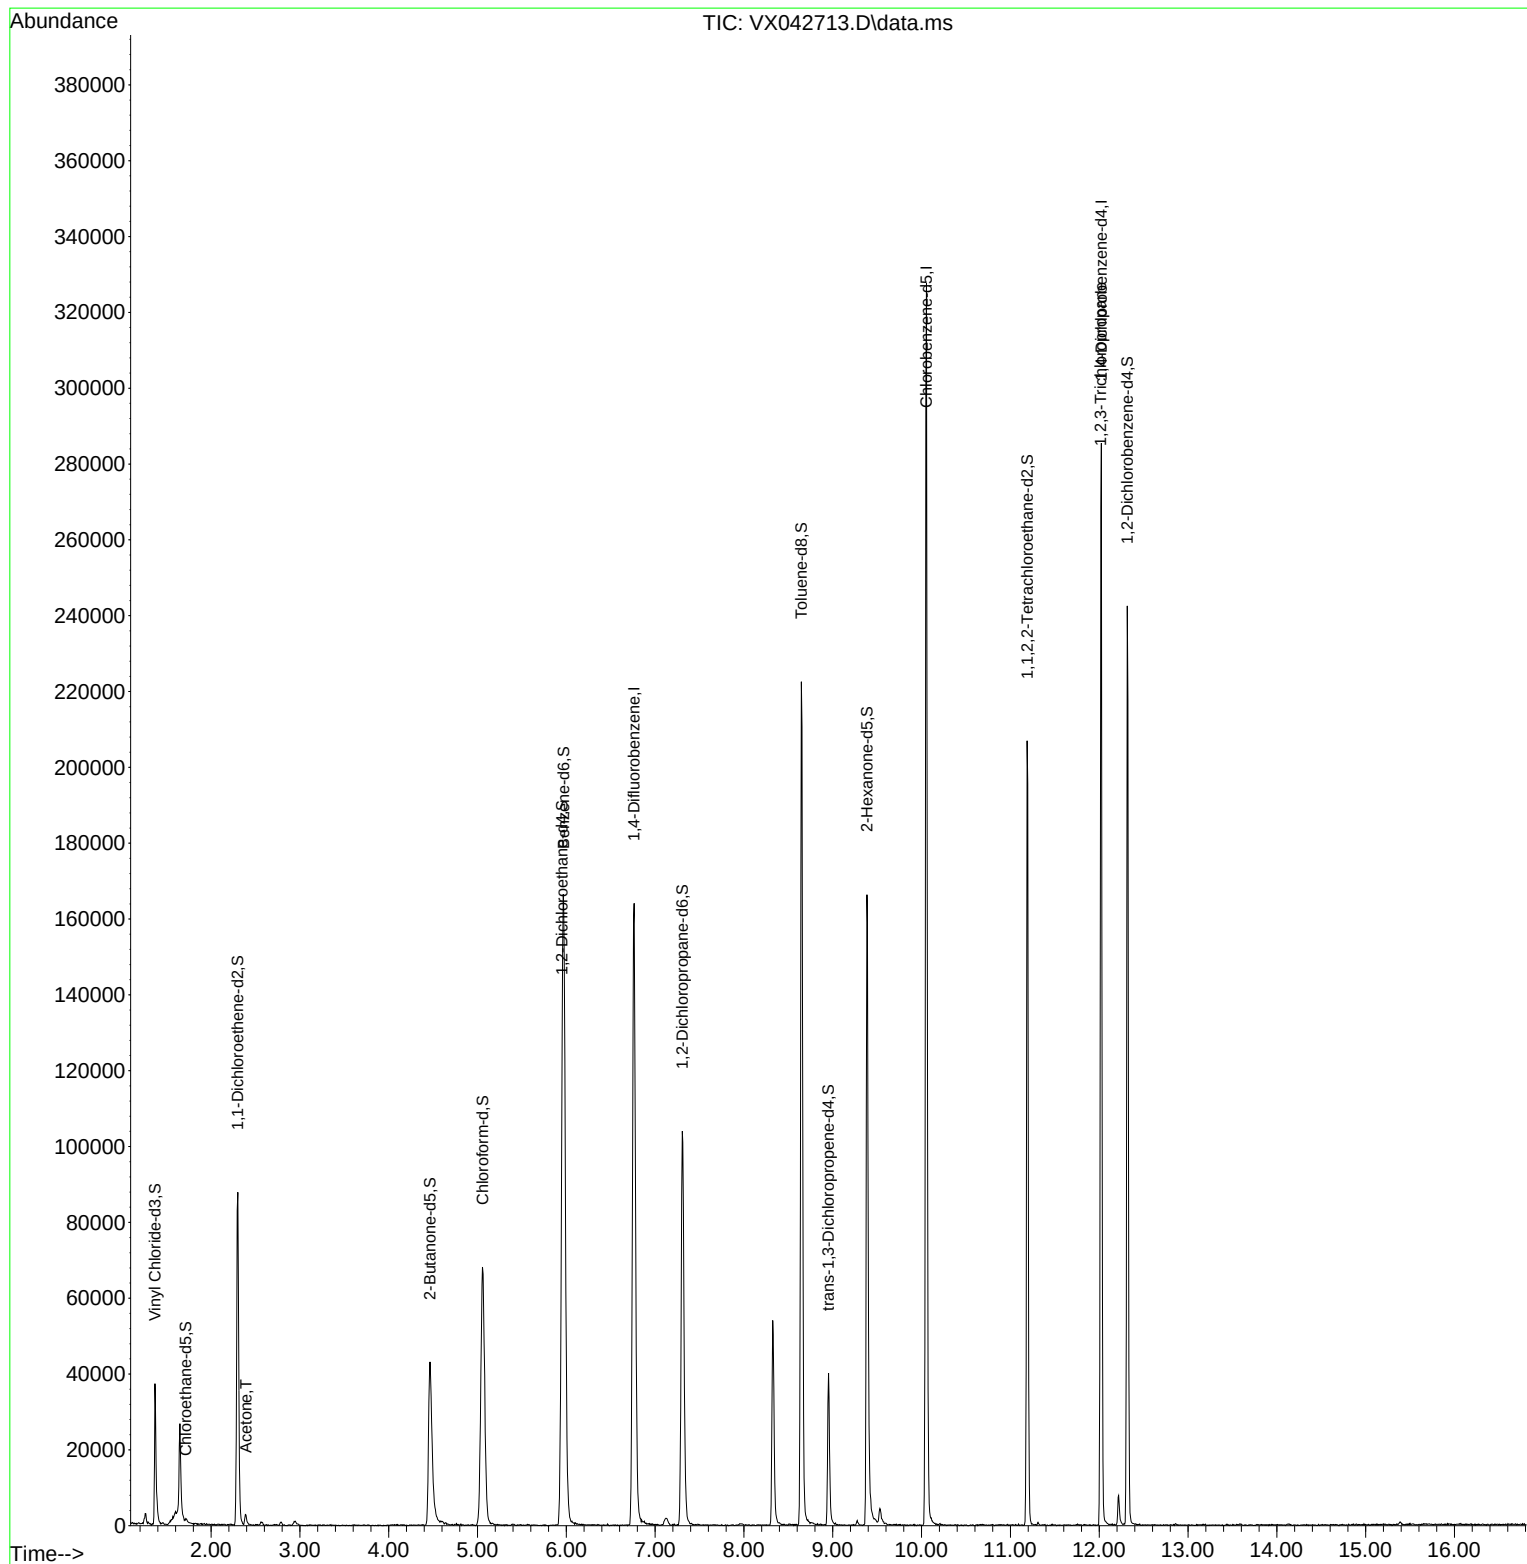

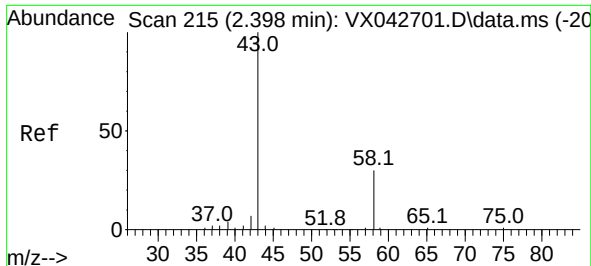

#13

Acetone

Concen: 4.871 ug/L

RT: 2.392 min Scan# 21

Delta R.T. -0.006 min

Lab File: VX042713.D

Acq: 29 Jul 2024 23:58

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 2882

Ion Ratio Lower Upper

43 100

58 32.0 0.0 62.4

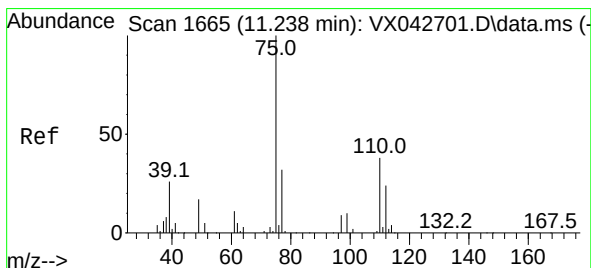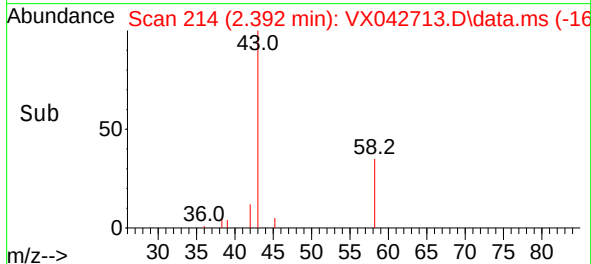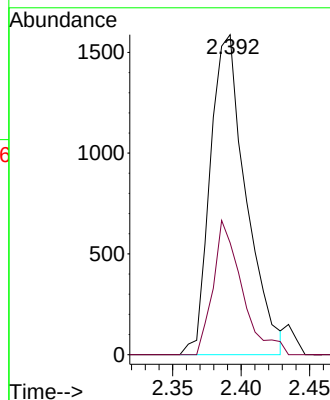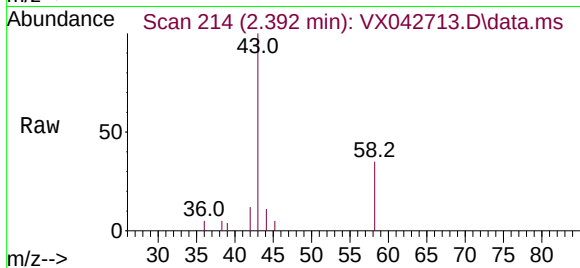

#61

1,2,3-Trichloropropane

Concen: 5.355 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.781 min

Lab File: VX042713.D

Acq: 29 Jul 2024 23:58

Tgt Ion: 75 Resp: 7263

Ion Ratio Lower Upper

75 100

77 35.1 26.2 39.4

110 3.7 33.0 49.4#

