

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042684.D
 Acq On : 29 Jul 2024 12:46
 Operator : JC/MD
 Sample : P3348-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08J4

Quant Time: Jul 29 13:13:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 29 03:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	167867	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	153221	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	58312	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	37996	37.256	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.520%
7) Chloroethane-d5	1.648	69	23495	55.907	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	111.820%
11) 1,1-Dichloroethene-d2	2.300	65	20419	40.636	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.280%
21) 2-Butanone-d5	4.465	46	81495	107.816	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.820%
24) Chloroform-d	5.056	84	104590	46.854	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.700%
26) 1,2-Dichloroethane-d4	5.958	65	73456	51.006	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.020%
32) Benzene-d6	5.970	84	202830	47.698	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	7.306	67	63703	50.617	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.240%
41) Toluene-d8	8.647	98	175005	45.900	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.800%
43) trans-1,3-Dichloroprop...	8.952	79	25690	43.619	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.240%
47) 2-Hexanone-d5	9.384	63	57540	102.258	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.260%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	91112	50.281	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.560%
66) 1,2-Dichlorobenzene-d4	12.323	152	56409	51.187	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.380%
Target Compounds						
13) Acetone	2.386	43	1836	3.107	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042684.D
Acq On : 29 Jul 2024 12:46
Operator : JC/MD
Sample : P3348-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08J4

Quant Time: Jul 29 13:13:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 29 03:03:42 2024
Response via : Initial Calibration

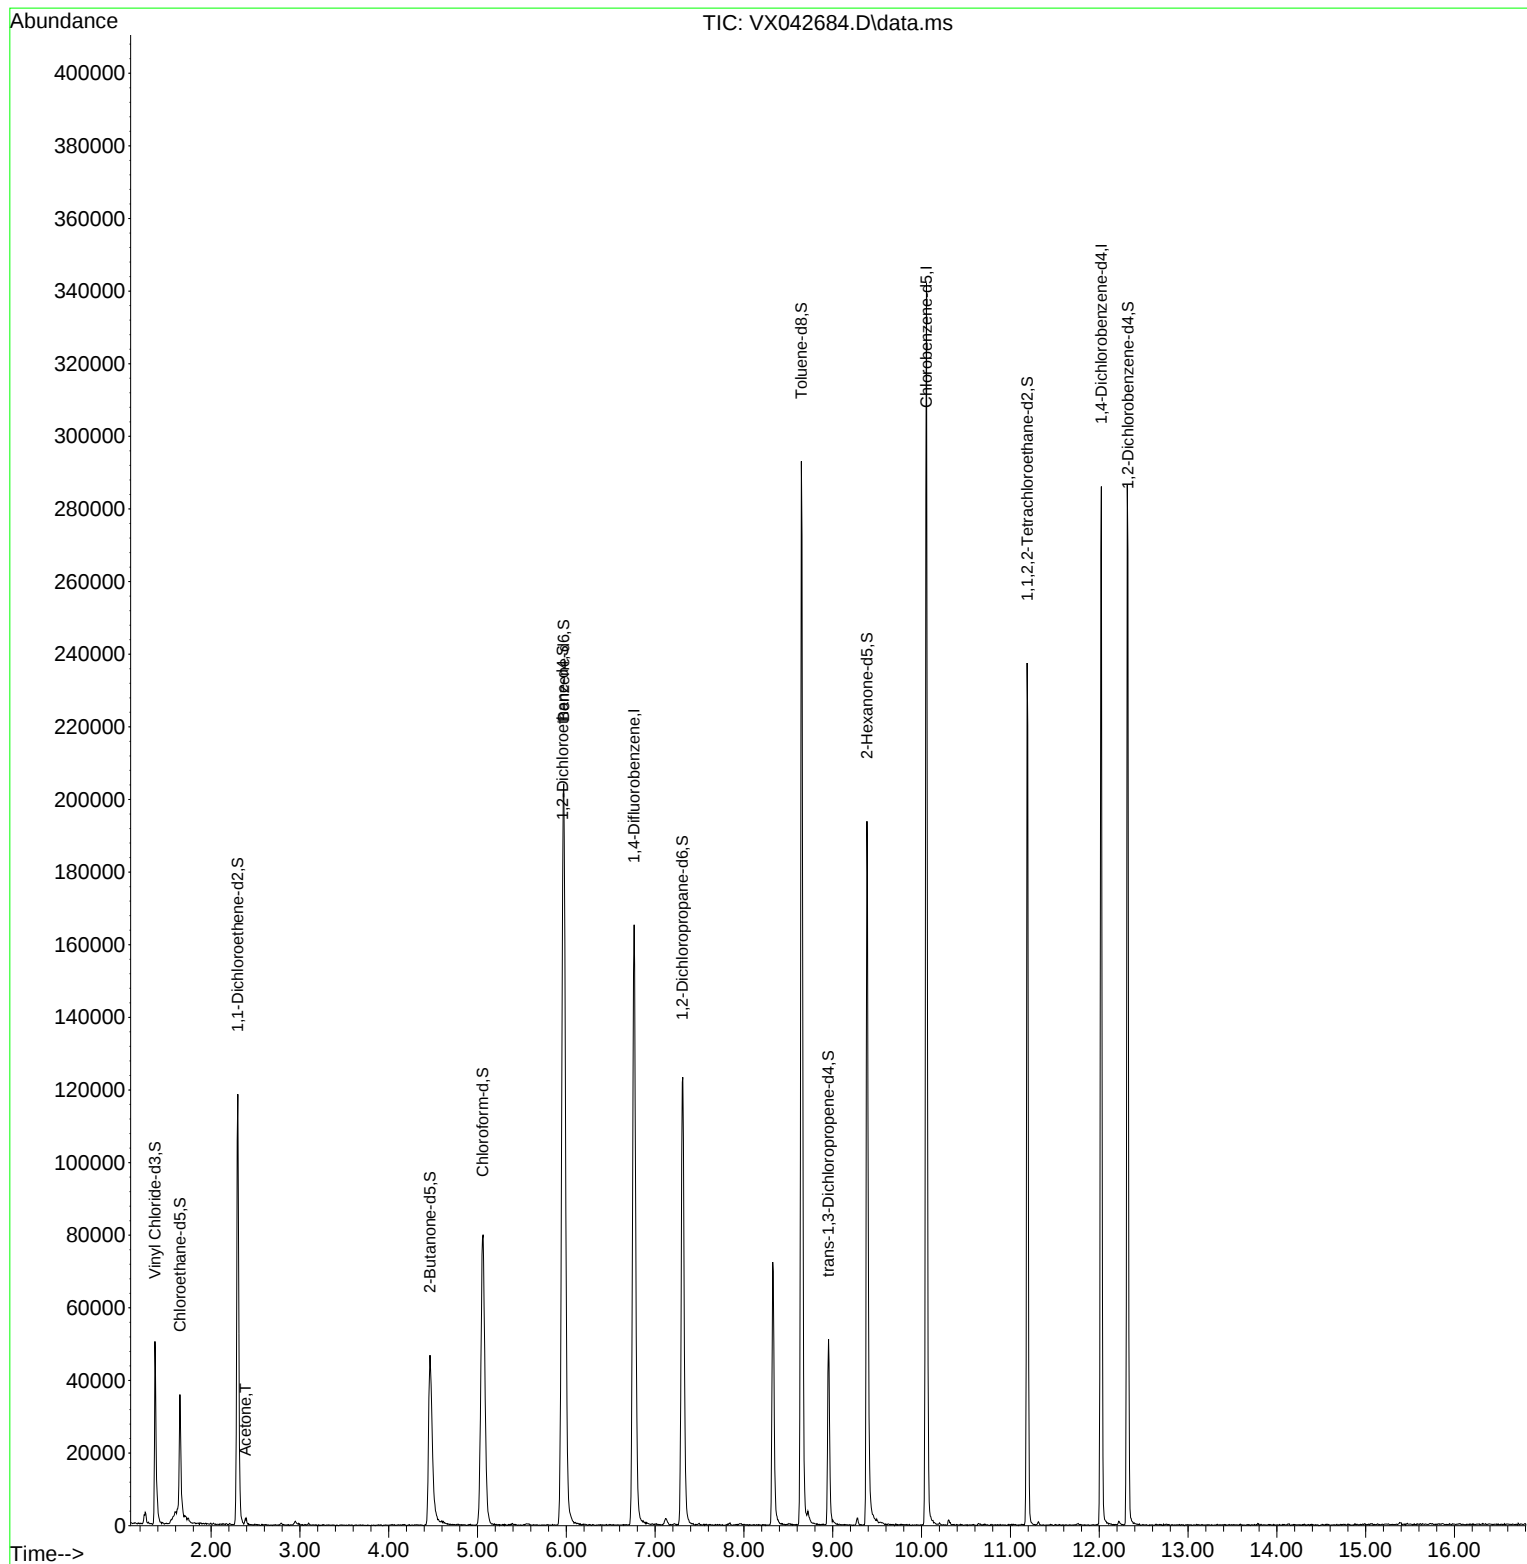

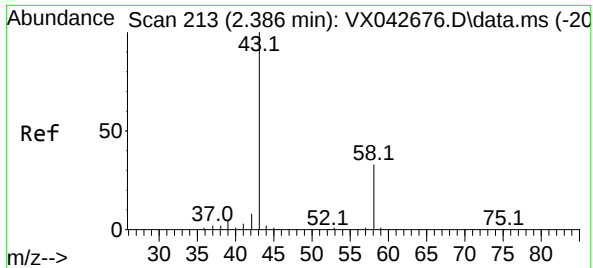

#13
 Acetone
 Concen: 3.107 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VX042684.D
 Acq: 29 Jul 2024 12:46

Instrument :
 MSVOA_X
 ClientSampleId :
 E08J4

Tgt Ion: 43 Resp: 1836
 Ion Ratio Lower Upper
 43 100
 58 31.5 0.0 62.4

