

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042688.D
 Acq On : 29 Jul 2024 14:17
 Operator : JC/MD
 Sample : P3335-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20KODL

Quant Time: Jul 30 01:09:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 30 00:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	158382	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	144601	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	54008	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	39463	41.012	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.020%
7) Chloroethane-d5	1.648	69	18620	46.960	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.920%
11) 1,1-Dichloroethene-d2	2.294	65	21929	46.254	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.500%
21) 2-Butanone-d5	4.464	46	85748	120.236	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.240%
24) Chloroform-d	5.056	84	107347	50.969	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.940%
26) 1,2-Dichloroethane-d4	5.958	65	74421	54.771	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.540%
32) Benzene-d6	5.976	84	207134	51.614	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.220%
36) 1,2-Dichloropropane-d6	7.311	67	66027	55.591	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.180%
41) Toluene-d8	8.646	98	176482	49.047	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.100%
43) trans-1,3-Dichloroprop...	8.951	79	25501	45.880	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.760%
47) 2-Hexanone-d5	9.384	63	58286	109.759	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.760%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	92626	54.163	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	108.320%
66) 1,2-Dichlorobenzene-d4	12.323	152	55727	54.598	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.200%
Target Compounds						
					Qvalue	
34) Trichloroethene	7.122	95	156121	132.051	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042688.D
Acq On : 29 Jul 2024 14:17
Operator : JC/MD
Sample : P3335-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20KODL

Quant Time: Jul 30 01:09:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 30 00:49:01 2024
Response via : Initial Calibration

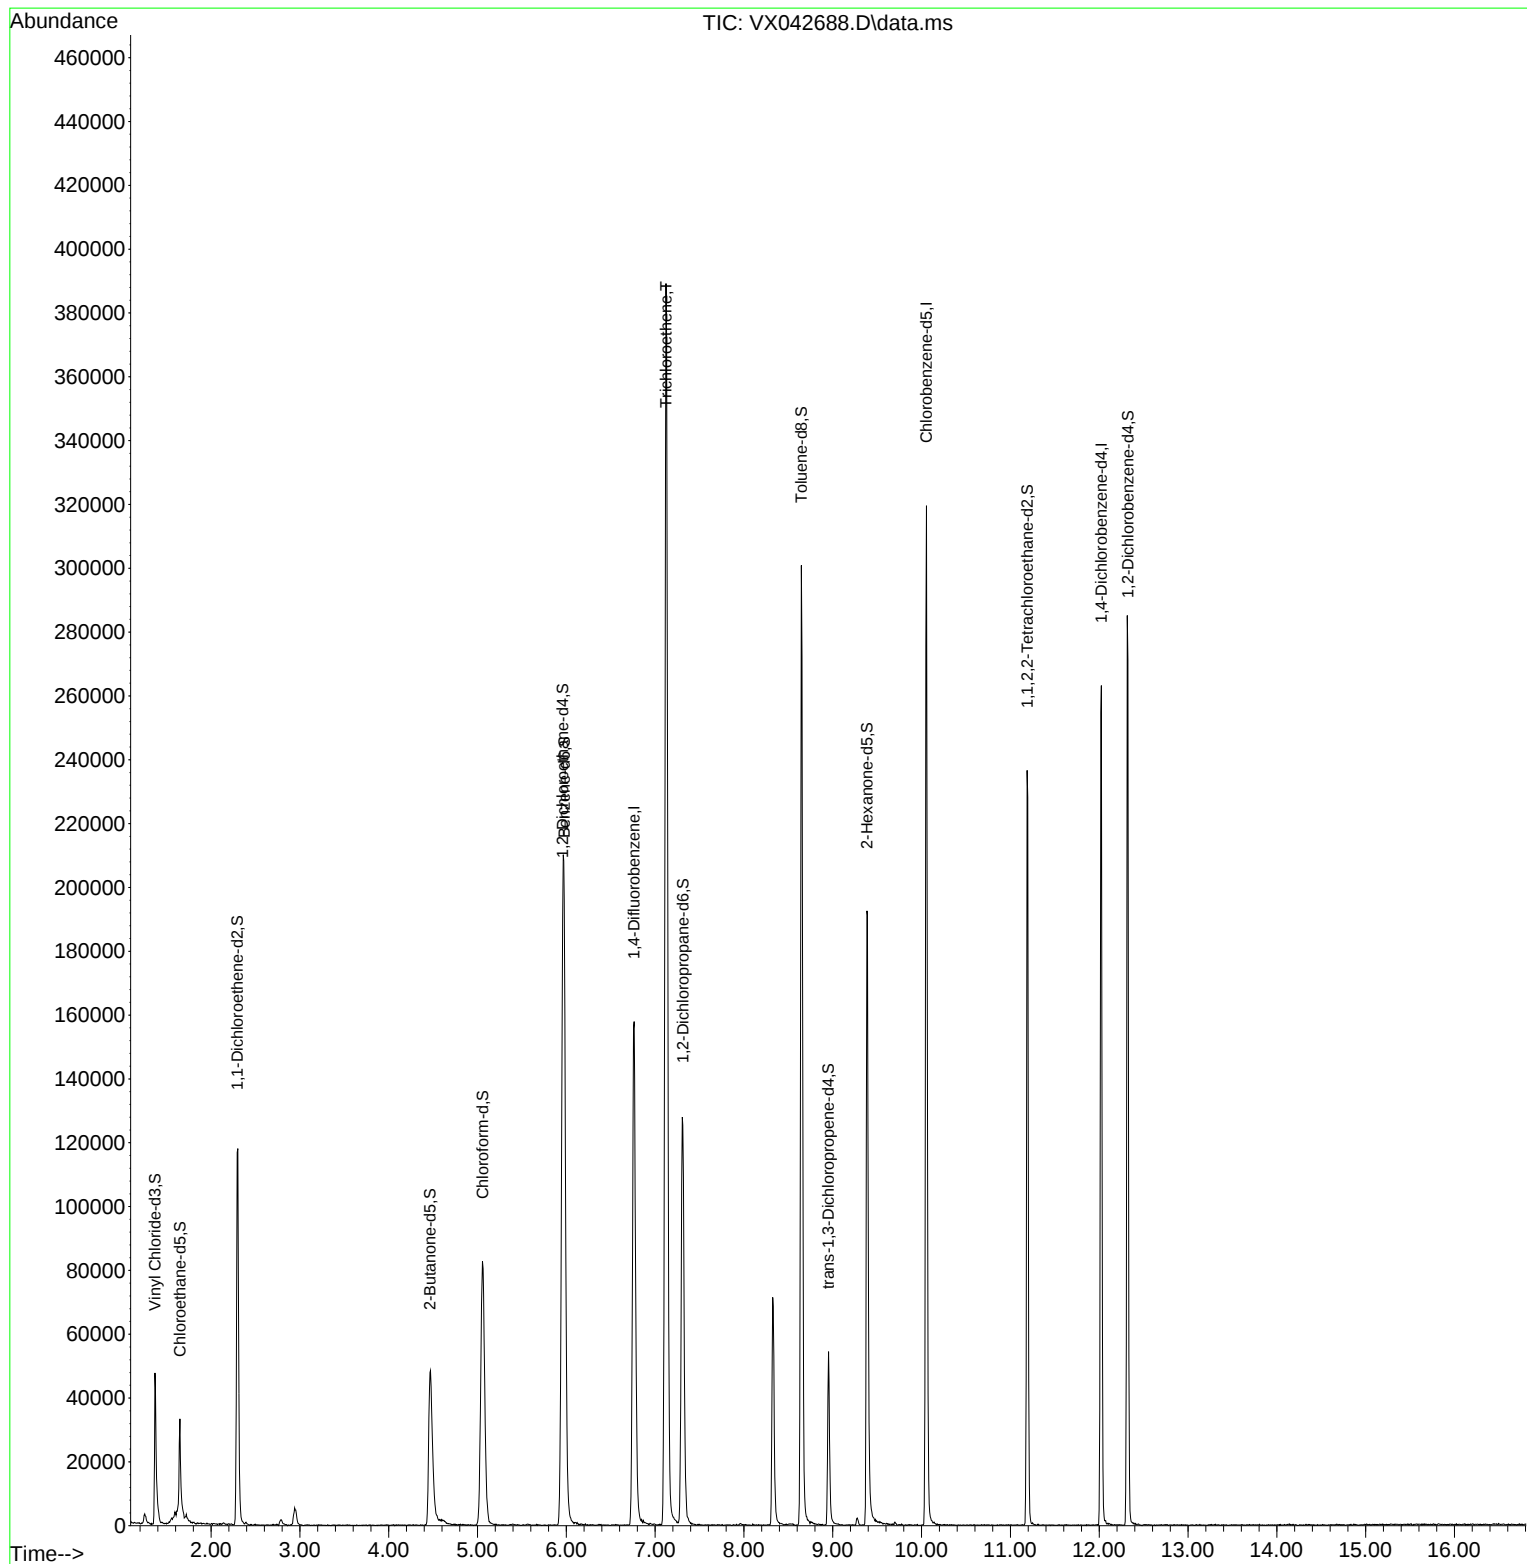

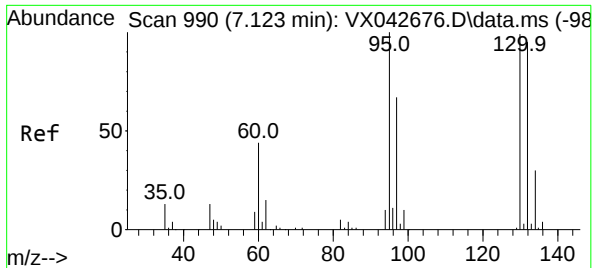

#34
 Trichloroethene
 Concen: 132.051 ug/L
 RT: 7.122 min Scan# 99
 Delta R.T. -0.000 min
 Lab File: VX042688.D
 Acq: 29 Jul 2024 14:17

Instrument :
 MSVOA_X
 ClientSampleId :
 E20KODL

Tgt Ion: 95 Resp: 156121

Ion	Ratio	Lower	Upper
95	100		
97	65.0	46.3	86.1
132	91.4	64.3	119.5
130	94.4	67.0	124.4

